

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014437.D
 Acq On : 31 Mar 2023 11:27
 Operator : CG/JU
 Sample : 02131-01DL 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG6DL

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/03/2023
 Supervised By : Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:52:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	161320	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	736651	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.669	164	477063	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.428	188	993442	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	687608	20.000	ng/u1	0.00
88) Perylene-d12	24.033	264	725138	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	5050	1.214	ng/uL	0.00
4) Pyridine-d5	3.869	84	11150m	1.046	ng/u1	0.05
7) Phenol-d5	7.181	99	21075	1.417	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	80637	8.448	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	66484	6.183	ng/u1	0.00
15) 4-Methylphenol-d8	8.734	113	44123	3.677	ng/u1	0.00
21) Nitrobenzene-d5	9.193	128	43040	7.237	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	47146	6.923	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	78590	6.337	ng/u1	0.01
31) 4-Chloroaniline-d4	10.993	131	39152	2.397	ng/u1	0.01
46) Dimethylphthalate-d6	14.069	166	329207	8.511	ng/u1	0.00
49) Acenaphthylene-d8	14.357	160	344705	8.031	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.663	176	274892	8.522	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	40479	5.538	ng/u1	0.00
73) Anthracene-d10	17.528	188	410992	8.548	ng/u1	0.00
81) Pyrene-d10	19.757	212	440767	9.543	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.868	264	313637	8.141	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.887	128	2086914	50.860	ng/u1	99
36) 2-Methylnaphthalene	12.492	142	216859	7.798	ng/u1	99
37) 1-Methylnaphthalene	12.710	142	182308	6.610	ng/u1	95
43) 1,1'-Biphenyl	13.498	154	61010	1.583	ng/u1	96
58) 2,3,4,6-Tetrachlorophenol	15.298	232	145204	14.418	ng/u1	98
71) Pentachlorophenol	17.080	266	2484754	302.053	ng/u1	99
72) Phenanthrene	17.469	178	88402	1.599	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014437.D
Acq On : 31 Mar 2023 11:27
Operator : CG/JU
Sample : 02131-01DL 5X
Misc :
ALS Vial : 46 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0QG6DL

Quant Time: Mar 31 22:52:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

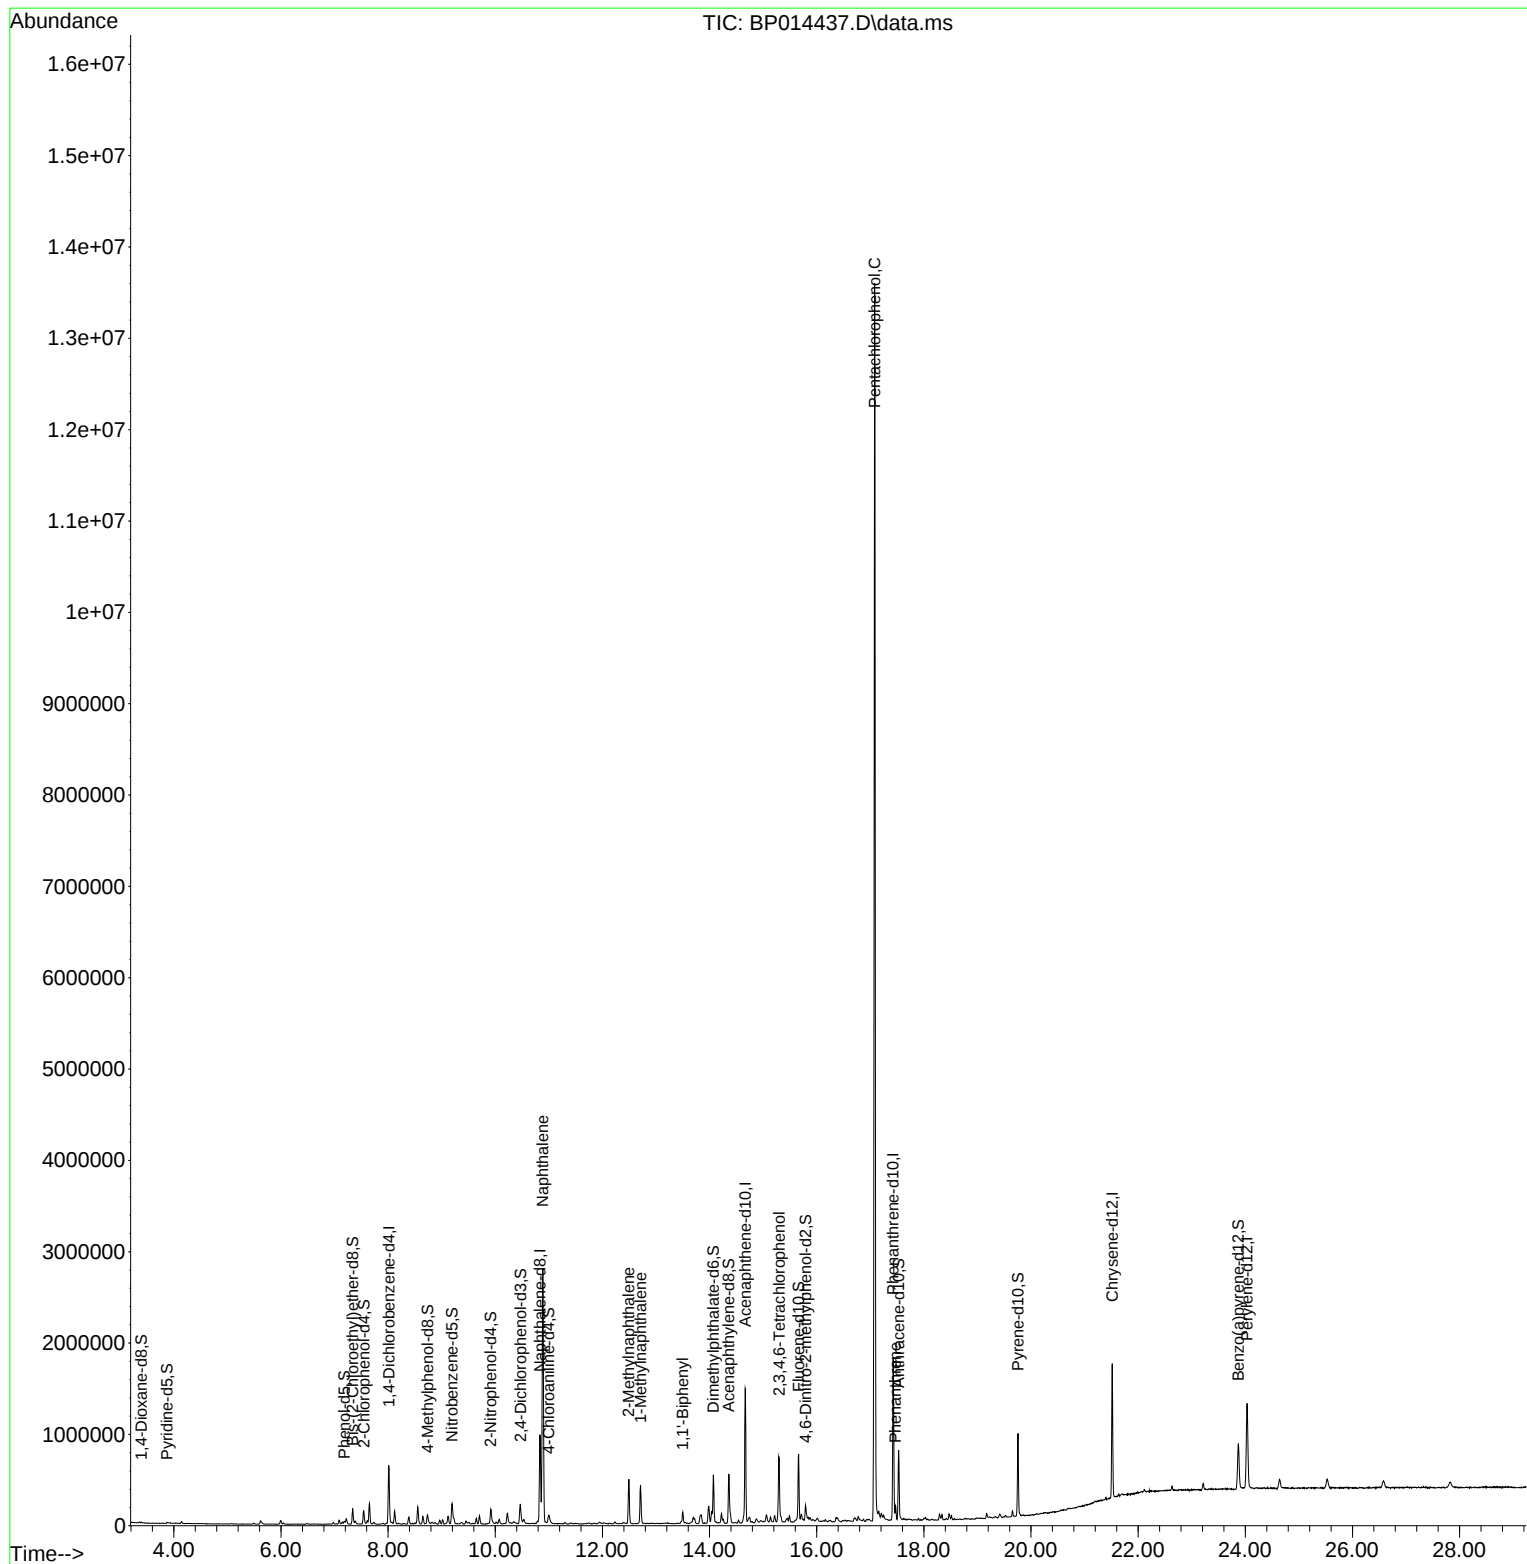

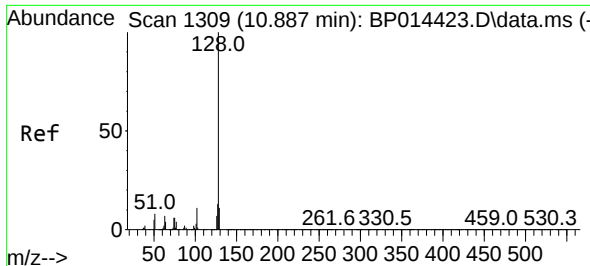

#30
Naphthalene
Concen: 50.860 ng/ul
RT: 10.887 min Scan# 1309
Delta R.T. -0.000 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27




Instrument :
BNA_P
ClientSampleId :
C0QG6DL

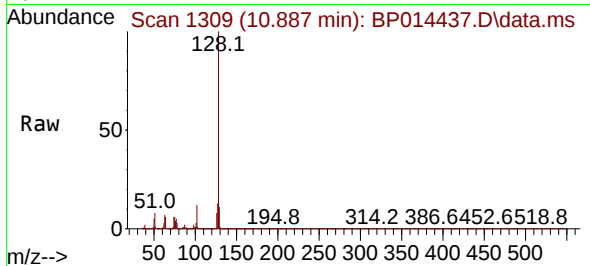


Tgt Ion:128 Resp: 2086914
Ion Ratio Lower Upper
128 100
129 11.2 8.9 13.3
127 13.4 11.0 16.6

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

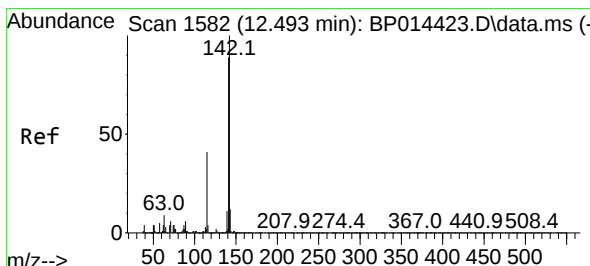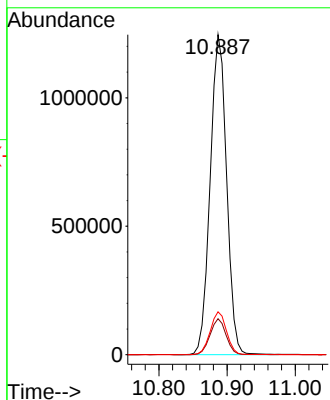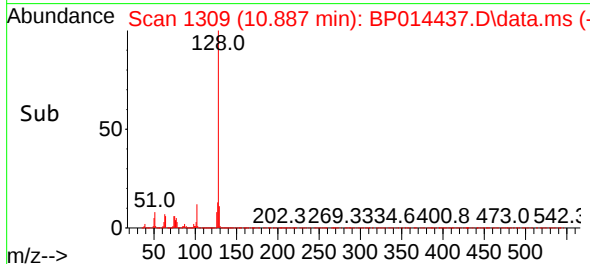


#36
2-Methylnaphthalene
Concen: 7.798 ng/ul
RT: 12.492 min Scan# 1582
Delta R.T. -0.000 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27

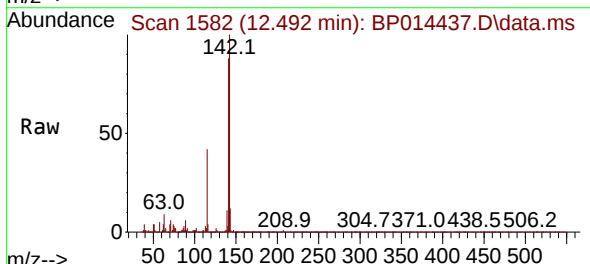


Tgt Ion:142 Resp: 216859
Ion Ratio Lower Upper
142 100
141 88.5 71.6 107.4

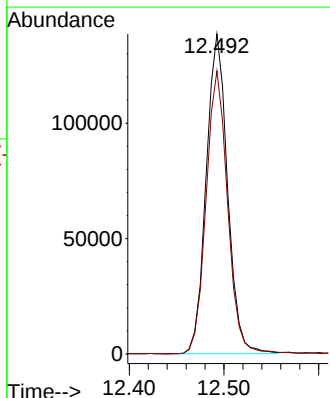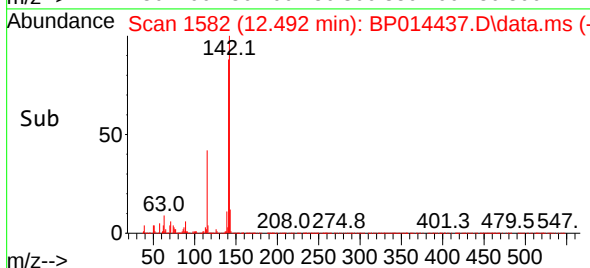

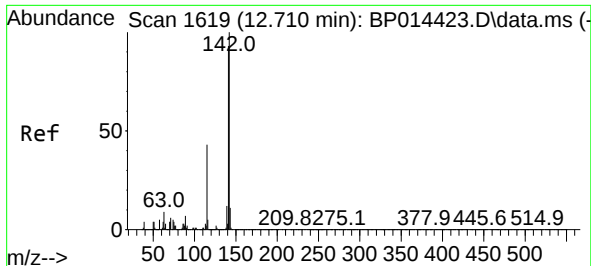

#37
1-Methylnaphthalene
Concen: 6.610 ng/ul
RT: 12.710 min Scan# 1619
Delta R.T. -0.000 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27




Instrument :
BNA_P
ClientSampleId :
C0QG6DL

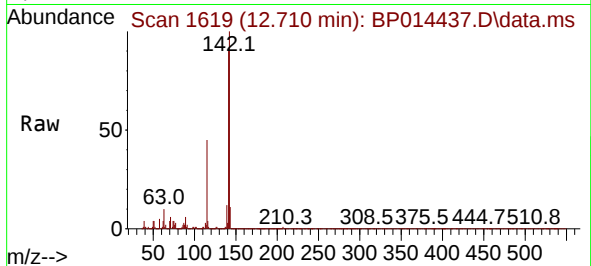


Tgt Ion:142 Resp: 182308
Ion Ratio Lower Upper
142 100
141 90.5 76.6 114.8
116 4.3 3.6 5.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

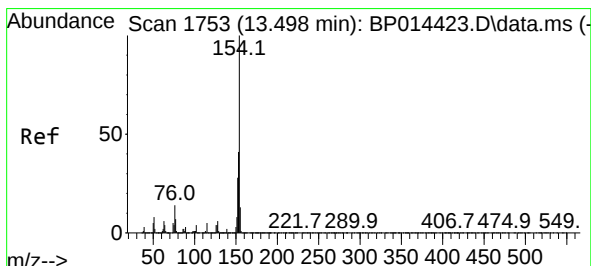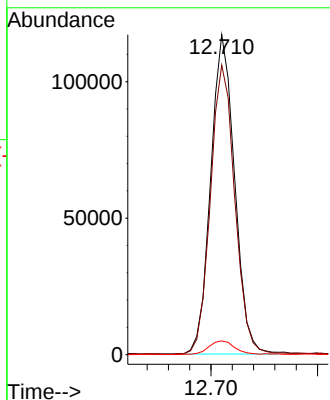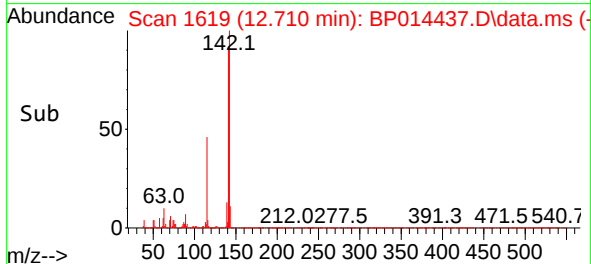


#43
1,1'-Biphenyl
Concen: 1.583 ng/ul
RT: 13.498 min Scan# 1753
Delta R.T. -0.000 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27

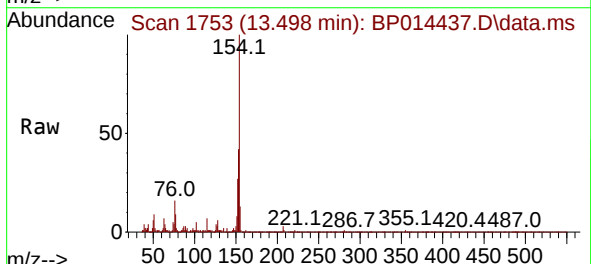


Tgt Ion:154 Resp: 61010
Ion Ratio Lower Upper
154 100
153 42.5 32.4 48.6
76 15.7 10.7 16.1

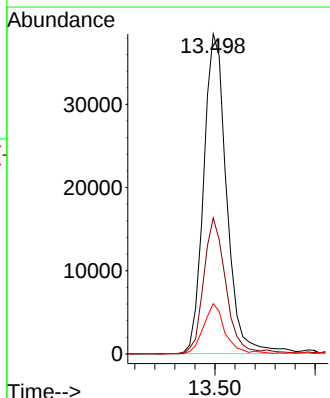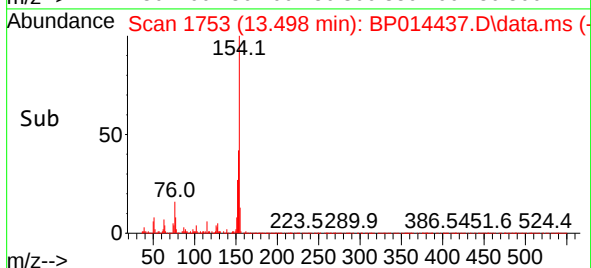

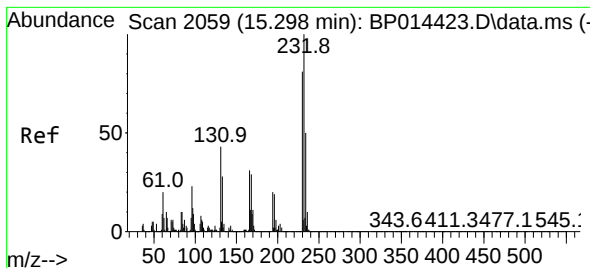

#58
2,3,4,6-Tetrachlorophenol
Concen: 14.418 ng/ul
RT: 15.298 min Scan# 2059
Delta R.T. -0.000 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27




Instrument :
BNA_P
ClientSampleId :
C0QG6DL

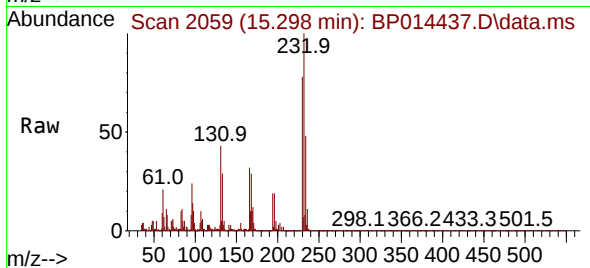


Tgt Ion:232 Resp: 145204
Ion Ratio Lower Upper
232 100
131 42.9 35.0 52.4
130 2.5 1.9 2.9
166 31.8 24.1 36.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

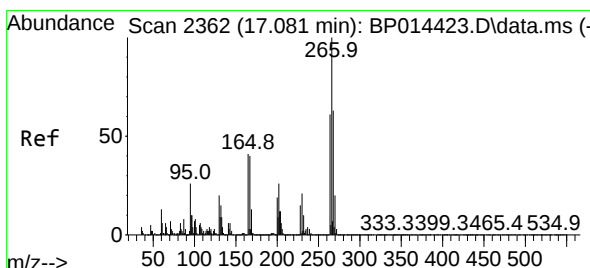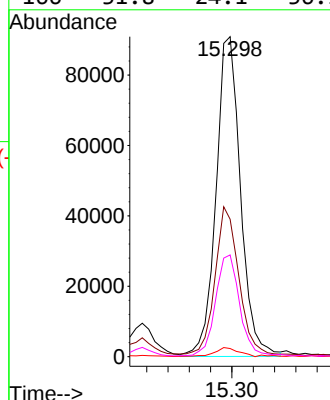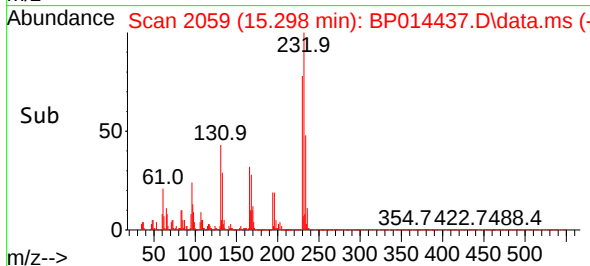


#71
Pentachlorophenol
Concen: 302.053 ng/ul
RT: 17.080 min Scan# 2362
Delta R.T. -0.000 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27

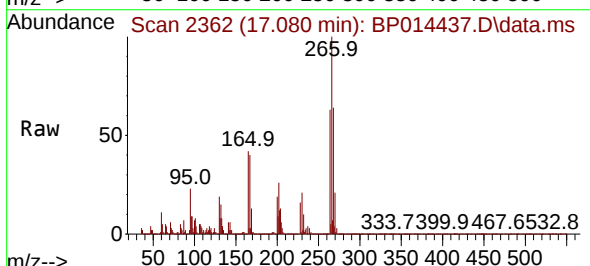


Tgt Ion:266 Resp: 2484754
Ion Ratio Lower Upper
266 100
264 63.2 51.0 76.4
268 64.0 51.4 77.2

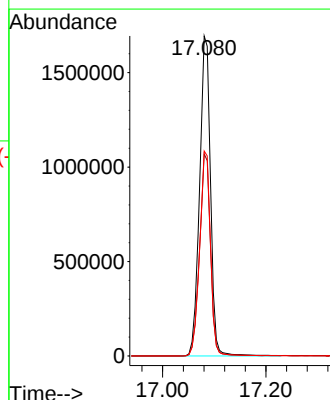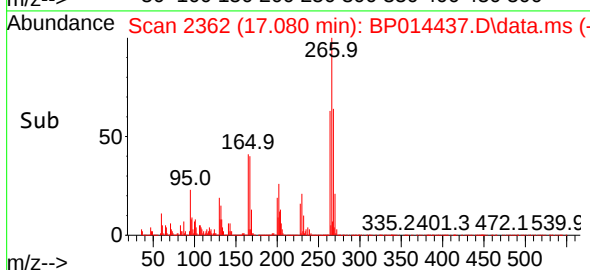

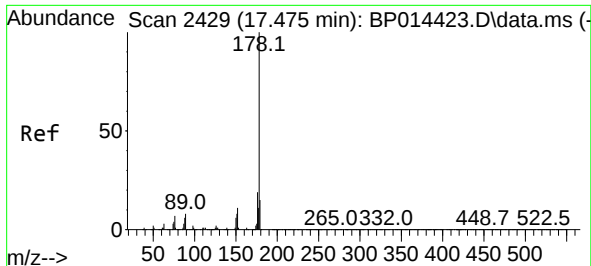

#72
Phenanthrene
Concen: 1.599 ng/ul
RT: 17.469 min Scan# 2428
Delta R.T. -0.006 min
Lab File: BP014437.D
Acq: 31 Mar 2023 11:27

Instrument :
BNA_P
ClientSampleId :
C0QG6DL

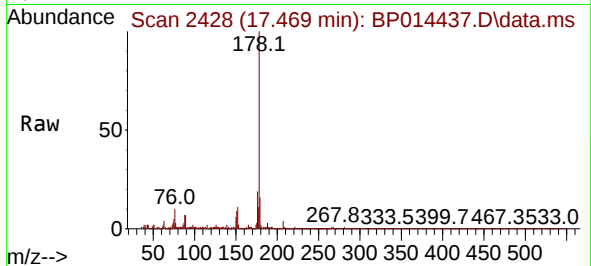

Tgt Ion:178 Resp: 8840
Ion Ratio Lower Upper
178 100
179 16.3 12.2 18.4
176 19.2 15.3 22.9

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

