

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014464.D
 Acq On : 01 Apr 2023 03:14
 Operator : CG/JU
 Sample : 02093-08
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB978

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/03/2023
 Supervised By : Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 03:55:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	157351	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	719514	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.669	164	480464	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.428	188	1005312	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	684186	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	702034	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	17129	4.221	ng/uL	0.00
4) Pyridine-d5	3.828	84	77994	7.501	ng/u1	0.01
7) Phenol-d5	7.187	99	108736	7.493	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	199688	21.447	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	186406	17.772	ng/u1	0.00
15) 4-Methylphenol-d8	8.740	113	166007	14.182	ng/u1	0.01
21) Nitrobenzene-d5	9.193	128	119379	20.552	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	127353	19.147	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	231855	19.141	ng/u1	0.01
31) 4-Chloroaniline-d4	10.987	131	91097	5.709	ng/u1	0.00
46) Dimethylphthalate-d6	14.075	166	883859	22.688	ng/u1	0.00
49) Acenaphthylene-d8	14.363	160	932954	21.583	ng/u1	0.00
54) 4-Nitrophenol-d4	14.922	143	30748m	5.225	ng/u1	0.04
60) Fluorene-d10	15.663	176	721028	22.194	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	90706	12.262	ng/u1	0.00
73) Anthracene-d10	17.528	188	1116932	22.957	ng/u1	0.00
81) Pyrene-d10	19.757	212	1168829	25.433	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.869	264	866774	23.239	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.423	88	401494	90.040	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014464.D
Acq On : 01 Apr 2023 03:14
Operator : CG/JU
Sample : 02093-08
Misc :
ALS Vial : 74 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
CB978

Quant Time: Apr 01 03:55:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

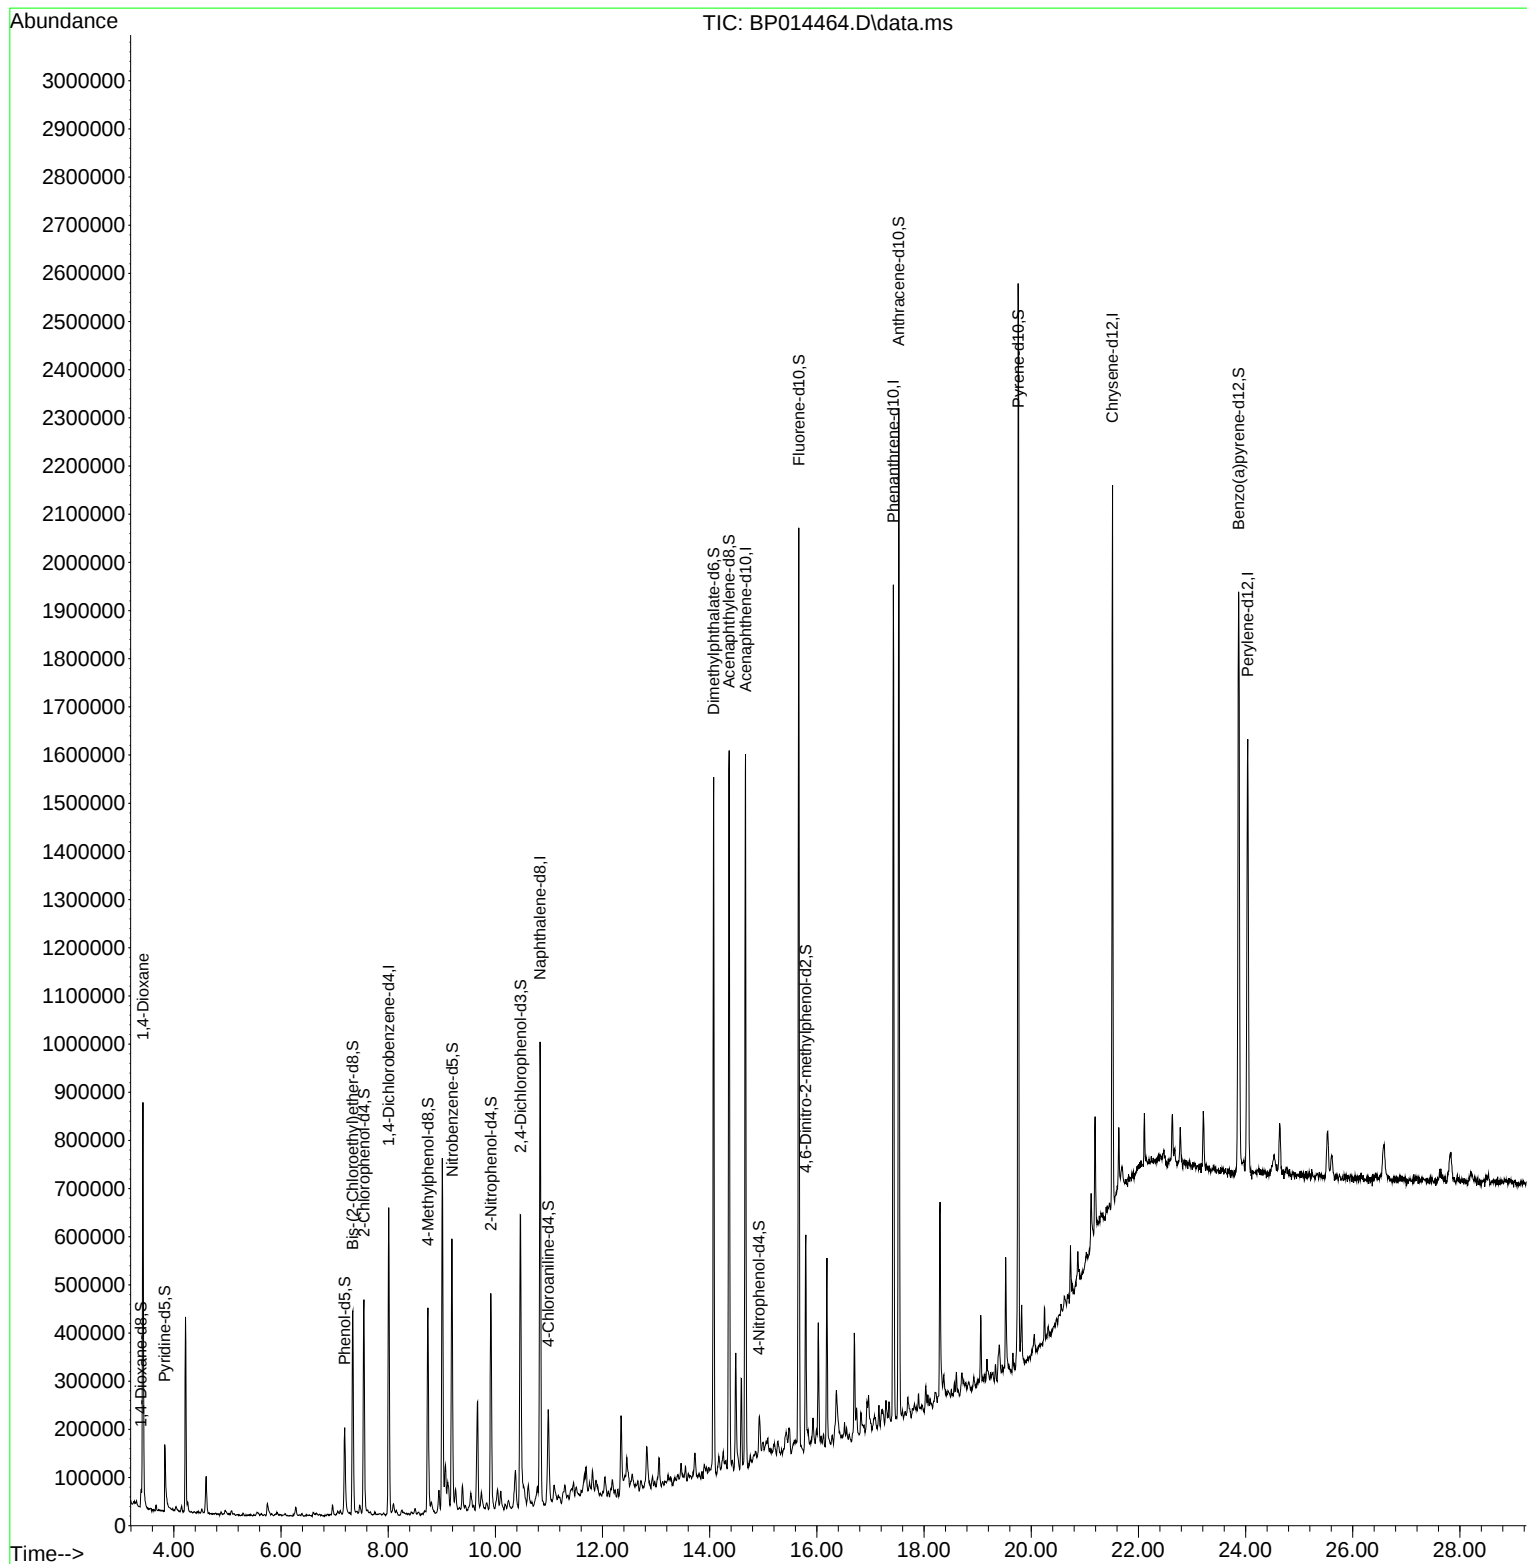

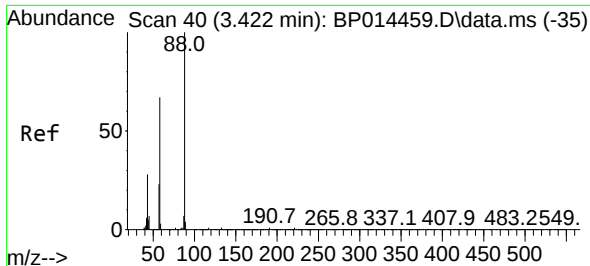

#2
 1,4-Dioxane
 Concen: 90.040 ng/uL
 RT: 3.423 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BP014464.D
 Acq: 01 Apr 2023 03:14

Instrument :
 BNA_P
 ClientSampleId :
 CB978

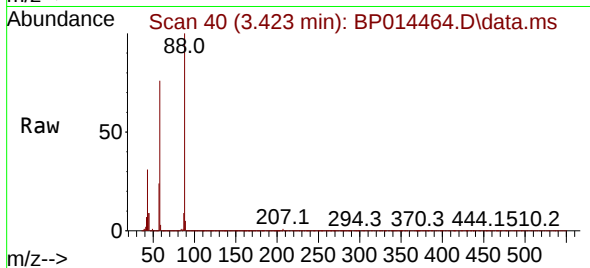

Tgt Ion: 88 Resp: 401494
 Ion Ratio Lower Upper
 88 100
 43 30.5 24.4 36.6
 58 76.1 57.4 86.0

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

