

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014469.D
 Acq On : 01 Apr 2023 06:03
 Operator : CG/JU
 Sample : 02093-07
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB977

Quant Time: Apr 03 00:41:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	197202	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	857936	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.663	164	543778	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.428	188	1026239	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	728604	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	881237	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	11656	2.292	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.181	99	17	0.001	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.317	67	204	0.017	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.534	132	14	0.001	ng/u1	0.00
15) 4-Methylphenol-d8	8.734	113	65	0.004	ng/u1	0.00
21) Nitrobenzene-d5	9.193	128	8	0.001	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	56	0.007	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/u1	
31) 4-Chloroaniline-d4	10.981	131	87	0.005	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	394	0.009	ng/u1	-0.02
49) Acenaphthylene-d8	14.357	160	204	0.004	ng/u1	0.00
54) 4-Nitrophenol-d4	14.869	143	266	0.040	ng/u1	-0.01
60) Fluorene-d10	15.645	176	1400	0.038	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.810	200	56	0.007	ng/u1	0.02
73) Anthracene-d10	0.000	188	0d	0.000	ng/u1	
81) Pyrene-d10	19.763	212	2856	0.058	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	1945	0.042	ng/u1	0.01


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.423	88	25759	4.609	ng/uL#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014469.D
Acq On : 01 Apr 2023 06:03
Operator : CG/JU
Sample : 02093-07
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB977

Quant Time: Apr 03 00:41:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

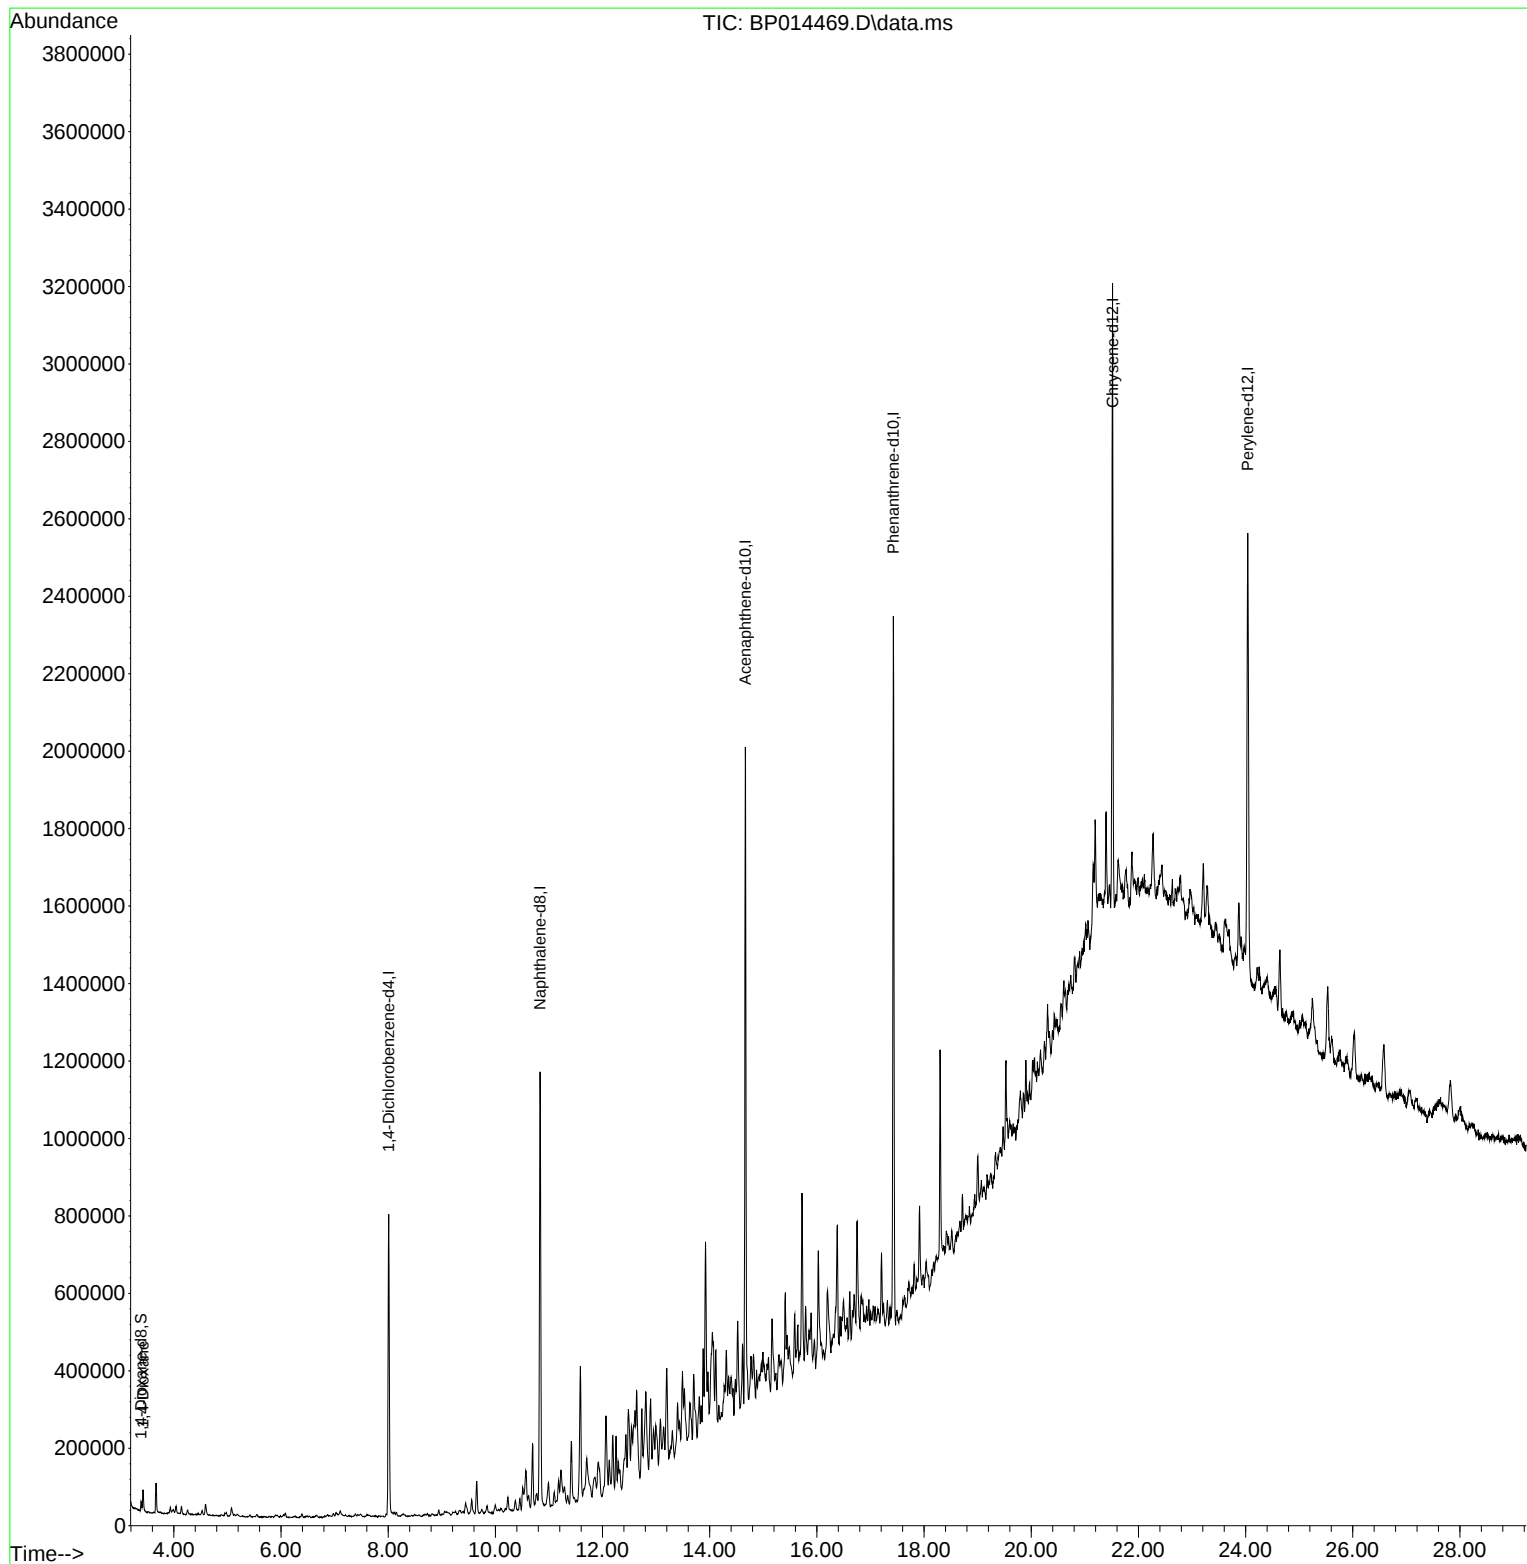

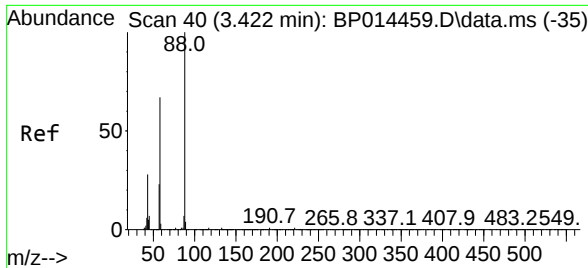

#2
 1,4-Dioxane
 Concen: 4.609 ng/uL
 RT: 3.423 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BP014469.D
 Acq: 01 Apr 2023 06:03

Instrument :
 BNA_P
 ClientSampleId :
 CB977

Tgt Ion:	88	Resp:	25759
Ion	Ratio	Lower	Upper
88	100		
43	37.6	24.4	36.6#
58	80.8	57.4	86.0

