

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014394.D
 Acq On : 30 Mar 2023 10:38
 Operator : CG/JU
 Sample : PB151777BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK777

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	31	34	43	rVB	29813	44937	1.18%	0.131%
2	3.828	107	109	126	rBV	152229	292864	7.68%	0.855%
3	4.146	160	163	171	rVB4	7346	10884	0.29%	0.032%
4	5.287	352	357	360	rBV5	3404	5932	0.16%	0.017%
5	7.175	672	678	694	rBV	477739	847099	22.21%	2.473%
6	7.340	700	706	719	rBV	404286	651754	17.09%	1.903%
7	7.546	734	741	751	rBV	504499	840625	22.04%	2.454%
8	8.016	814	821	832	rBV	391909	648216	16.99%	1.893%
9	8.734	936	943	958	rBV	594850	1077178	28.24%	3.145%
10	9.193	1013	1021	1036	rBV	512782	878103	23.02%	2.564%
11	9.922	1137	1145	1159	rBV	426817	772435	20.25%	2.255%
12	10.469	1230	1238	1266	rBV	433048	1086182	28.47%	3.171%
13	10.840	1294	1301	1317	rBV	566249	945937	24.80%	2.762%
14	11.022	1325	1332	1347	rBV3	15908	57344	1.50%	0.167%
15	12.451	1567	1575	1585	rBV6	7774	18299	0.48%	0.053%
16	14.075	1843	1851	1866	rBV	1264791	1810270	47.46%	5.285%
17	14.363	1894	1900	1915	rBV	1333873	1988349	52.13%	5.805%
18	14.669	1945	1952	1963	rBV	919080	1373440	36.01%	4.010%
19	14.893	1983	1990	2015	rBV	244303	798139	20.92%	2.330%
20	15.669	2115	2122	2136	rBV	1725687	2625293	68.82%	7.665%
21	15.792	2136	2143	2158	rBV	594710	930623	24.40%	2.717%
22	15.904	2160	2162	2171	rVB7	11215	20926	0.55%	0.061%
23	17.110	2364	2367	2372	rVB7	3389	4229	0.11%	0.012%
24	17.222	2382	2386	2390	rBV7	4488	7367	0.19%	0.022%
25	17.434	2415	2422	2432	rBV	1296563	1789345	46.91%	5.224%
26	17.534	2432	2439	2454	rVV	2087145	3021207	79.20%	8.821%
27	19.339	2743	2746	2751	rVB2	26592	34748	0.91%	0.101%
28	19.410	2755	2758	2765	rVB	20490	34314	0.90%	0.100%
29	19.763	2812	2818	2827	rBV	2746381	3709932	97.26%	10.831%
30	21.522	3112	3117	3125	rBV	1489216	2041541	53.52%	5.960%
31	23.880	3510	3518	3529	rBV2	1854518	3814537	100.00%	11.137%
32	24.045	3539	3546	3557	rVB	990308	2069352	54.25%	6.042%




Sum of corrected areas: 34251401

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014394.D
Acq On : 30 Mar 2023 10:38
Operator : CG/JU
Sample : PB151777BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK777

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

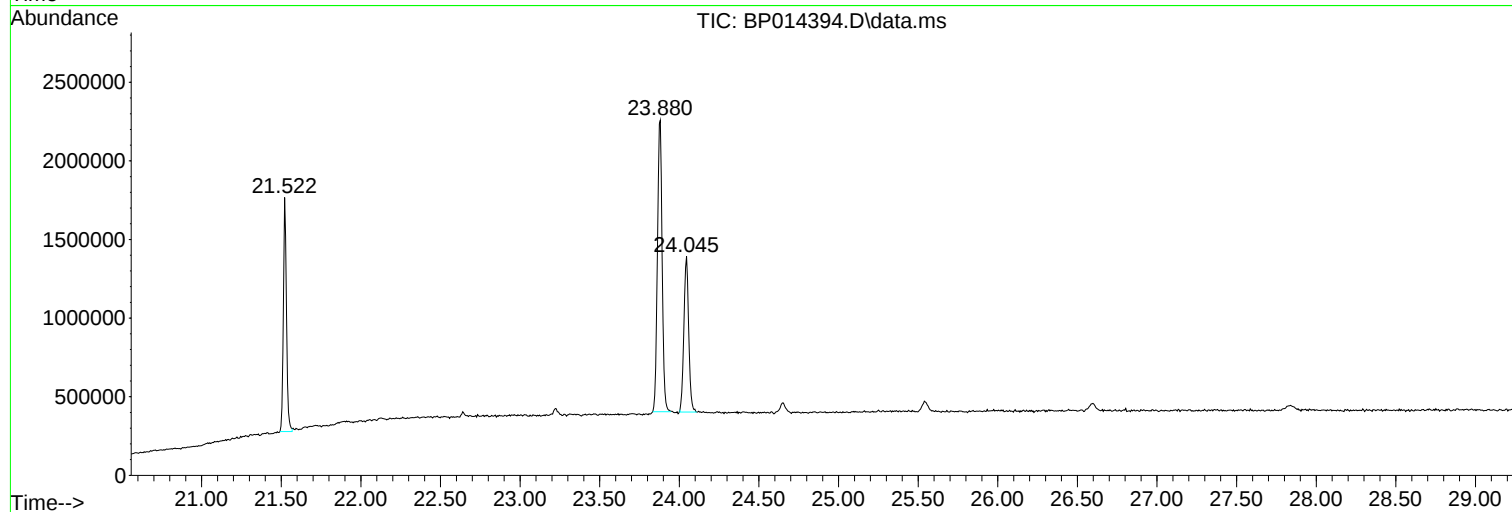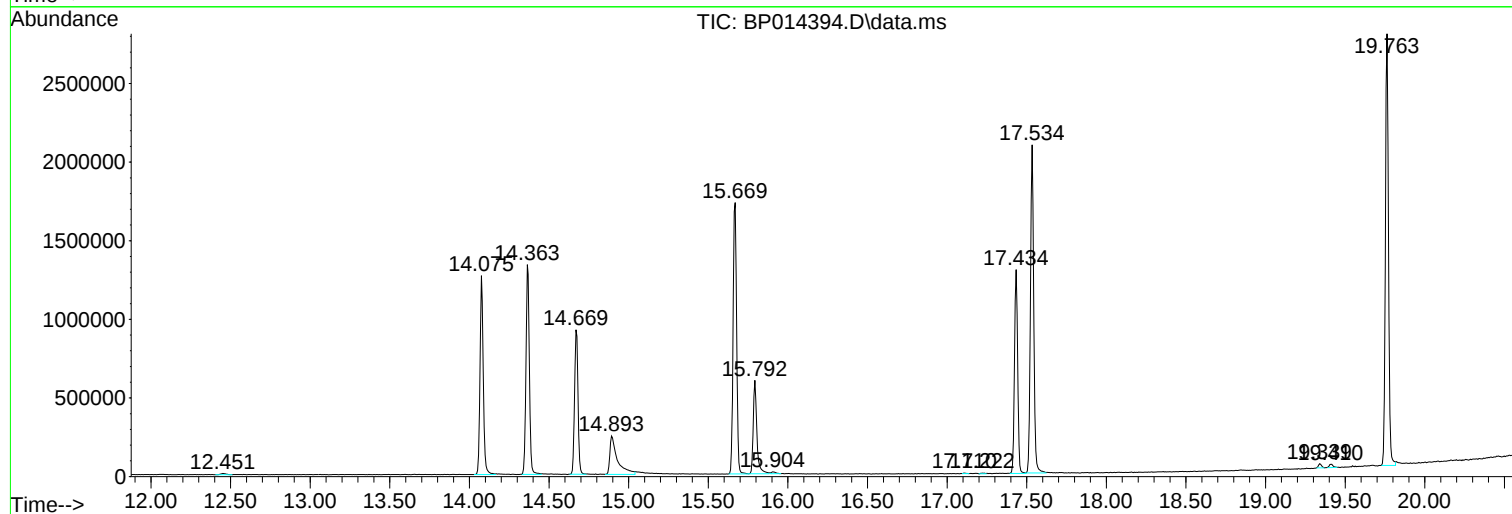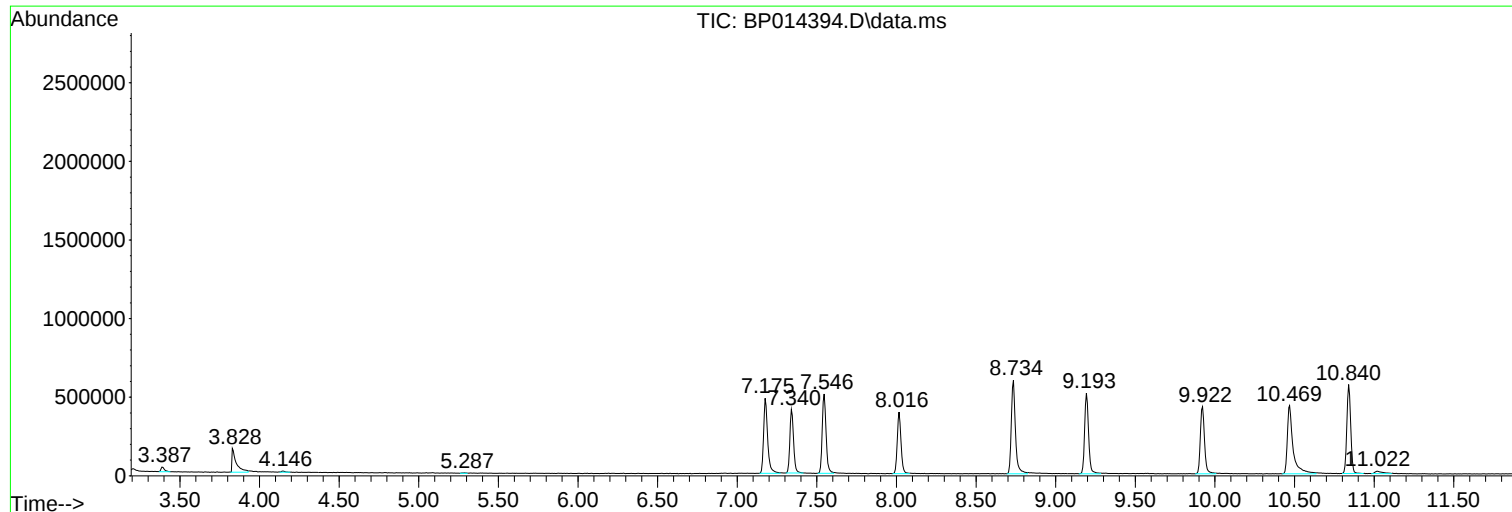

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014394.D
Acq On : 30 Mar 2023 10:38
Operator : CG/JU
Sample : PB151777BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK777

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014394.D
Acq On : 30 Mar 2023 10:38
Operator : CG/JU
Sample : PB151777BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK777

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc