

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014395.D
 Acq On : 30 Mar 2023 11:12
 Operator : CG/JU
 Sample : PB151778BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	31	34	42	rVB	26078	39207	1.02%	0.119%
2	3.546	56	61	62	rBV5	3088	5097	0.13%	0.015%
3	3.828	107	109	127	rBV	139583	282602	7.35%	0.855%
4	4.146	160	163	171	rVB3	7086	10321	0.27%	0.031%
5	7.175	672	678	696	rBV	453820	815516	21.22%	2.468%
6	7.340	700	706	719	rBV	391072	628096	16.34%	1.901%
7	7.546	734	741	754	rBV	476450	802388	20.87%	2.428%
8	8.016	815	821	830	rBV	369627	610444	15.88%	1.847%
9	8.734	934	943	956	rBV	563484	1030980	26.82%	3.120%
10	9.193	1013	1021	1033	rBV	470044	829390	21.58%	2.510%
11	9.922	1135	1145	1159	rBV	403020	716050	18.63%	2.167%
12	10.469	1231	1238	1262	rBV	397837	1014464	26.39%	3.070%
13	10.840	1293	1301	1313	rBV	528846	908710	23.64%	2.750%
14	11.022	1325	1332	1341	rBV4	15012	45632	1.19%	0.138%
15	12.451	1570	1575	1581	rBV5	5907	12055	0.31%	0.036%
16	14.075	1843	1851	1866	rBV	1173463	1737841	45.21%	5.259%
17	14.363	1891	1900	1914	rBV	1300053	1944566	50.59%	5.884%
18	14.669	1946	1952	1963	rBV2	872034	1314371	34.19%	3.977%
19	14.892	1984	1990	2019	rBV2	229592	766701	19.95%	2.320%
20	15.669	2115	2122	2135	rBV	1698513	2499406	65.02%	7.563%
21	15.792	2137	2143	2159	rVV	573384	892897	23.23%	2.702%
22	15.910	2160	2163	2169	rVB6	9656	15907	0.41%	0.048%
23	16.451	2252	2255	2260	rBV6	2430	3957	0.10%	0.012%
24	17.433	2415	2422	2432	rBV	1193834	1697953	44.17%	5.138%
25	17.533	2433	2439	2460	rVV	1974008	2911394	75.74%	8.810%
26	17.710	2465	2469	2473	rVB6	2777	5347	0.14%	0.016%
27	19.339	2742	2746	2752	rBV4	28181	43312	1.13%	0.131%
28	19.410	2755	2758	2765	rVB	21483	33571	0.87%	0.102%
29	19.763	2812	2818	2828	rBV	2643307	3491589	90.83%	10.565%
30	21.521	3112	3117	3130	rBV	1415512	2053014	53.41%	6.212%
31	23.880	3510	3518	3531	rBV	1842360	3843963	100.00%	11.631%
32	24.039	3539	3545	3558	rVB2	919681	2041413	53.11%	6.177%




Sum of corrected areas: 33048154

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014395.D
Acq On : 30 Mar 2023 11:12
Operator : CG/JU
Sample : PB151778BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK778

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

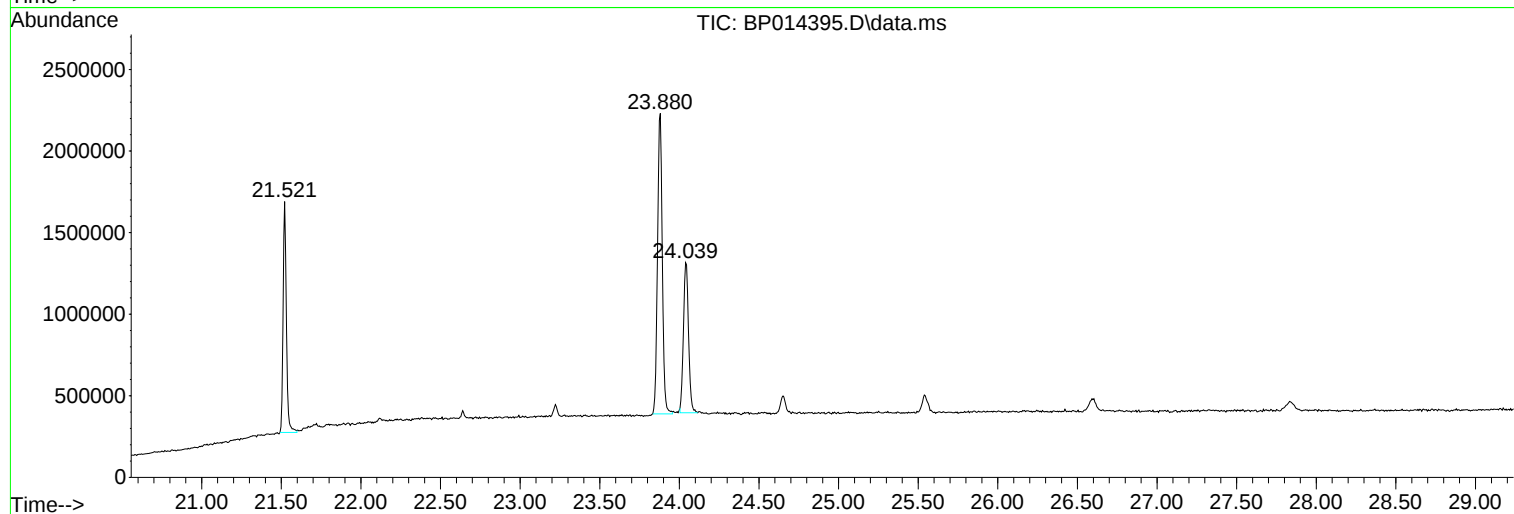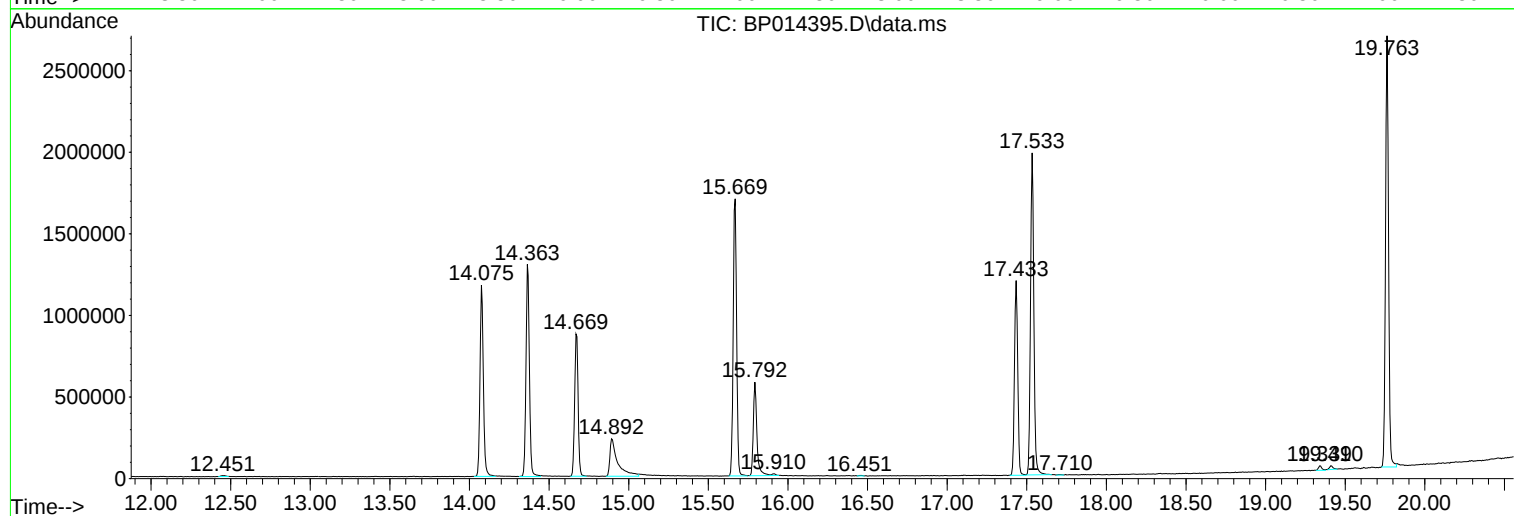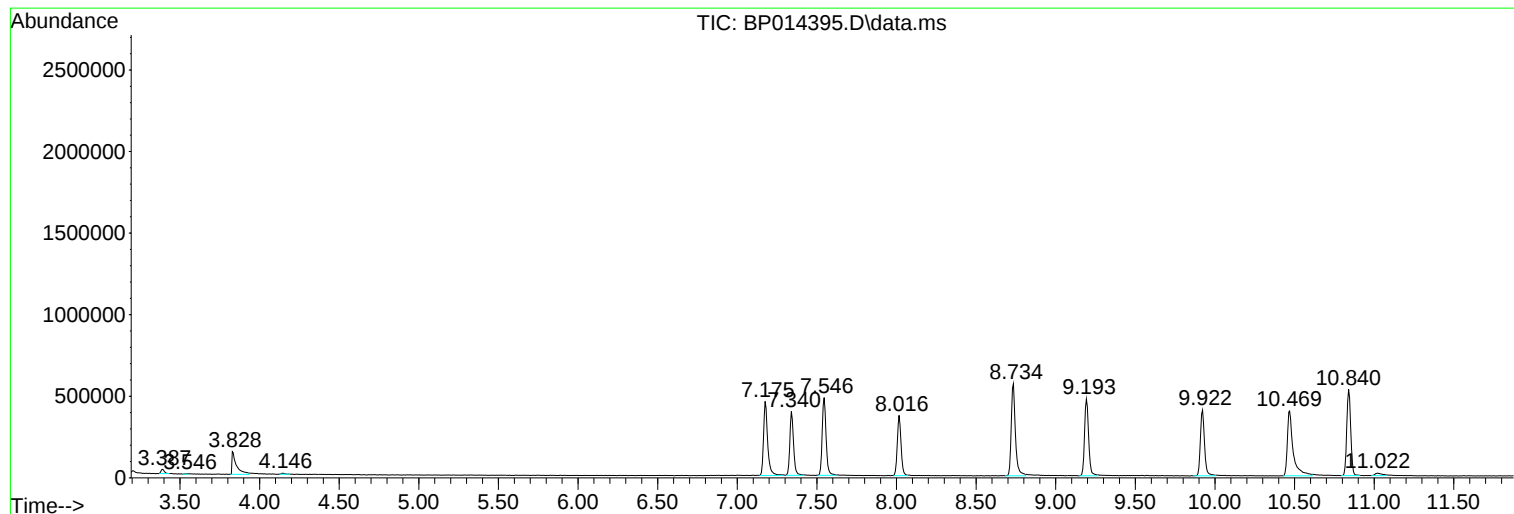

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014395.D
Acq On : 30 Mar 2023 11:12
Operator : CG/JU
Sample : PB151778BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK778

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014395.D
Acq On : 30 Mar 2023 11:12
Operator : CG/JU
Sample : PB151778BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK778

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc