

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014399.D
 Acq On : 30 Mar 2023 13:38
 Operator : CG/JU
 Sample : 02092-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB984

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	35227	53459	1.17%	0.122%
2	3.852	111	113	122	rBV	23719	52520	1.15%	0.120%
3	4.046	140	146	153	rVB3	17567	27474	0.60%	0.063%
4	4.146	159	163	168	rBV2	10774	15673	0.34%	0.036%
5	4.257	178	182	186	rVB5	9001	11548	0.25%	0.026%
6	4.528	226	228	233	rVB5	3761	5668	0.12%	0.013%
7	5.081	317	322	330	rBV	11281	21180	0.46%	0.048%
8	6.393	539	545	554	rVB4	8307	16078	0.35%	0.037%
9	7.110	663	667	672	rVB7	3172	5427	0.12%	0.012%
10	7.181	672	679	695	rBV	129429	252986	5.52%	0.577%
11	7.340	699	706	721	rBV	635704	1004284	21.93%	2.291%
12	7.451	724	725	733	rVB8	3267	4874	0.11%	0.011%
13	7.545	733	741	757	rBV	579161	984991	21.51%	2.247%
14	8.016	814	821	829	rBV	603865	967849	21.14%	2.208%
15	8.734	936	943	964	rBV	429020	795177	17.37%	1.814%
16	9.192	1014	1021	1037	rBV	793340	1349817	29.48%	3.079%
17	9.569	1080	1085	1092	rVB	11964	21050	0.46%	0.048%
18	9.922	1137	1145	1161	rBV	639121	1141769	24.94%	2.604%
19	10.463	1228	1237	1252	rBV	738649	1510241	32.98%	3.445%
20	10.839	1294	1301	1312	rBV	846180	1437832	31.40%	3.280%
21	10.998	1322	1328	1340	rBV	97895	230775	5.04%	0.526%
22	12.063	1503	1509	1516	rBV	3164	6311	0.14%	0.014%
23	12.251	1536	1541	1545	rBV8	5772	9289	0.20%	0.021%
24	12.439	1567	1573	1580	rVB4	14057	29436	0.64%	0.067%
25	12.669	1609	1612	1616	rVB4	3429	4961	0.11%	0.011%
26	13.475	1744	1749	1752	rBV2	9677	12966	0.28%	0.030%
27	13.510	1752	1755	1760	rVV3	5579	10675	0.23%	0.024%
28	13.557	1760	1763	1768	rVB6	6826	10538	0.23%	0.024%
29	13.639	1774	1777	1782	rBV7	3318	4923	0.11%	0.011%
30	14.075	1843	1851	1867	rBV	1862538	2632073	57.48%	6.004%
31	14.192	1869	1871	1877	rVB7	6344	7695	0.17%	0.018%
32	14.363	1893	1900	1915	rBV	1934657	2942453	64.26%	6.712%
33	14.669	1944	1952	1967	rBV	1311850	1990906	43.48%	4.541%
34	14.827	1973	1979	1981	rBV6	4817	8195	0.18%	0.019%
35	14.922	1987	1995	2008	rBV2	46945	164701	3.60%	0.376%
36	15.416	2074	2079	2085	rBV	25797	39508	0.86%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014399.D
 Acq On : 30 Mar 2023 13:38
 Operator : CG/JU
 Sample : 02092-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB984

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.486	2085	2091	2104	rBV	986574	1317053	28.76%	3.004%
38	15.669	2115	2122	2134	rBV	2581488	3700461	80.81%	8.441%
39	15.792	2137	2143	2157	rVV	900731	1371776	29.96%	3.129%
40	15.910	2159	2163	2170	rVB6	14049	24706	0.54%	0.056%
41	16.033	2179	2184	2193	rBV	38474	60560	1.32%	0.138%
42	16.463	2252	2257	2263	rBV10	3959	7146	0.16%	0.016%
43	17.104	2361	2366	2371	rBV9	10422	18260	0.40%	0.042%
44	17.433	2415	2422	2432	rBV	1745909	2406415	52.55%	5.489%
45	17.533	2433	2439	2454	rVV	2851528	4107318	89.70%	9.369%
46	18.298	2565	2569	2575	rBV	141466	218532	4.77%	0.498%
47	19.339	2742	2746	2750	rBV2	33183	51549	1.13%	0.118%
48	19.410	2753	2758	2768	rVV2	42703	82281	1.80%	0.188%
49	19.527	2774	2778	2788	rBV2	90093	148665	3.25%	0.339%
50	19.762	2812	2818	2824	rBV	3516832	4578942	100.00%	10.445%
51	20.704	2975	2978	2981	rVB2	53953	57559	1.26%	0.131%
52	21.198	3059	3062	3069	rBV4	104440	202405	4.42%	0.462%
53	21.521	3112	3117	3129	rBV	1566411	2181814	47.65%	4.977%
54	23.880	3511	3518	3530	rVB2	1773670	3599431	78.61%	8.210%
55	24.039	3539	3545	3557	rVB2	893198	1919294	41.92%	4.378%




Sum of corrected areas: 43839469

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014399.D
Acq On : 30 Mar 2023 13:38
Operator : CG/JU
Sample : 02092-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB984

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

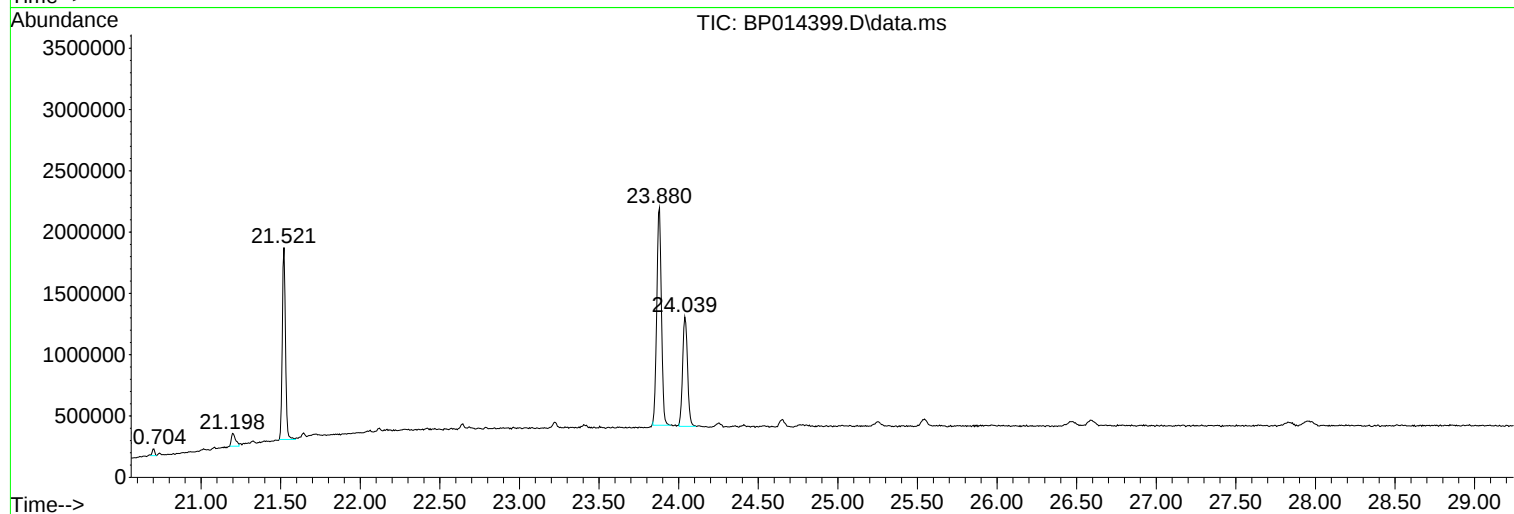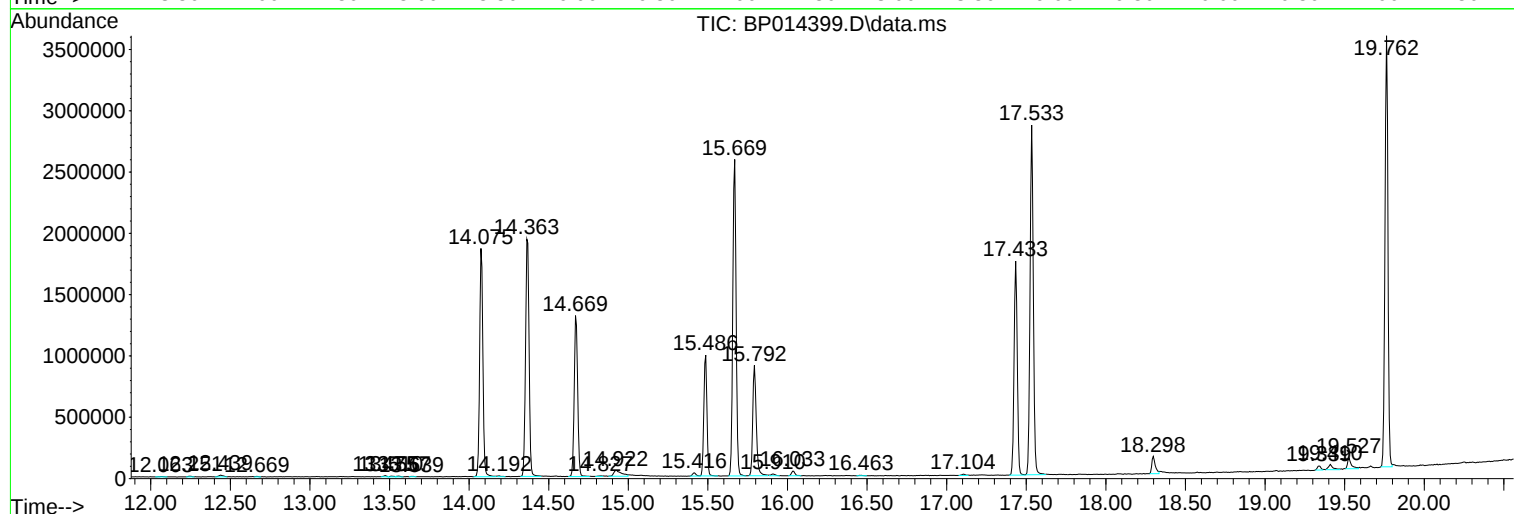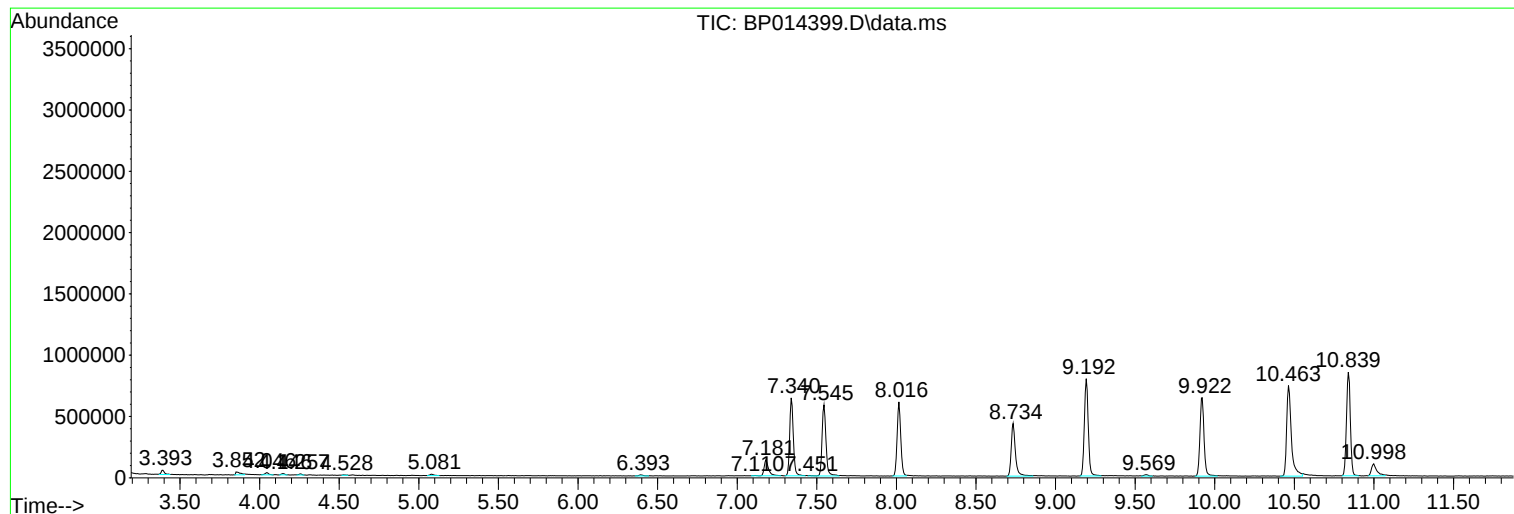

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014399.D
Acq On : 30 Mar 2023 13:38
Operator : CG/JU
Sample : 02092-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB984

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014399.D
Acq On : 30 Mar 2023 13:38
Operator : CG/JU
Sample : 02092-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB984

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc