

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014410.D
 Acq On : 30 Mar 2023 19:48
 Operator : CG/JU
 Sample : PB151800BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK800

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	42	rBV	44948	62567	1.41%	0.134%
2	3.817	104	107	128	rBV	534708	941686	21.29%	2.018%
3	4.146	158	163	169	rBV	10854	15595	0.35%	0.033%
4	7.175	671	678	696	rBV	692720	1206046	27.27%	2.585%
5	7.340	700	706	718	rVV	616941	952914	21.55%	2.042%
6	7.546	734	741	756	rBV	715801	1204127	27.23%	2.581%
7	8.016	813	821	835	rBV	570290	944293	21.35%	2.024%
8	8.728	934	942	961	rBV	877547	1555157	35.17%	3.333%
9	9.193	1013	1021	1034	rBV	748021	1263373	28.57%	2.708%
10	9.916	1136	1144	1158	rBV	652578	1125729	25.46%	2.413%
11	10.463	1230	1237	1262	rBV	785642	1580204	35.73%	3.387%
12	10.840	1293	1301	1312	rBV	860605	1434206	32.43%	3.074%
13	10.987	1318	1326	1347	rBV	750236	1560048	35.28%	3.344%
14	12.446	1568	1574	1586	rVB3	11315	31200	0.71%	0.067%
15	14.075	1844	1851	1866	rBV	1886072	2695178	60.94%	5.777%
16	14.363	1893	1900	1915	rBV	2019552	2962238	66.98%	6.349%
17	14.669	1944	1952	1960	rBV	1436758	2077144	46.97%	4.452%
18	14.887	1981	1989	2013	rBV	350143	1037729	23.47%	2.224%
19	15.122	2027	2029	2037	rVB8	3895	4964	0.11%	0.011%
20	15.663	2114	2121	2133	rBV	2572857	3760598	85.04%	8.060%
21	15.792	2137	2143	2158	rVV	907125	1410199	31.89%	3.022%
22	15.910	2159	2163	2169	rVB6	15309	26540	0.60%	0.057%
23	16.445	2251	2254	2264	rVB6	3934	8250	0.19%	0.018%
24	17.228	2382	2387	2390	rBV7	5170	8397	0.19%	0.018%
25	17.434	2414	2422	2432	rBV	1765704	2512773	56.82%	5.386%
26	17.534	2432	2439	2457	rVV	2814819	4066282	91.95%	8.715%
27	18.339	2571	2576	2581	rBV9	6072	15357	0.35%	0.033%
28	19.339	2742	2746	2750	rBV3	31275	43842	0.99%	0.094%
29	19.410	2754	2758	2764	rVV	32810	44939	1.02%	0.096%
30	19.763	2812	2818	2827	rBV	3392908	4422362	100.00%	9.478%
31	21.522	3112	3117	3128	rBV	1522823	2197782	49.70%	4.710%
32	23.880	3510	3518	3529	rBV2	1669144	3525992	79.73%	7.557%
33	24.039	3539	3545	3559	rVB2	902843	1959744	44.31%	4.200%




Sum of corrected areas: 46657455

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014410.D
Acq On : 30 Mar 2023 19:48
Operator : CG/JU
Sample : PB151800BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

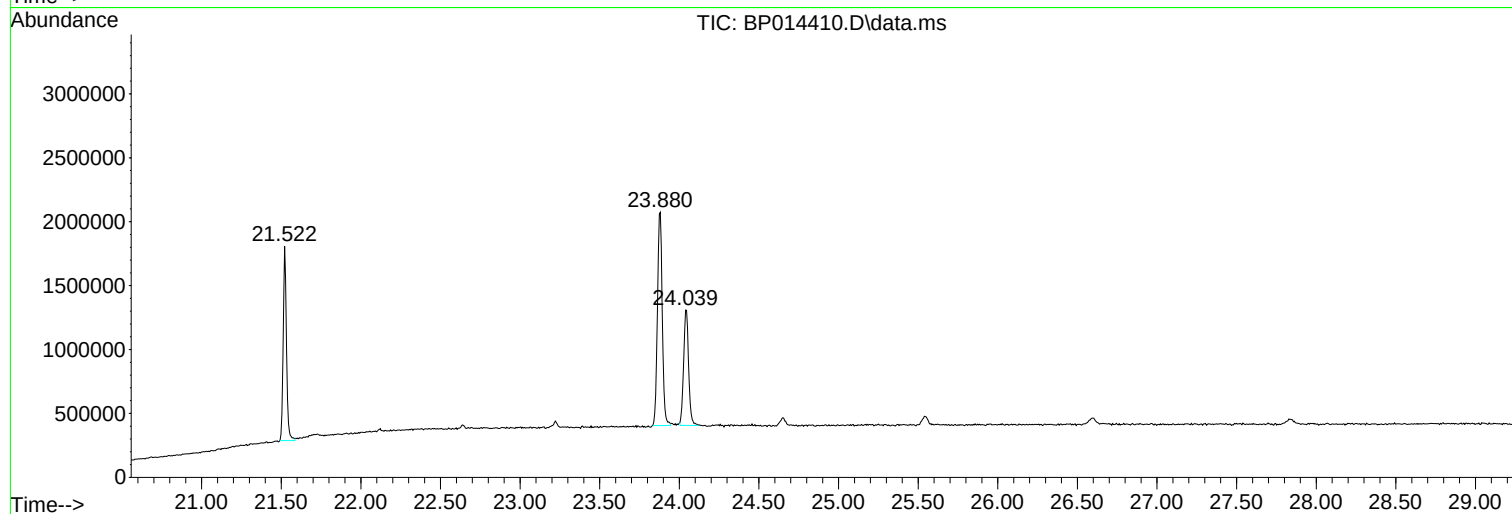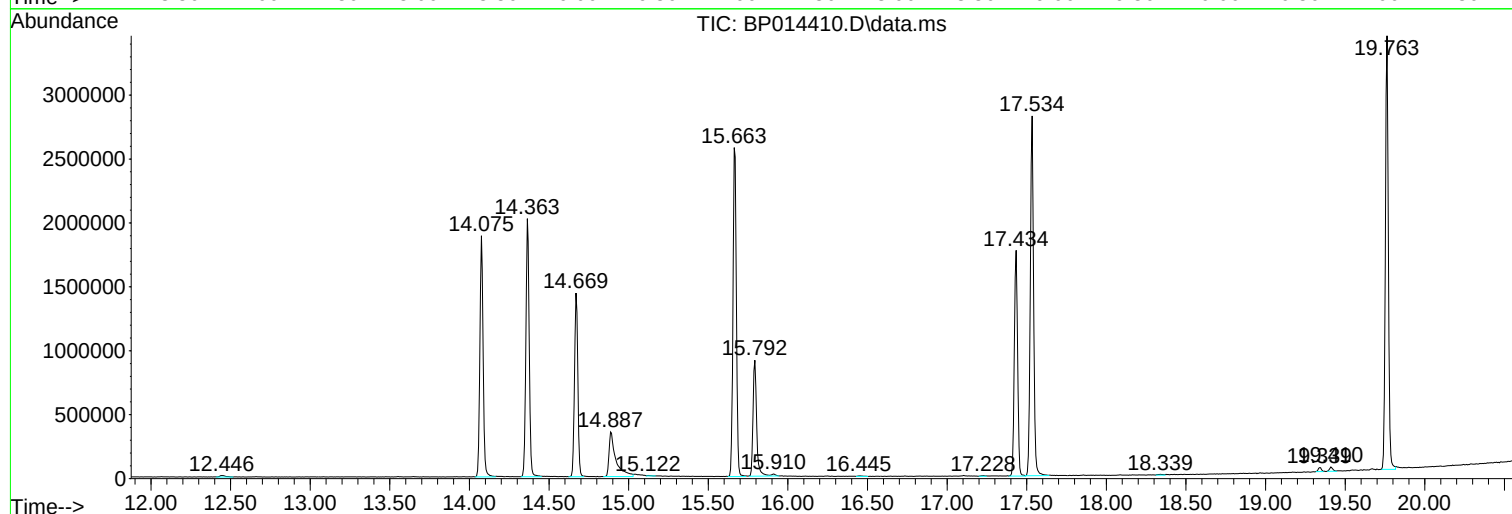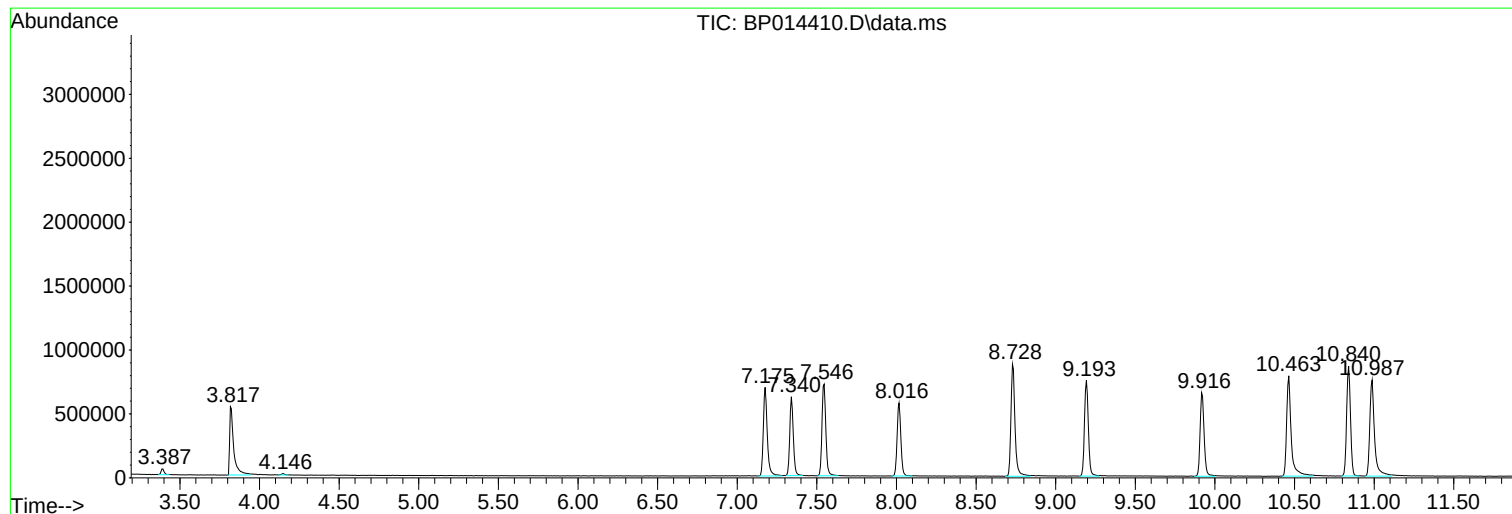

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014410.D
Acq On : 30 Mar 2023 19:48
Operator : CG/JU
Sample : PB151800BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014410.D
Acq On : 30 Mar 2023 19:48
Operator : CG/JU
Sample : PB151800BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc