

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014413.D
 Acq On : 30 Mar 2023 21:29
 Operator : CG/JU
 Sample : 02038-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	43624	59507	1.18%	0.116%
2	3.828	106	109	123	rBV	172038	290745	5.77%	0.568%
3	4.046	141	146	152	rVB	19319	33069	0.66%	0.065%
4	4.146	159	163	168	rBV2	15221	21495	0.43%	0.042%
5	4.257	178	182	187	rVB3	12085	17895	0.36%	0.035%
6	5.081	318	322	331	rVB	12594	19661	0.39%	0.038%
7	6.393	540	545	551	rVB4	10267	16956	0.34%	0.033%
8	7.175	673	678	688	rBV	153699	297963	5.91%	0.582%
9	7.340	698	706	722	rBV	766737	1206334	23.94%	2.356%
10	7.545	734	741	751	rBV	677109	1142011	22.66%	2.230%
11	8.016	813	821	836	rBV	690315	1128217	22.39%	2.203%
12	8.734	935	943	959	rBV	508791	938751	18.63%	1.833%
13	9.192	1013	1021	1038	rBV	966135	1620094	32.15%	3.164%
14	9.569	1081	1085	1092	rVB9	4861	9646	0.19%	0.019%
15	9.916	1137	1144	1164	rBV	794154	1381751	27.42%	2.698%
16	10.463	1229	1237	1258	rBV	885822	1790481	35.53%	3.497%
17	10.839	1291	1301	1315	rBV	1010070	1705445	33.85%	3.331%
18	10.986	1317	1326	1351	rBV	851759	1754689	34.82%	3.427%
19	12.069	1505	1510	1515	rVB5	4841	7874	0.16%	0.015%
20	12.439	1566	1573	1581	rBV4	14879	34068	0.68%	0.067%
21	13.551	1760	1762	1768	rVB7	5099	5582	0.11%	0.011%
22	14.074	1842	1851	1867	rBV	2310693	3271365	64.92%	6.389%
23	14.363	1893	1900	1915	rBV2	2460387	3694583	73.32%	7.215%
24	14.669	1944	1952	1963	rBV	1608901	2380334	47.24%	4.649%
25	14.927	1988	1996	2010	rBV2	42642	171238	3.40%	0.334%
26	15.451	2079	2085	2087	rBV6	3938	6575	0.13%	0.013%
27	15.486	2087	2091	2095	rVB5	4136	6550	0.13%	0.013%
28	15.663	2115	2121	2134	rBV	3171530	4639931	92.09%	9.061%
29	15.792	2137	2143	2157	rVV	1075434	1628811	32.33%	3.181%
30	15.910	2159	2163	2169	rVB2	15275	28381	0.56%	0.055%
31	16.027	2181	2183	2190	rVB8	4615	8636	0.17%	0.017%
32	16.374	2238	2242	2246	rBV7	3580	6392	0.13%	0.012%
33	16.451	2252	2255	2262	rVB9	3586	6417	0.13%	0.013%
34	16.551	2268	2272	2276	rVB7	4097	6324	0.13%	0.012%
35	17.110	2364	2367	2371	rVB6	4718	6614	0.13%	0.013%
36	17.221	2381	2386	2391	rBV6	5943	10858	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014413.D
 Acq On : 30 Mar 2023 21:29
 Operator : CG/JU
 Sample : 02038-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.433	2414	2422	2431	rBV	1953531	2693878	53.46%	5.261%
38	17.533	2432	2439	2455	rVV	3438593	4911110	97.47%	9.591%
39	18.310	2569	2571	2576	rVB5	5438	5723	0.11%	0.011%
40	19.339	2742	2746	2751	rVB2	40182	54094	1.07%	0.106%
41	19.410	2754	2758	2766	rVV2	35655	56335	1.12%	0.110%
42	19.762	2812	2818	2831	rBV	3723788	5038743	100.00%	9.840%
43	21.521	3112	3117	3126	rBV	1613544	2280952	45.27%	4.454%
44	23.880	3510	3518	3527	rBV2	2206375	4548983	90.28%	8.884%
45	24.039	3539	3545	3556	rVB2	1046548	2261206	44.88%	4.416%




Sum of corrected areas: 51206267

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014413.D
Acq On : 30 Mar 2023 21:29
Operator : CG/JU
Sample : 02038-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

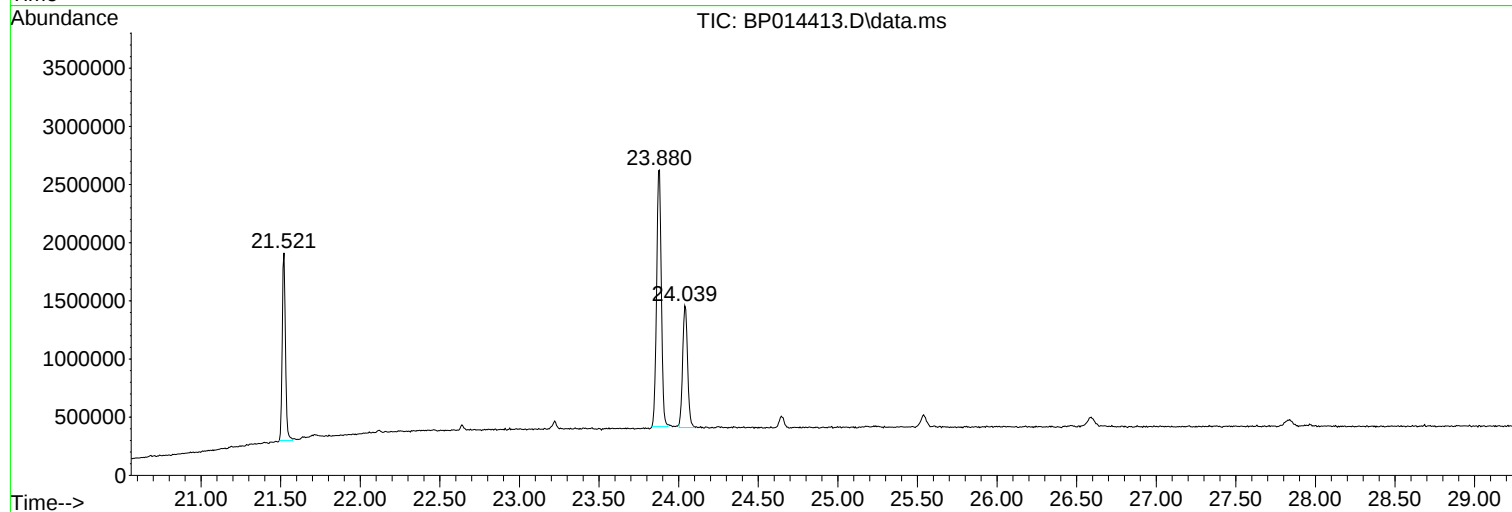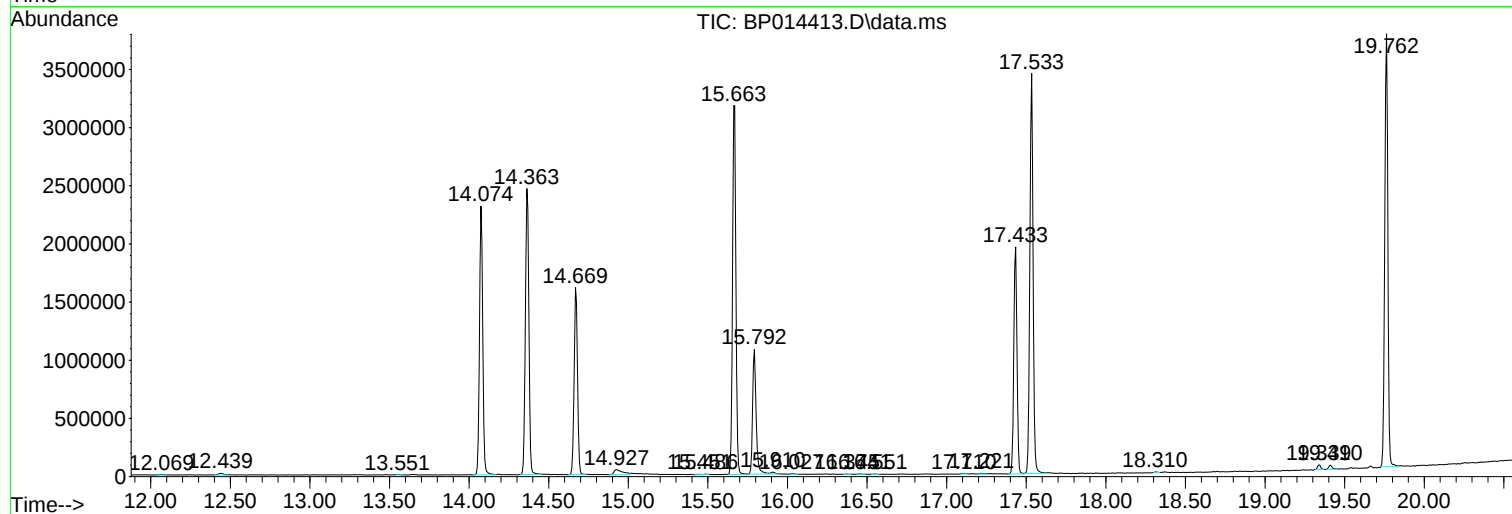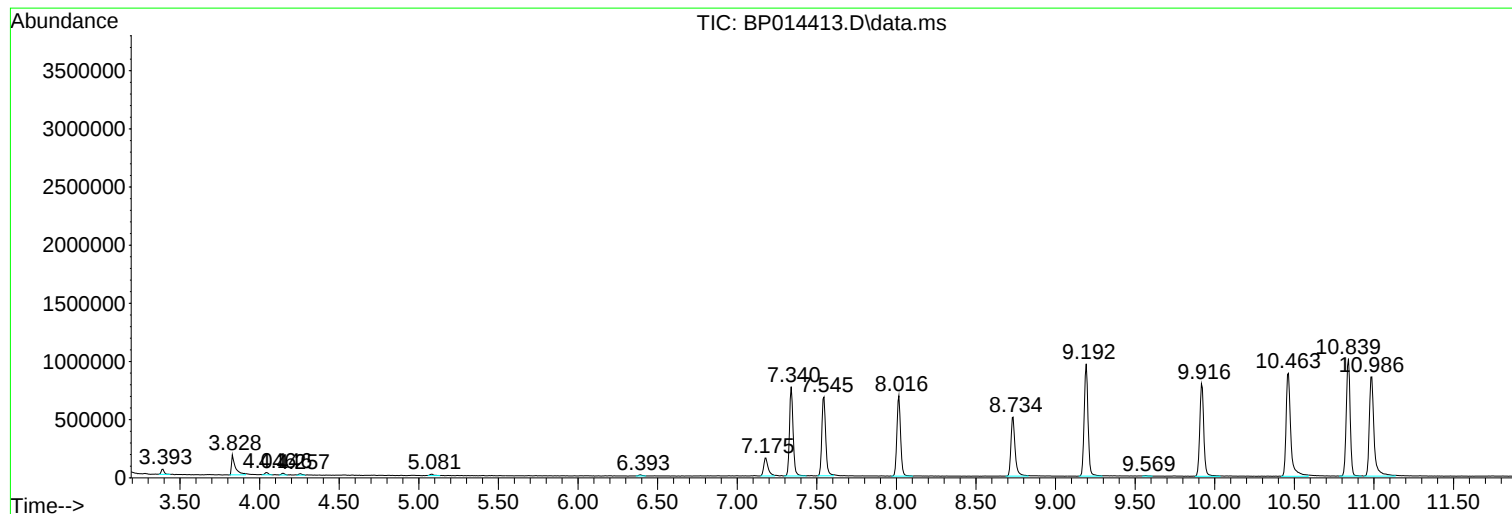

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014413.D
Acq On : 30 Mar 2023 21:29
Operator : CG/JU
Sample : 02038-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014413.D
Acq On : 30 Mar 2023 21:29
Operator : CG/JU
Sample : 02038-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc