

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014416.D
 Acq On : 30 Mar 2023 23:10
 Operator : CG/JU
 Sample : 02038-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	13	15	20	rBV6	4462	6569	0.12%	0.013%
2	3.387	31	34	47	rVB	42485	62403	1.09%	0.122%
3	3.828	106	109	127	rBV	154283	303486	5.32%	0.592%
4	4.040	141	145	151	rVB	17007	26730	0.47%	0.052%
5	4.146	160	163	168	rVB	9390	11534	0.20%	0.023%
6	4.258	178	182	187	rVB4	10490	16473	0.29%	0.032%
7	5.081	317	322	326	rBV	11762	17711	0.31%	0.035%
8	6.393	540	545	551	rBV2	9481	14497	0.25%	0.028%
9	7.105	663	666	670	rBV3	7971	11281	0.20%	0.022%
10	7.175	673	678	693	rBV	138395	281646	4.94%	0.550%
11	7.340	698	706	720	rBV	750790	1206905	21.16%	2.356%
12	7.540	733	740	759	rBV	640840	1118259	19.61%	2.183%
13	8.016	814	821	830	rBV	535823	890275	15.61%	1.738%
14	8.728	936	942	957	rBV	487624	892270	15.65%	1.741%
15	9.193	1013	1021	1038	rBV	944533	1613896	28.30%	3.150%
16	9.569	1079	1085	1092	rBV2	21583	36604	0.64%	0.071%
17	9.916	1134	1144	1156	rBV	806058	1368740	24.00%	2.671%
18	10.457	1225	1236	1260	rBV	895990	1795089	31.48%	3.504%
19	10.840	1293	1301	1309	rBV	803051	1363099	23.90%	2.660%
20	10.981	1319	1325	1350	rBV	864105	1731248	30.36%	3.379%
21	11.140	1350	1352	1362	rVB	4620	8122	0.14%	0.016%
22	12.069	1502	1510	1514	rVB2	18151	27867	0.49%	0.054%
23	12.440	1565	1573	1584	rBV2	14766	37315	0.65%	0.073%
24	14.075	1841	1851	1866	rBV	2421026	3409908	59.79%	6.655%
25	14.363	1890	1900	1918	rBV	2623619	3848544	67.48%	7.511%
26	14.669	1945	1952	1962	rBV	1355095	1991501	34.92%	3.887%
27	14.922	1988	1995	2014	rBV3	45500	193808	3.40%	0.378%
28	15.075	2019	2021	2027	rVB7	5679	9198	0.16%	0.018%
29	15.610	2107	2112	2114	rBV6	4753	6084	0.11%	0.012%
30	15.663	2114	2121	2129	rBV	3422775	4857013	85.17%	9.480%
31	15.792	2136	2143	2159	rBV	1153285	1757803	30.82%	3.431%
32	15.910	2159	2163	2170	rVB2	16062	28655	0.50%	0.056%
33	16.039	2180	2185	2191	rVB3	8230	15365	0.27%	0.030%
34	16.457	2250	2256	2261	rBV9	3977	7973	0.14%	0.016%
35	17.098	2363	2365	2367	rBV3	5770	6847	0.12%	0.013%
36	17.428	2415	2421	2432	rBV	1628190	2397173	42.03%	4.679%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014416.D
 Acq On : 30 Mar 2023 23:10
 Operator : CG/JU
 Sample : 02038-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.533	2432	2439	2455	rVV	3625431	5345393	93.73%	10.433%
38	18.298	2565	2569	2578	rBV6	39120	76391	1.34%	0.149%
39	19.339	2741	2746	2751	rBV	49877	77296	1.36%	0.151%
40	19.404	2753	2757	2767	rVV	45967	87029	1.53%	0.170%
41	19.527	2775	2778	2783	rBV4	28036	43333	0.76%	0.085%
42	19.657	2798	2800	2804	rBV5	15548	18105	0.32%	0.035%
43	19.757	2811	2817	2825	rBV	4148545	5702817	100.00%	11.131%
44	21.516	3111	3116	3127	rBV	1446882	2184584	38.31%	4.264%
45	23.874	3509	3517	3529	rBV2	2168560	4476467	78.50%	8.737%
46	24.039	3538	3545	3557	rVB2	840063	1852439	32.48%	3.616%




Sum of corrected areas: 51235745

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014416.D
Acq On : 30 Mar 2023 23:10
Operator : CG/JU
Sample : 02038-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

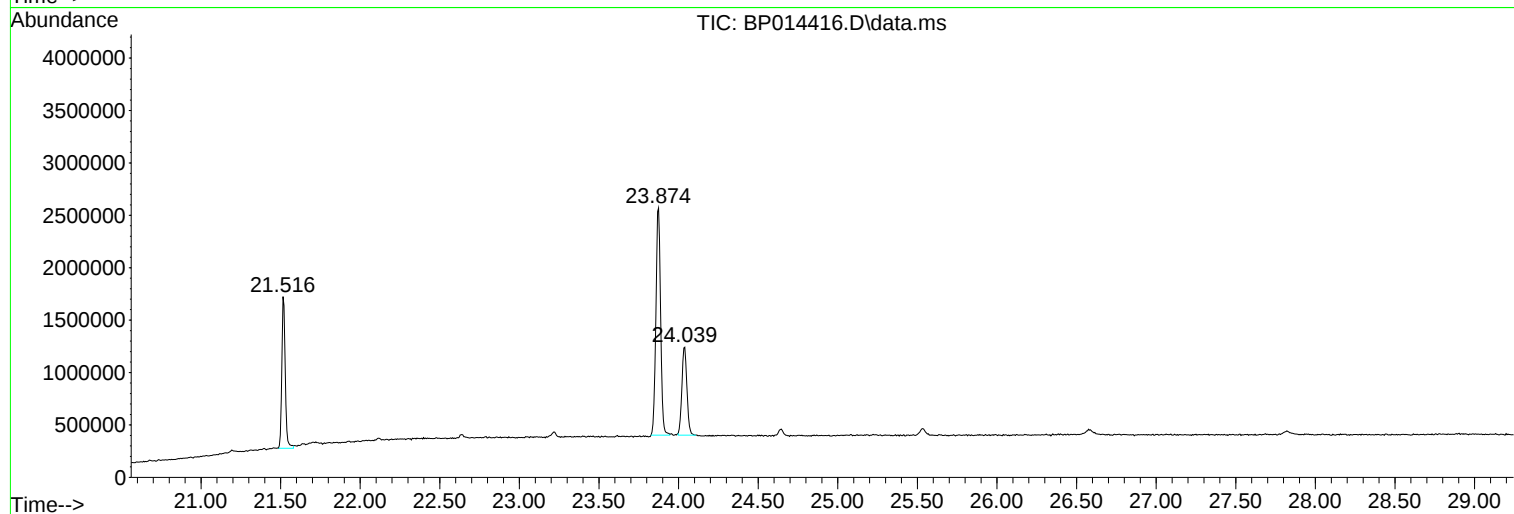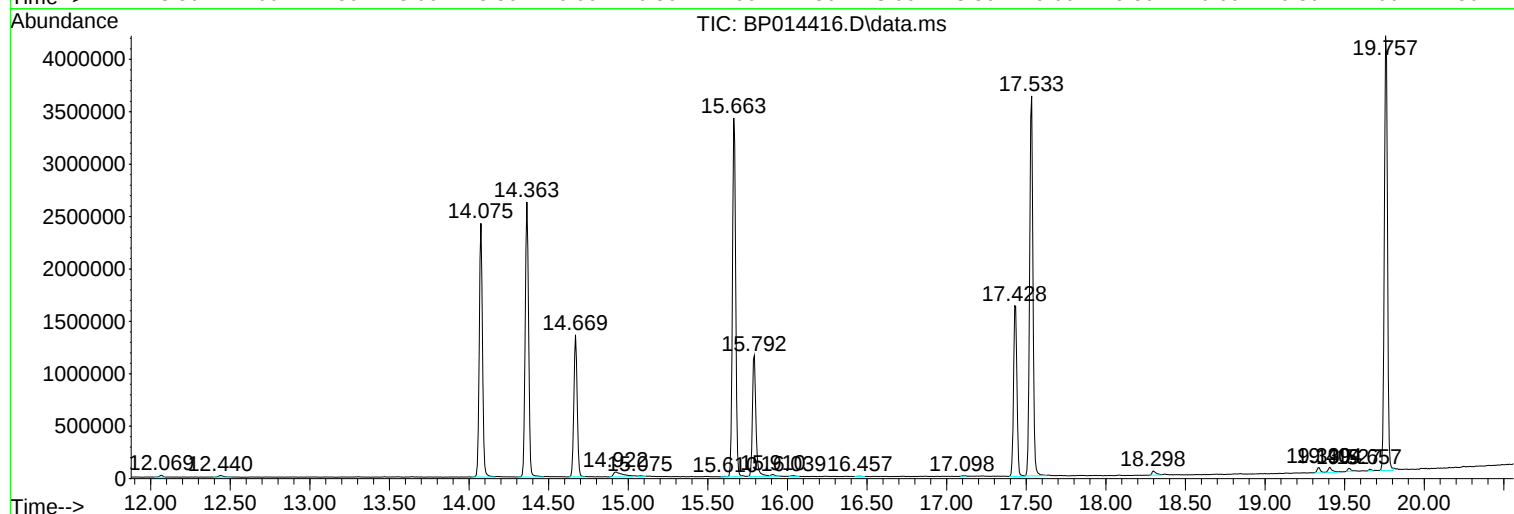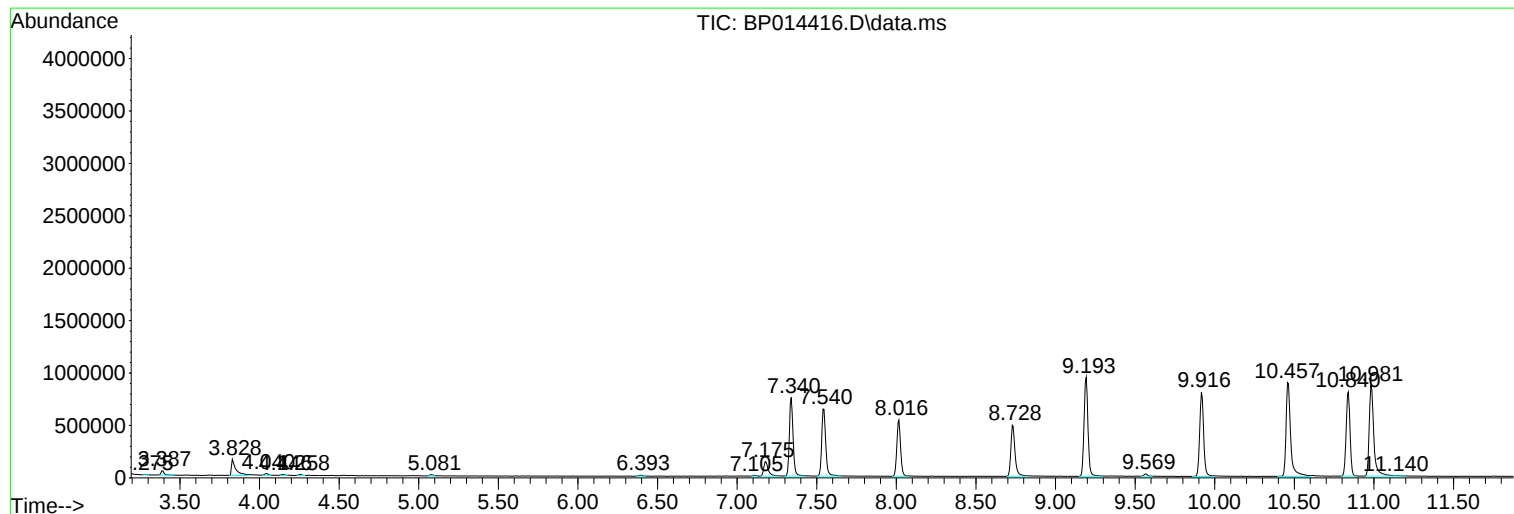

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014416.D
Acq On : 30 Mar 2023 23:10
Operator : CG/JU
Sample : 02038-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014416.D
Acq On : 30 Mar 2023 23:10
Operator : CG/JU
Sample : 02038-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc