

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014417.D
 Acq On : 30 Mar 2023 23:43
 Operator : CG/JU
 Sample : 02038-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	31	34	41	rVB	42038	53987	1.16%	0.114%
2	3.828	106	109	131	rBV	162730	305915	6.59%	0.644%
3	4.046	141	146	152	rVB2	18428	27860	0.60%	0.059%
4	4.146	160	163	168	rVB2	13000	18704	0.40%	0.039%
5	4.252	178	181	186	rVB5	9525	12526	0.27%	0.026%
6	5.081	316	322	331	rBV	12796	22249	0.48%	0.047%
7	6.387	539	544	549	rBV3	9066	15662	0.34%	0.033%
8	7.105	659	666	672	rBV	17675	29797	0.64%	0.063%
9	7.175	672	678	692	rVV	141978	274630	5.91%	0.578%
10	7.340	699	706	720	rBV	747099	1178812	25.38%	2.481%
11	7.540	732	740	762	rBV	649132	1115331	24.01%	2.347%
12	8.016	813	821	834	rBV	589296	990559	21.32%	2.085%
13	8.728	935	942	960	rBV	469480	871435	18.76%	1.834%
14	9.193	1014	1021	1035	rBV	906007	1560771	33.60%	3.285%
15	9.569	1077	1085	1092	rVB	57898	94488	2.03%	0.199%
16	9.916	1136	1144	1159	rBV	758727	1315933	28.33%	2.770%
17	10.457	1228	1236	1259	rBV	860971	1717338	36.97%	3.614%
18	10.746	1281	1285	1290	rVB6	5130	8510	0.18%	0.018%
19	10.840	1290	1301	1315	rBV	866323	1471658	31.68%	3.097%
20	10.981	1318	1325	1344	rBV	764075	1552551	33.42%	3.268%
21	12.069	1505	1510	1516	rVB	23906	35896	0.77%	0.076%
22	12.440	1567	1573	1581	rBV4	13552	29755	0.64%	0.063%
23	13.481	1744	1750	1753	rBV8	3052	5171	0.11%	0.011%
24	14.075	1842	1851	1866	rBV	2217838	3128809	67.35%	6.585%
25	14.187	1868	1870	1875	rVB6	4512	6219	0.13%	0.013%
26	14.363	1892	1900	1914	rBV	2419880	3511679	75.59%	7.391%
27	14.545	1926	1931	1936	rVB7	7105	11332	0.24%	0.024%
28	14.669	1942	1952	1963	rBV	1384817	2022283	43.53%	4.256%
29	14.922	1990	1995	2002	rBV4	33370	94310	2.03%	0.198%
30	15.069	2018	2020	2025	rVB6	5104	7521	0.16%	0.016%
31	15.492	2088	2092	2096	rVB4	11826	15890	0.34%	0.033%
32	15.663	2114	2121	2136	rBV	3024389	4372469	94.12%	9.202%
33	15.792	2136	2143	2156	rVV	904409	1434096	30.87%	3.018%
34	15.904	2159	2162	2170	rVB4	18681	30464	0.66%	0.064%
35	16.034	2181	2184	2190	rVB6	7196	11828	0.25%	0.025%
36	16.234	2215	2218	2224	rVB8	3605	6365	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014417.D
 Acq On : 30 Mar 2023 23:43
 Operator : CG/JU
 Sample : 02038-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.363	2234	2240	2248	rBV3	16314	30675	0.66%	0.065%
38	16.451	2251	2255	2262	rVB9	5069	8860	0.19%	0.019%
39	16.716	2295	2300	2301	rBV5	3756	5239	0.11%	0.011%
40	17.163	2373	2376	2379	rVV2	12330	13382	0.29%	0.028%
41	17.222	2381	2386	2389	rVB6	5802	9060	0.20%	0.019%
42	17.428	2414	2421	2432	rBV	1512545	2206328	47.49%	4.643%
43	17.534	2432	2439	2454	rVV	3007514	4460710	96.02%	9.388%
44	17.704	2467	2468	2473	rVB5	4901	4966	0.11%	0.010%
45	17.839	2487	2491	2494	rBV6	3891	5461	0.12%	0.011%
46	17.898	2498	2501	2506	rVV4	9579	12160	0.26%	0.026%
47	18.081	2529	2532	2538	rBV7	7037	10315	0.22%	0.022%
48	18.304	2567	2570	2578	rBV8	10859	24339	0.52%	0.051%
49	18.569	2613	2615	2618	rVB3	9485	7482	0.16%	0.016%
50	19.339	2742	2746	2751	rBV3	38852	57274	1.23%	0.121%
51	19.404	2753	2757	2764	rVV2	35377	59298	1.28%	0.125%
52	19.757	2811	2817	2832	rBV	3467245	4645521	100.00%	9.777%
53	21.516	3111	3116	3125	rBV	1369723	2011154	43.29%	4.233%
54	23.874	3509	3517	3528	rBV2	2205067	4557447	98.10%	9.592%
55	24.033	3538	3544	3554	rVB2	959944	2022424	43.53%	4.256%




Sum of corrected areas: 47514898

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014417.D
Acq On : 30 Mar 2023 23:43
Operator : CG/JU
Sample : 02038-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

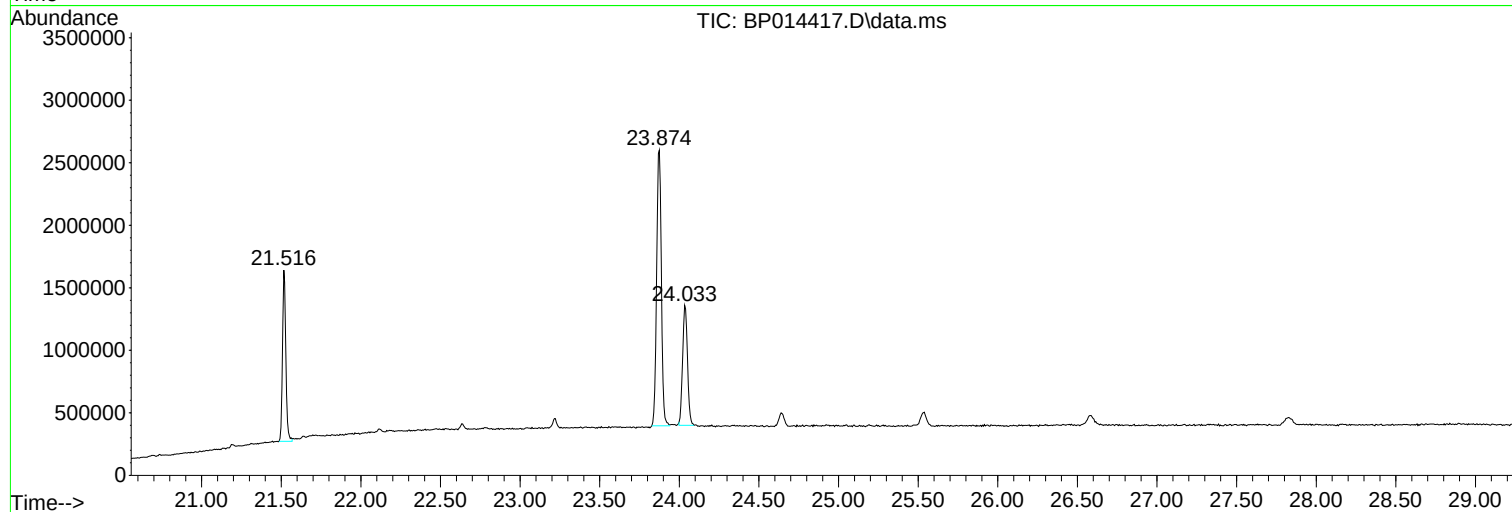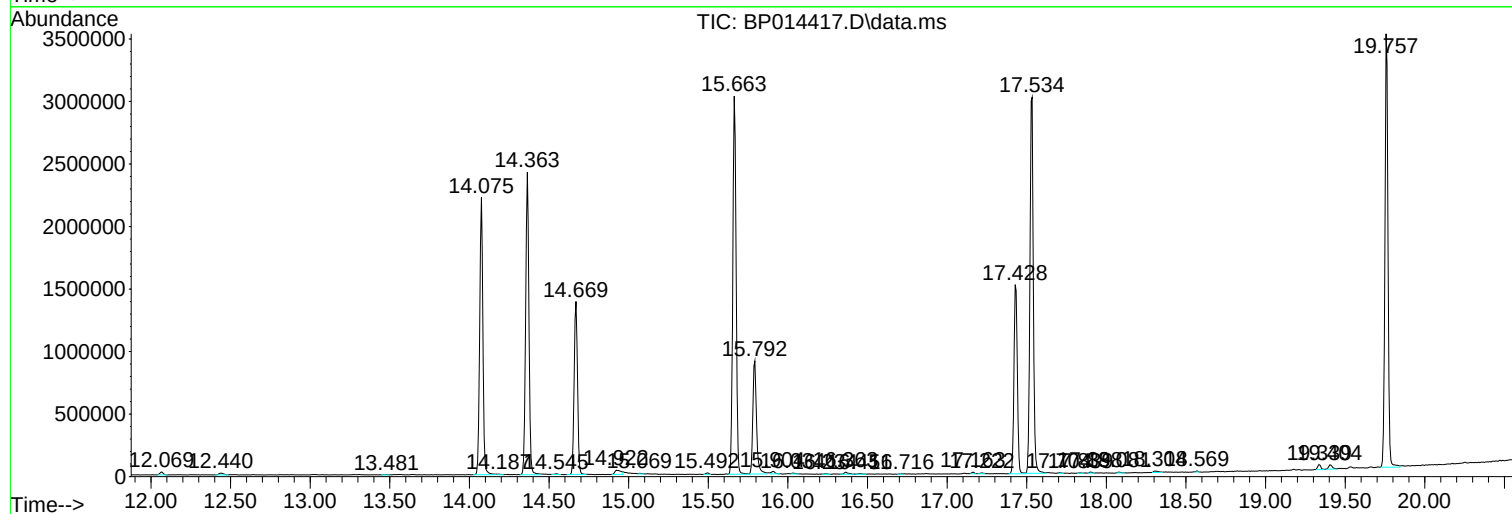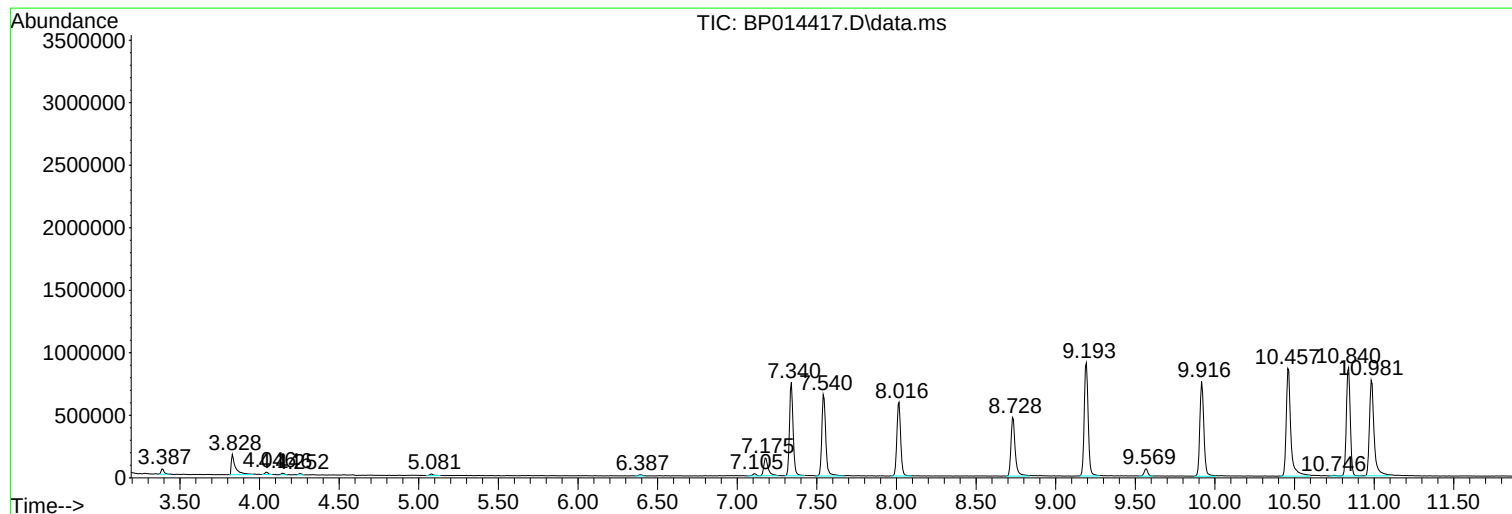

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014417.D
Acq On : 30 Mar 2023 23:43
Operator : CG/JU
Sample : 02038-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014417.D
Acq On : 30 Mar 2023 23:43
Operator : CG/JU
Sample : 02038-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc