

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014418.D
 Acq On : 31 Mar 2023 00:17
 Operator : CG/JU
 Sample : 02038-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	14	16	22	rVB7	6469	6084	0.13%	0.013%
2	3.387	30	34	42	rVB	36993	50531	1.05%	0.109%
3	3.834	107	110	121	rBV	91993	170613	3.53%	0.368%
4	4.046	141	146	154	rVB	18558	36667	0.76%	0.079%
5	4.146	159	163	168	rVV2	10744	14458	0.30%	0.031%
6	4.252	176	181	186	rBV6	8873	14791	0.31%	0.032%
7	4.575	233	236	242	rVB7	3873	6391	0.13%	0.014%
8	5.081	317	322	331	rVB2	11965	21775	0.45%	0.047%
9	6.393	540	545	552	rVB7	7631	14213	0.29%	0.031%
10	7.105	662	666	672	rVB	16263	26507	0.55%	0.057%
11	7.175	672	678	693	rBV	131746	267666	5.54%	0.578%
12	7.340	699	706	722	rBV	670747	1078381	22.32%	2.327%
13	7.540	733	740	756	rBV	597236	1020425	21.12%	2.202%
14	8.010	813	820	831	rBV	546818	911641	18.87%	1.967%
15	8.728	936	942	958	rBV	441656	804351	16.65%	1.736%
16	9.193	1014	1021	1036	rBV	840858	1436358	29.73%	3.100%
17	9.563	1078	1084	1093	rVB2	37927	60439	1.25%	0.130%
18	9.916	1135	1144	1157	rBV	697127	1204617	24.94%	2.600%
19	10.457	1229	1236	1256	rBV	798731	1577999	32.67%	3.405%
20	10.752	1282	1286	1291	rVB5	3103	5299	0.11%	0.011%
21	10.840	1293	1301	1312	rVB	833292	1394917	28.88%	3.010%
22	10.981	1318	1325	1353	rBV	711502	1451235	30.04%	3.132%
23	12.063	1504	1509	1515	rVB2	12194	19871	0.41%	0.043%
24	12.446	1568	1574	1582	rVB2	11608	27114	0.56%	0.059%
25	13.475	1742	1749	1756	rBV2	5077	10342	0.21%	0.022%
26	14.075	1842	1851	1865	rBV	2145691	3046230	63.06%	6.574%
27	14.181	1865	1869	1876	rVV10	5644	14219	0.29%	0.031%
28	14.363	1893	1900	1921	rBV	2342343	3415025	70.70%	7.370%
29	14.545	1926	1931	1935	rVB	15748	20816	0.43%	0.045%
30	14.669	1945	1952	1960	rBV	1383818	2008020	41.57%	4.334%
31	15.492	2088	2092	2097	rBV	37292	49012	1.01%	0.106%
32	15.610	2106	2112	2114	rBV7	4446	7388	0.15%	0.016%
33	15.663	2114	2121	2130	rBV	3062287	4349480	90.04%	9.387%
34	15.792	2136	2143	2156	rBV	948708	1483211	30.70%	3.201%
35	15.904	2158	2162	2167	rVB5	22819	38722	0.80%	0.084%
36	16.034	2180	2184	2191	rVB2	29527	45810	0.95%	0.099%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014418.D
 Acq On : 31 Mar 2023 00:17
 Operator : CG/JU
 Sample : 02038-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.239	2216	2219	2224	rVB7	3224	4993	0.10%	0.011%
38	16.363	2235	2240	2249	rBV	53833	95380	1.97%	0.206%
39	16.451	2253	2255	2260	rVB6	4804	6943	0.14%	0.015%
40	16.939	2335	2338	2343	rBV7	4882	7915	0.16%	0.017%
41	17.104	2363	2366	2368	rBV3	5281	6636	0.14%	0.014%
42	17.163	2371	2376	2379	rVV	45120	56638	1.17%	0.122%
43	17.210	2381	2384	2394	rVB7	16366	32472	0.67%	0.070%
44	17.428	2414	2421	2432	rBV	1665627	2348028	48.61%	5.067%
45	17.534	2432	2439	2454	rVV	3118309	4578823	94.79%	9.882%
46	17.634	2454	2456	2463	rVV8	10044	18432	0.38%	0.040%
47	17.710	2465	2469	2473	rVB7	7215	11099	0.23%	0.024%
48	17.898	2497	2501	2506	rBV	32813	40704	0.84%	0.088%
49	18.075	2528	2531	2536	rVB2	20264	26342	0.55%	0.057%
50	18.298	2565	2569	2577	rBV3	43525	90811	1.88%	0.196%
51	18.569	2611	2615	2619	rBV	24471	29279	0.61%	0.063%
52	19.175	2715	2718	2721	rBV	17339	21492	0.44%	0.046%
53	19.333	2741	2745	2751	rBV3	46526	74378	1.54%	0.161%
54	19.404	2753	2757	2765	rVV	35980	69214	1.43%	0.149%
55	19.528	2775	2778	2781	rBV5	26855	34847	0.72%	0.075%
56	19.757	2811	2817	2831	rBV	3663239	4830537	100.00%	10.425%
57	21.516	3111	3116	3124	rBV2	1388429	2005862	41.52%	4.329%
58	23.874	3509	3517	3530	rBV2	1848779	4033010	83.49%	8.704%
59	24.033	3538	3544	3553	rVB	881480	1802483	37.31%	3.890%




Sum of corrected areas: 46336936

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014418.D
Acq On : 31 Mar 2023 00:17
Operator : CG/JU
Sample : 02038-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

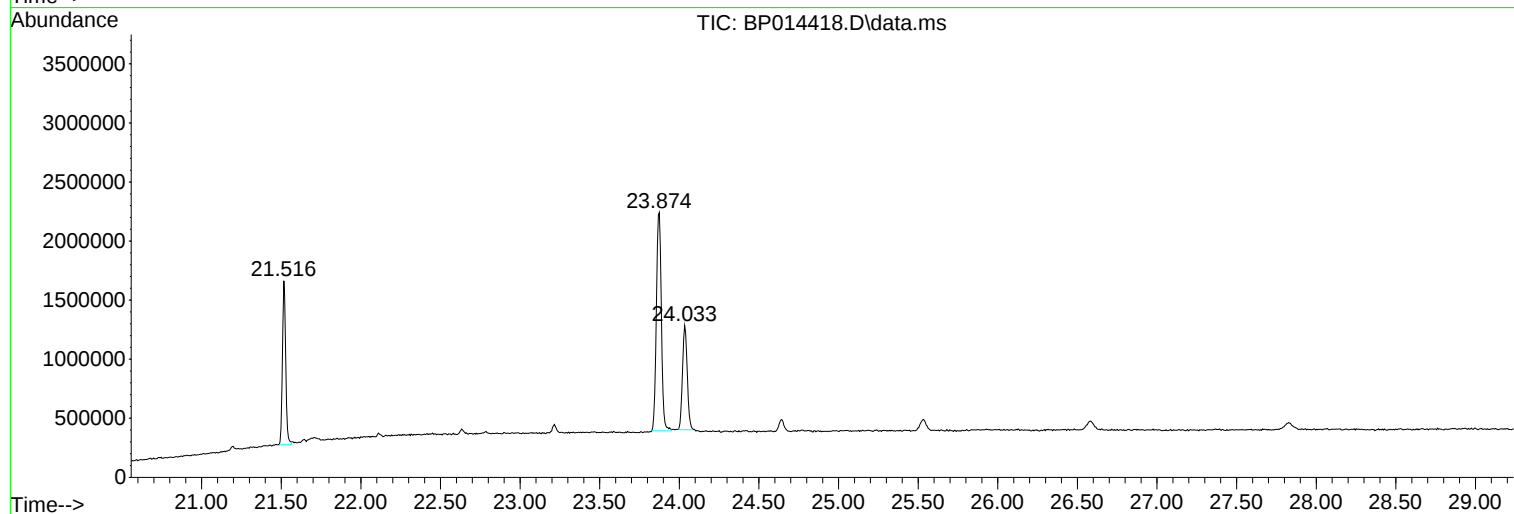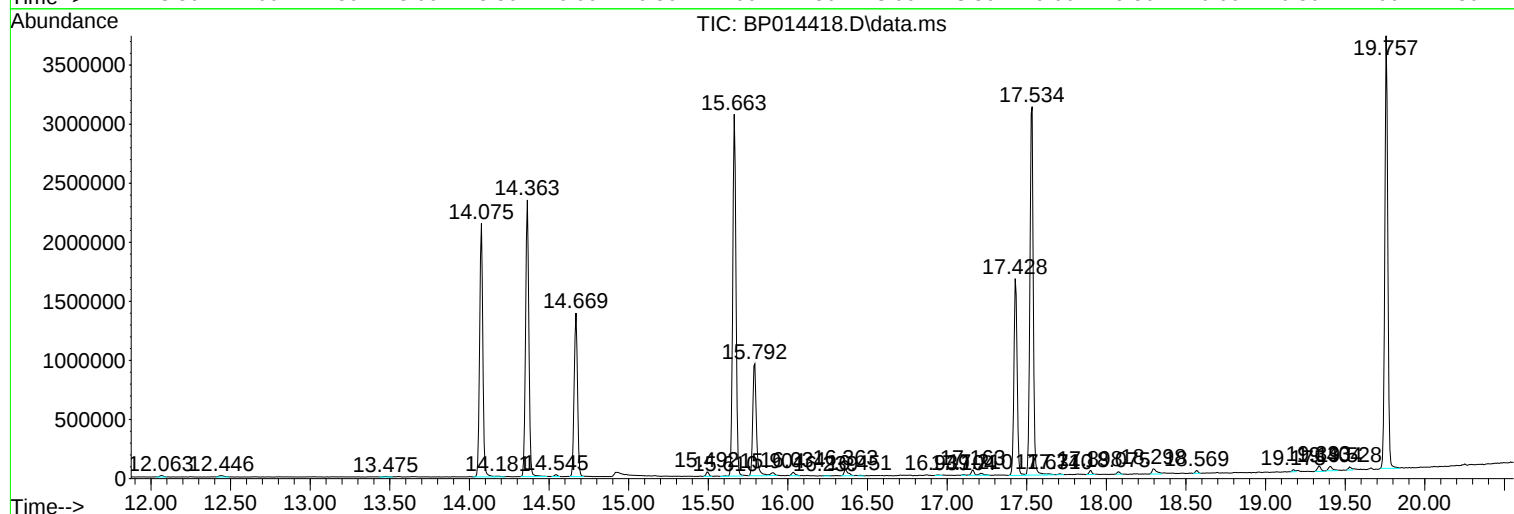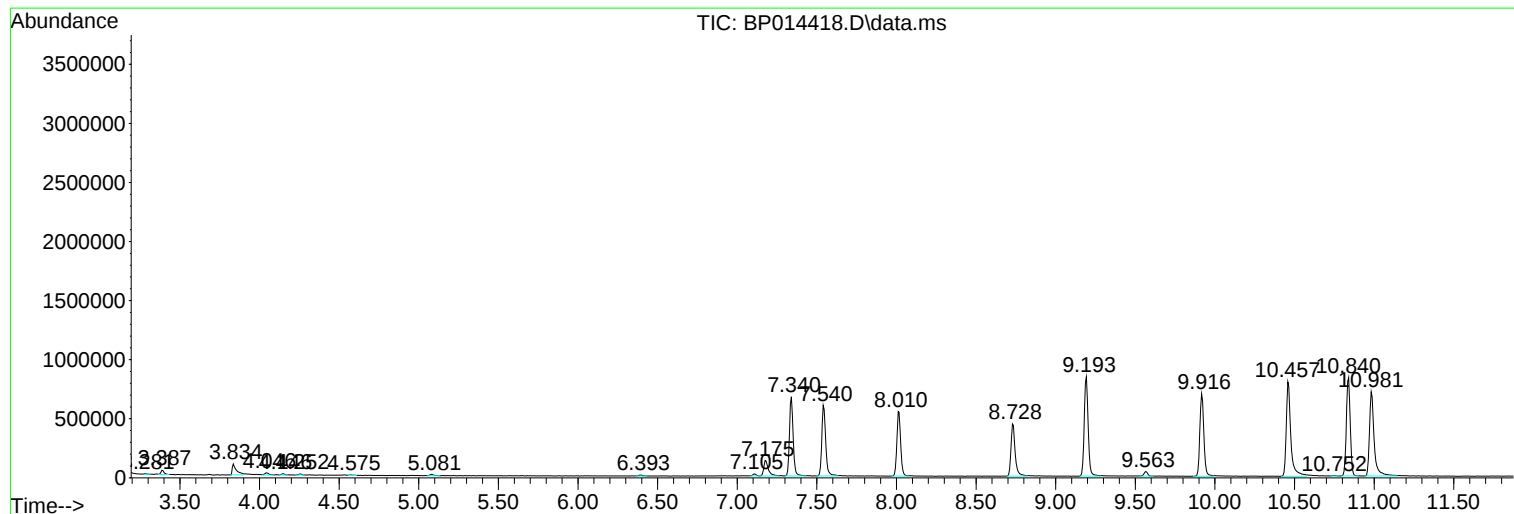

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014418.D
Acq On : 31 Mar 2023 00:17
Operator : CG/JU
Sample : 02038-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014418.D
Acq On : 31 Mar 2023 00:17
Operator : CG/JU
Sample : 02038-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc