

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014424.D
 Acq On : 31 Mar 2023 04:11
 Operator : CG/JU
 Sample : PB151686BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	40	rBV	50936	66775	1.74%	0.154%
2	3.817	104	107	131	rBV	496568	839441	21.88%	1.933%
3	4.146	159	163	169	rVB	13892	19132	0.50%	0.044%
4	6.546	563	571	575	rBV10	2143	4513	0.12%	0.010%
5	6.752	601	606	609	rVB7	2273	4286	0.11%	0.010%
6	7.169	669	677	695	rBV	710781	1245746	32.47%	2.868%
7	7.340	699	706	721	rVB	613829	983165	25.63%	2.263%
8	7.540	732	740	755	rBV	766171	1254214	32.69%	2.887%
9	8.010	814	820	832	rBV	686889	1117834	29.14%	2.573%
10	8.728	935	942	955	rBV	879269	1516123	39.52%	3.490%
11	9.187	1014	1020	1032	rVV	726539	1260112	32.85%	2.901%
12	9.916	1136	1144	1159	rBV	632902	1105290	28.81%	2.545%
13	10.457	1229	1236	1263	rBV	739549	1540400	40.15%	3.546%
14	10.834	1292	1300	1311	rBV	959242	1637703	42.69%	3.770%
15	10.981	1318	1325	1347	rBV	460189	1016580	26.50%	2.340%
16	12.440	1569	1573	1583	rBV6	10097	24777	0.65%	0.057%
17	13.463	1742	1747	1750	rBV7	2147	3853	0.10%	0.009%
18	14.075	1844	1851	1865	rBV	1485741	2253818	58.75%	5.189%
19	14.363	1891	1900	1912	rBV	1749652	2597155	67.70%	5.979%
20	14.669	1945	1952	1967	rBV	1414211	2096589	54.65%	4.827%
21	14.887	1983	1989	2014	rBV	255079	846558	22.07%	1.949%
22	15.663	2114	2121	2129	rBV	2225676	3139925	81.85%	7.229%
23	15.786	2136	2142	2157	rBV	709120	1110399	28.94%	2.556%
24	15.910	2159	2163	2167	rVB6	11677	18953	0.49%	0.044%
25	16.233	2215	2218	2222	rVB6	3575	5264	0.14%	0.012%
26	16.445	2250	2254	2261	rBV10	3224	5543	0.14%	0.013%
27	17.104	2363	2366	2371	rVB7	3565	5471	0.14%	0.013%
28	17.216	2382	2385	2392	rBV6	4069	6440	0.17%	0.015%
29	17.428	2414	2421	2428	rBV	1553691	2256842	58.83%	5.196%
30	17.528	2432	2438	2454	rVV	2089966	3202588	83.48%	7.373%
31	17.857	2488	2494	2497	rBV8	2929	4505	0.12%	0.010%
32	19.339	2742	2746	2753	rBV3	27123	35857	0.93%	0.083%
33	19.404	2753	2757	2761	rBV	25608	41148	1.07%	0.095%
34	19.757	2811	2817	2827	rBV	2614765	3562569	92.86%	8.202%
35	21.516	3111	3116	3128	rBV	1627278	2311006	60.24%	5.320%
36	23.868	3509	3516	3531	rVB2	1905086	3836324	100.00%	8.832%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014424.D
Acq On : 31 Mar 2023 04:11
Operator : CG/JU
Sample : PB151686BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK686

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	24.033	3537	3544	3560	rVB2	1133320	2460254	64.13%	5.664%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 43437152

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014424.D
Acq On : 31 Mar 2023 04:11
Operator : CG/JU
Sample : PB151686BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

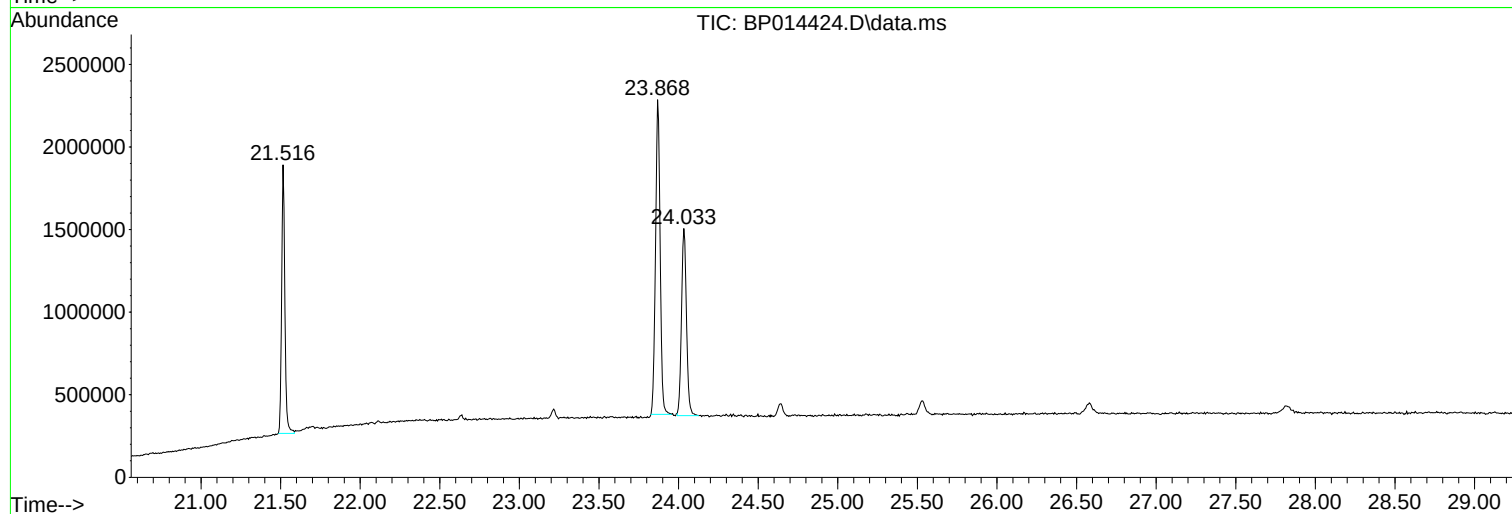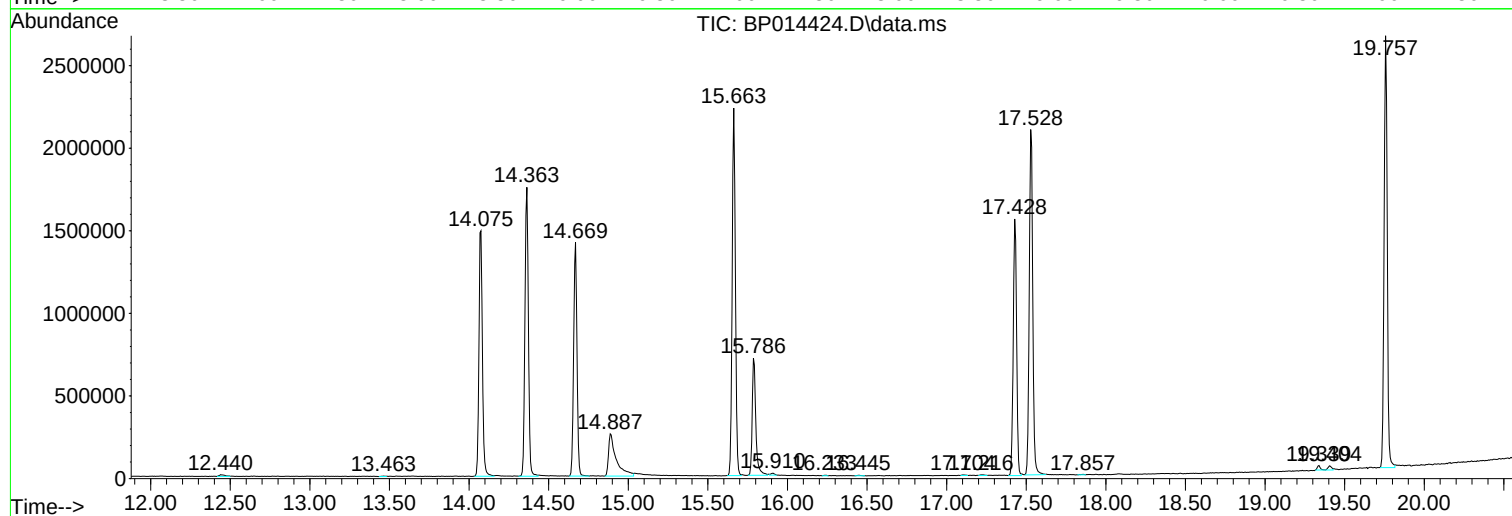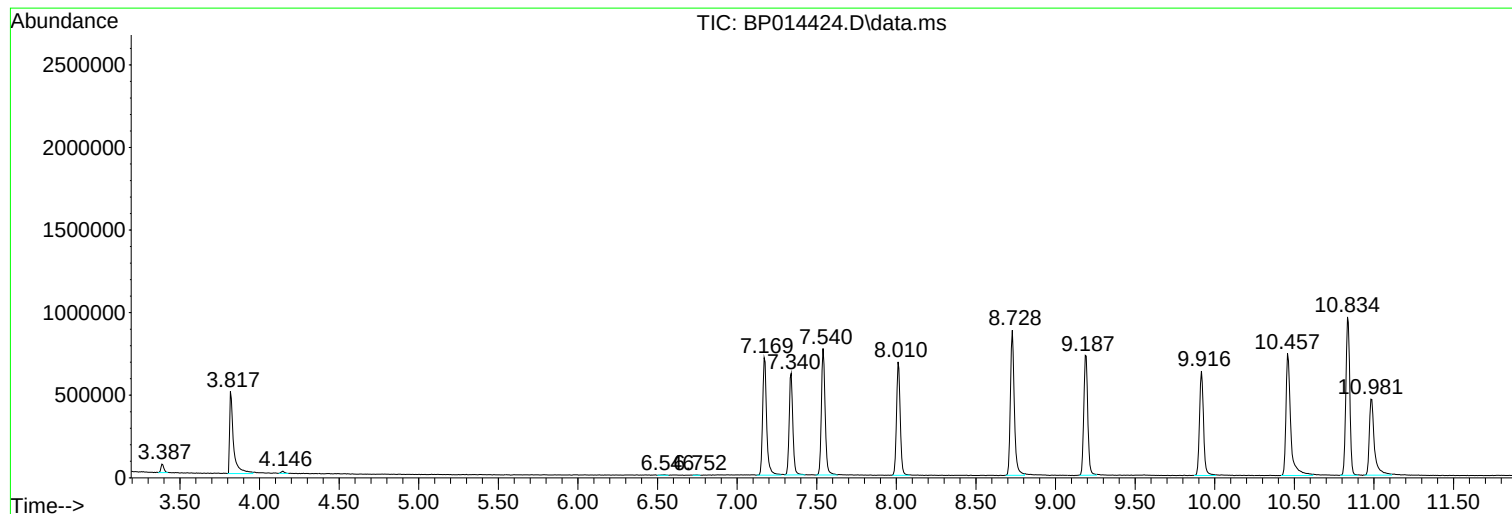

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014424.D
Acq On : 31 Mar 2023 04:11
Operator : CG/JU
Sample : PB151686BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014424.D
Acq On : 31 Mar 2023 04:11
Operator : CG/JU
Sample : PB151686BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc