

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014425.D
 Acq On : 31 Mar 2023 04:44
 Operator : CG/JU
 Sample : PB151687BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	39	rBV	52879	66345	1.70%	0.142%
2	3.816	104	107	126	rBV	550917	891236	22.82%	1.912%
3	4.146	159	163	168	rVB	11159	16984	0.43%	0.036%
4	7.169	671	677	696	rBV	766729	1333358	34.14%	2.860%
5	7.340	699	706	720	rVB	671978	1052541	26.95%	2.258%
6	7.540	731	740	763	rBV	829689	1343842	34.40%	2.882%
7	8.010	814	820	830	rBV	671156	1101051	28.19%	2.362%
8	8.728	935	942	962	rBV	970950	1688492	43.23%	3.622%
9	8.851	962	963	969	rVB6	3490	4960	0.13%	0.011%
10	9.193	1012	1021	1038	rBV	807429	1400319	35.85%	3.004%
11	9.916	1137	1144	1162	rBV	719262	1228629	31.46%	2.635%
12	10.457	1227	1236	1253	rBV	847287	1685194	43.14%	3.615%
13	10.834	1292	1300	1310	rBV	968039	1667440	42.69%	3.577%
14	10.981	1319	1325	1343	rBV	545714	1159354	29.68%	2.487%
15	12.445	1566	1574	1580	rBV4	12429	30310	0.78%	0.065%
16	13.557	1758	1763	1769	rVB8	3581	7691	0.20%	0.016%
17	14.075	1843	1851	1867	rBV	1885918	2664362	68.21%	5.715%
18	14.175	1867	1868	1875	rVB7	3493	5356	0.14%	0.011%
19	14.363	1892	1900	1915	rBV	2025010	2997306	76.74%	6.429%
20	14.669	1944	1952	1962	rBV	1512018	2214185	56.69%	4.749%
21	14.886	1979	1989	2013	rBV	323389	961879	24.63%	2.063%
22	15.663	2114	2121	2136	rBV	2554208	3679904	94.21%	7.893%
23	15.786	2136	2142	2159	rVV	837807	1342640	34.37%	2.880%
24	15.910	2159	2163	2172	rVB5	16063	30763	0.79%	0.066%
25	17.110	2361	2367	2369	rBV7	3594	5801	0.15%	0.012%
26	17.222	2382	2386	2393	rVB8	4815	8893	0.23%	0.019%
27	17.427	2414	2421	2432	rBV	1755889	2408458	61.66%	5.166%
28	17.527	2432	2438	2458	rVB	2500341	3698464	94.69%	7.933%
29	19.339	2742	2746	2752	rBV2	27542	40172	1.03%	0.086%
30	19.410	2754	2758	2762	rBV	27580	37972	0.97%	0.081%
31	19.757	2811	2817	2830	rBV	2758907	3905979	100.00%	8.378%
32	21.515	3111	3116	3128	rBV	1461516	2165960	55.45%	4.646%
33	23.868	3509	3516	3528	rBV2	1775549	3668688	93.92%	7.869%
34	24.033	3538	3544	3554	rVB2	969670	2106302	53.93%	4.518%

Sum of corrected areas: 46620830

Instrument :

BNA_P

ClientSampleId :




SBLK687

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014425.D
Acq On : 31 Mar 2023 04:44
Operator : CG/JU
Sample : PB151687BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

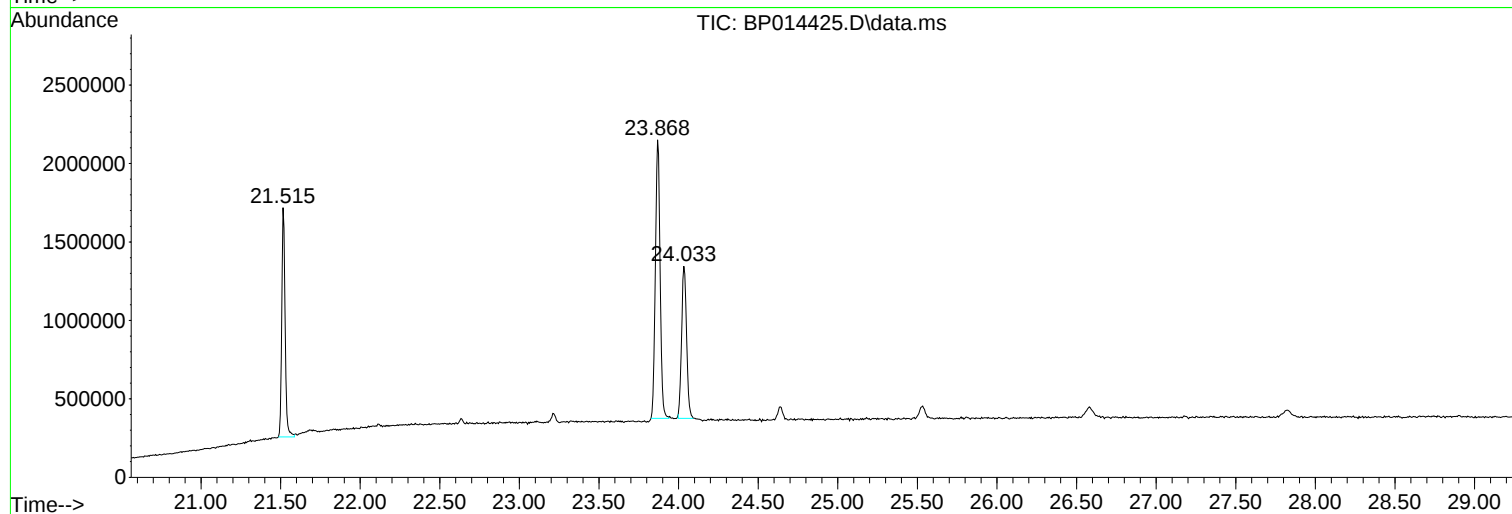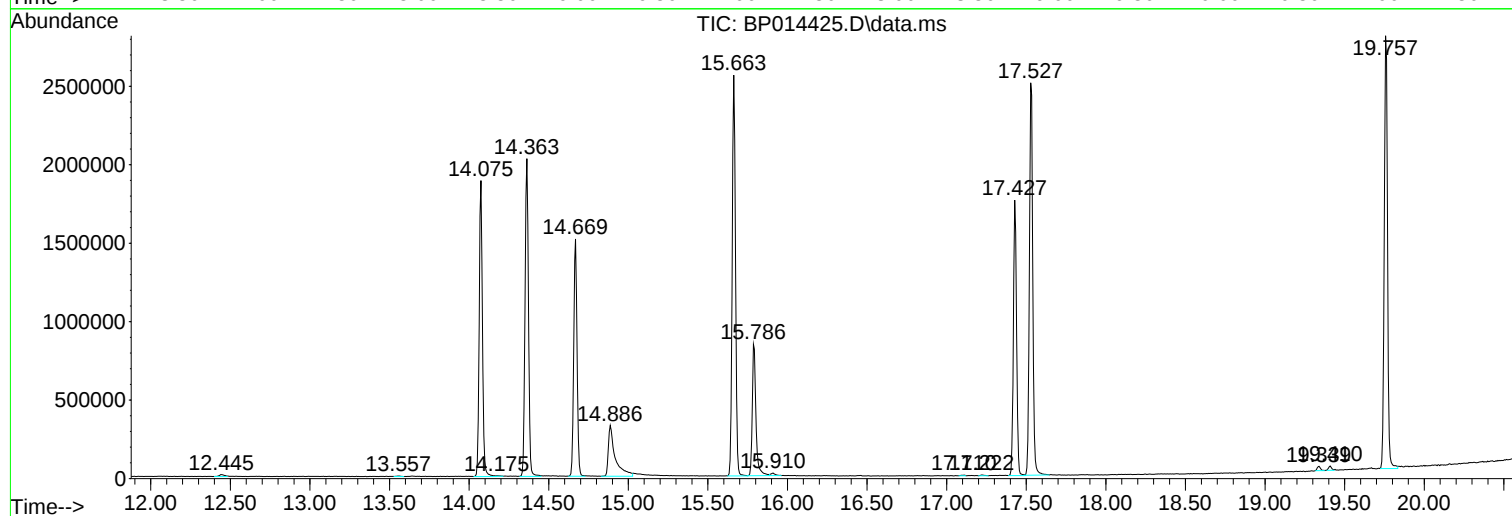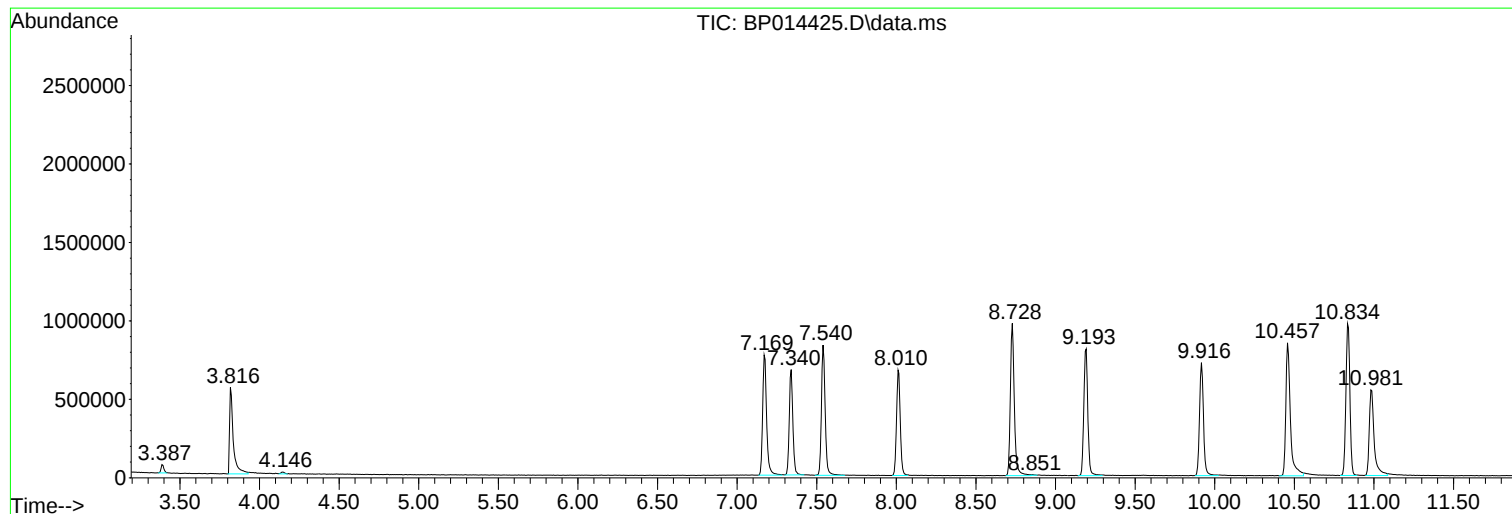

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014425.D
Acq On : 31 Mar 2023 04:44
Operator : CG/JU
Sample : PB151687BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014425.D
Acq On : 31 Mar 2023 04:44
Operator : CG/JU
Sample : PB151687BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc