

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014430.D
 Acq On : 31 Mar 2023 07:32
 Operator : CG/JU
 Sample : 02041-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	31	34	46	rVB	46181	66182	1.30%	0.130%
2	3.822	107	108	121	rBV	211997	342850	6.76%	0.672%
3	4.046	141	146	152	rVB	15484	26587	0.52%	0.052%
4	4.146	158	163	172	rVB2	14356	22172	0.44%	0.043%
5	4.252	177	181	185	rBV5	10199	15299	0.30%	0.030%
6	4.534	223	229	235	rBV10	3784	10738	0.21%	0.021%
7	4.575	235	236	240	rVB2	5996	5094	0.10%	0.010%
8	5.075	318	321	330	rBV2	14758	23012	0.45%	0.045%
9	6.393	540	545	551	rVB3	10075	15599	0.31%	0.031%
10	7.105	660	666	671	rVB7	4584	8959	0.18%	0.018%
11	7.175	671	678	693	rBV	161832	309475	6.10%	0.606%
12	7.334	699	705	719	rBV	746937	1210368	23.86%	2.371%
13	7.540	733	740	751	rBV	704934	1143983	22.55%	2.241%
14	8.010	814	820	831	rBV	684890	1104575	21.78%	2.164%
15	8.728	935	942	957	rBV	538680	955455	18.84%	1.871%
16	9.128	1004	1010	1013	rBV7	4148	8277	0.16%	0.016%
17	9.187	1013	1020	1034	rBV	960280	1627815	32.09%	3.188%
18	9.563	1077	1084	1091	rVB2	20324	32083	0.63%	0.063%
19	9.916	1135	1144	1156	rBV	802436	1370855	27.03%	2.685%
20	10.457	1229	1236	1263	rBV	968348	1858940	36.65%	3.641%
21	10.834	1292	1300	1309	rBV	995018	1685992	33.24%	3.302%
22	10.981	1317	1325	1353	rBV	841765	1707650	33.67%	3.345%
23	12.063	1504	1509	1516	rVB3	13528	21770	0.43%	0.043%
24	12.240	1535	1539	1544	rBV4	6991	9546	0.19%	0.019%
25	12.434	1564	1572	1584	rVB2	15441	35990	0.71%	0.070%
26	13.469	1743	1748	1755	rBV2	16123	24995	0.49%	0.049%
27	13.551	1755	1762	1766	rVV7	8613	14521	0.29%	0.028%
28	13.645	1773	1778	1785	rBV7	3570	6438	0.13%	0.013%
29	14.075	1843	1851	1864	rBV	2373130	3381205	66.66%	6.623%
30	14.363	1893	1900	1909	rBV	2505650	3658768	72.14%	7.166%
31	14.539	1927	1930	1935	rVB7	4909	6650	0.13%	0.013%
32	14.669	1945	1952	1959	rBV	1561123	2305368	45.45%	4.515%
33	14.922	1989	1995	2010	rBV5	41826	173830	3.43%	0.340%
34	15.069	2018	2020	2024	rVB5	5728	6406	0.13%	0.013%
35	15.492	2089	2092	2096	rVB6	4190	5721	0.11%	0.011%
36	15.610	2108	2112	2114	rBV5	6037	7612	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014430.D
 Acq On : 31 Mar 2023 07:32
 Operator : CG/JU
 Sample : 02041-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.663	2114	2121	2129	rBV	3220715	4686635	92.40%	9.180%
38	15.786	2136	2142	2155	rBV	851921	1326828	26.16%	2.599%
39	15.910	2159	2163	2170	rVB2	18788	32368	0.64%	0.063%
40	16.028	2178	2183	2193	rBV	108813	166139	3.28%	0.325%
41	16.451	2253	2255	2261	rVB7	3474	5120	0.10%	0.010%
42	17.104	2362	2366	2372	rBV9	6131	9183	0.18%	0.018%
43	17.280	2393	2396	2400	rBV6	4197	6317	0.12%	0.012%
44	17.428	2415	2421	2432	rBV	1779356	2575903	50.79%	5.045%
45	17.528	2432	2438	2454	rVV2	3290289	4838943	95.40%	9.478%
46	17.933	2503	2507	2510	rBV6	5114	7642	0.15%	0.015%
47	18.080	2528	2532	2535	rBV6	5793	8868	0.17%	0.017%
48	18.292	2563	2568	2577	rBV2	78966	153322	3.02%	0.300%
49	19.333	2741	2745	2751	rBV3	46265	64932	1.28%	0.127%
50	19.410	2753	2758	2765	rVV	41127	73912	1.46%	0.145%
51	19.522	2774	2777	2787	rBV7	38408	74699	1.47%	0.146%
52	19.757	2811	2817	2828	rBV	3847388	5072027	100.00%	9.934%
53	21.198	3059	3062	3071	rBV5	65455	121844	2.40%	0.239%
54	21.516	3111	3116	3126	rBV	1507579	2173345	42.85%	4.257%
55	23.874	3509	3517	3527	rBV	2147164	4373627	86.23%	8.567%
56	24.033	3538	3544	3555	rVB2	973955	2072302	40.86%	4.059%




Sum of corrected areas: 51054736

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014430.D
Acq On : 31 Mar 2023 07:32
Operator : CG/JU
Sample : 02041-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

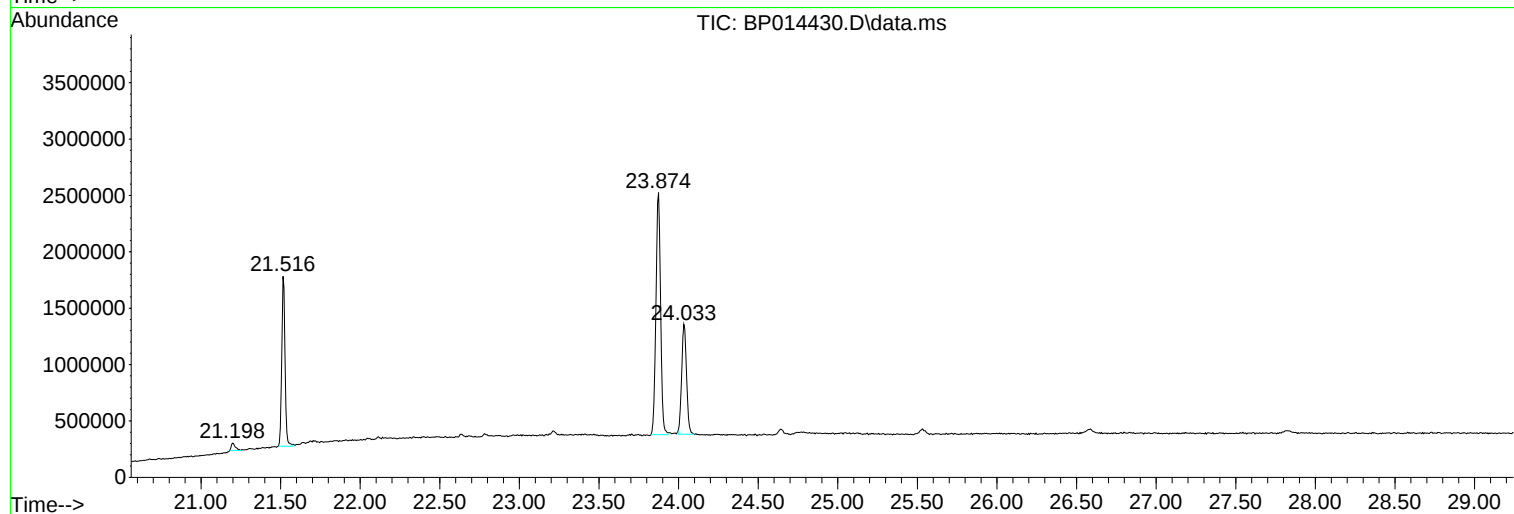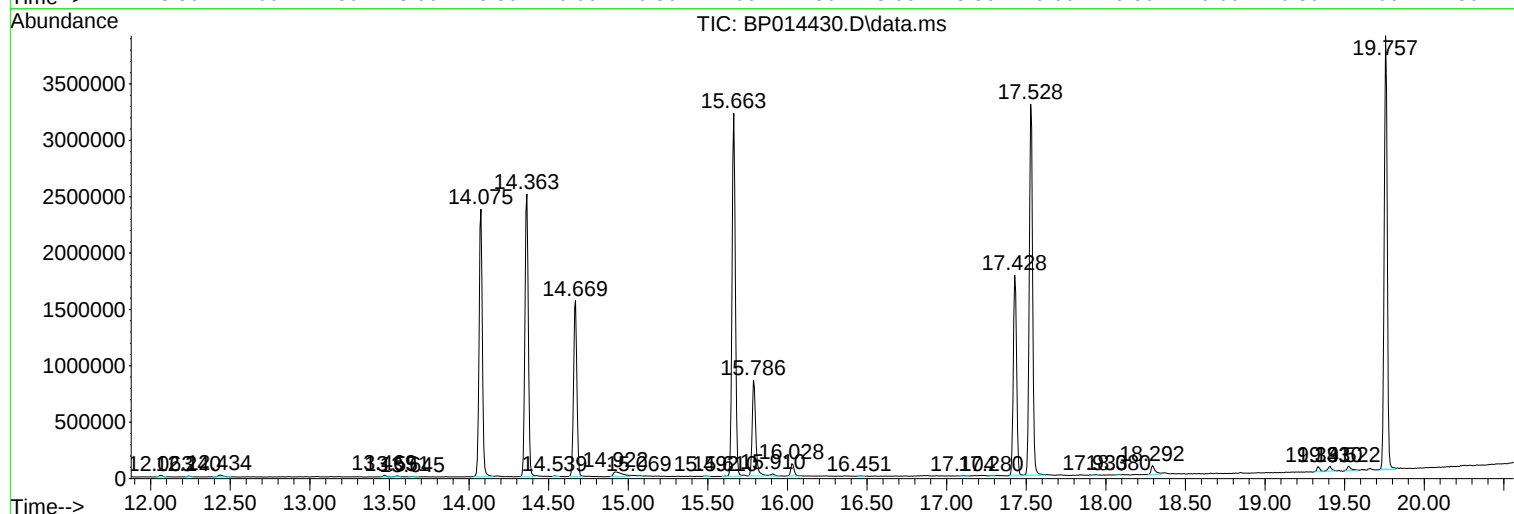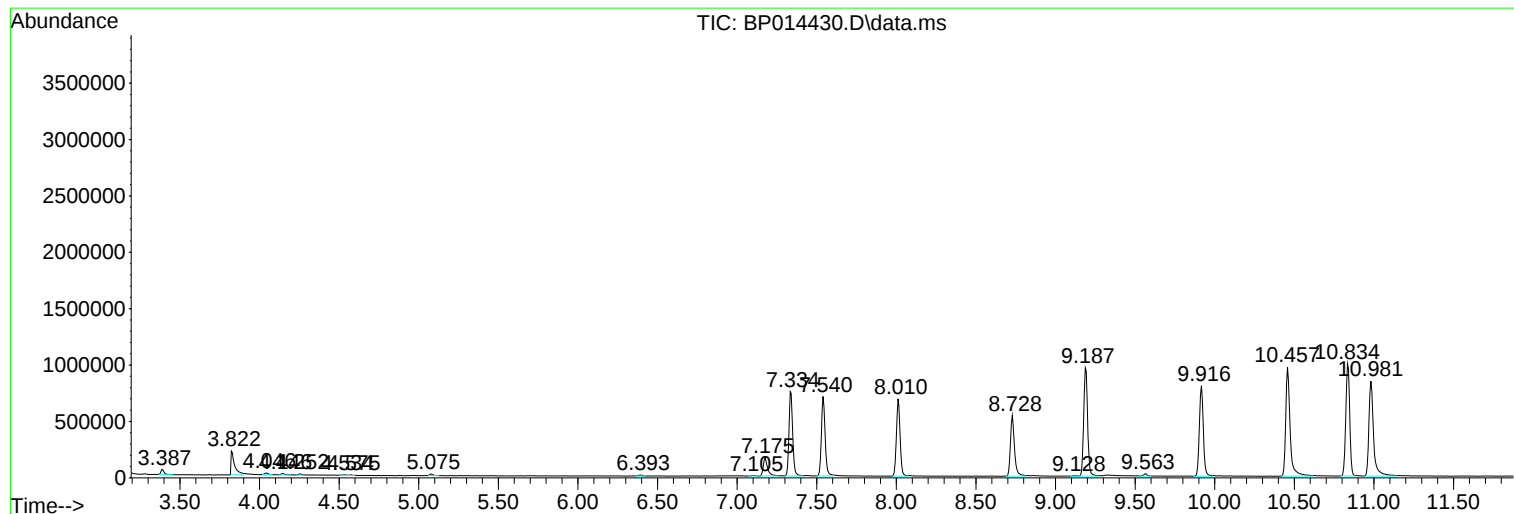

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014430.D
Acq On : 31 Mar 2023 07:32
Operator : CG/JU
Sample : 02041-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014430.D
Acq On : 31 Mar 2023 07:32
Operator : CG/JU
Sample : 02041-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc