

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014435.D
 Acq On : 31 Mar 2023 10:19
 Operator : CG/JU
 Sample : 02059-02DL2 25X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.857	112	114	121	rBV8	1980	4118	0.10%	0.020%
2	4.146	159	163	169	rVB2	14535	19890	0.49%	0.098%
3	5.493	389	392	396	rVB6	2971	4214	0.10%	0.021%
4	5.622	410	414	422	rBV5	5721	13242	0.33%	0.065%
5	5.998	469	478	485	rBV7	7750	16733	0.42%	0.082%
6	6.981	640	645	649	rVB8	3164	7045	0.17%	0.035%
7	7.087	658	663	667	rBV3	7861	12377	0.31%	0.061%
8	7.216	681	685	695	rVB4	11633	22735	0.56%	0.112%
9	7.345	702	707	711	rBV	25857	42851	1.06%	0.210%
10	7.387	711	714	724	rVB4	7617	17151	0.43%	0.084%
11	7.551	735	742	747	rBV2	22328	43379	1.08%	0.213%
12	7.651	754	759	765	rVB	38894	61809	1.53%	0.303%
13	7.740	769	774	780	rVB9	3391	6497	0.16%	0.032%
14	8.010	814	820	834	rBV	675017	1128800	28.02%	5.537%
15	8.122	834	839	847	rVV	26400	48010	1.19%	0.236%
16	8.387	878	884	890	rVB2	14061	26289	0.65%	0.129%
17	8.557	907	913	924	rVV2	30297	55894	1.39%	0.274%
18	8.651	924	929	936	rVV2	12356	21919	0.54%	0.108%
19	8.745	942	945	947	rBV4	7789	9716	0.24%	0.048%
20	8.892	967	970	976	rVB8	3211	5559	0.14%	0.027%
21	8.969	976	983	986	rVV2	7154	11656	0.29%	0.057%
22	9.022	988	992	1000	rVB	7693	13093	0.32%	0.064%
23	9.122	1005	1009	1017	rVB2	12177	19106	0.47%	0.094%
24	9.204	1017	1023	1033	rBV2	31511	73315	1.82%	0.360%
25	9.363	1044	1050	1052	rBV7	3590	6119	0.15%	0.030%
26	9.457	1060	1066	1071	rBV6	5527	9261	0.23%	0.045%
27	9.522	1074	1077	1081	rVB6	3030	4209	0.10%	0.021%
28	9.645	1093	1098	1103	rBV	10863	16980	0.42%	0.083%
29	9.710	1103	1109	1115	rVB	14135	23688	0.59%	0.116%
30	9.928	1140	1146	1155	rBV4	19694	48954	1.22%	0.240%
31	10.016	1157	1161	1166	rVV7	4043	6655	0.17%	0.033%
32	10.081	1166	1172	1178	rVV5	7691	14357	0.36%	0.070%
33	10.228	1190	1197	1204	rBV5	20315	38927	0.97%	0.191%
34	10.357	1215	1219	1223	rVB7	2996	5213	0.13%	0.026%
35	10.463	1233	1237	1239	rBV3	7608	12153	0.30%	0.060%
36	10.504	1239	1244	1247	rVV6	10097	23360	0.58%	0.115%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014435.D
 Acq On : 31 Mar 2023 10:19
 Operator : CG/JU
 Sample : 02059-02DL2 25X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	10.834	1288	1300	1305	rBV	1009456	1757782	43.63%	8.623%
38	10.886	1305	1309	1320	rVB	499338	845389	20.98%	4.147%
39	11.010	1326	1330	1340	rVB6	14477	34899	0.87%	0.171%
40	11.304	1377	1380	1386	rVB8	3781	6436	0.16%	0.032%
41	11.416	1395	1399	1401	rBV5	2749	4197	0.10%	0.021%
42	11.745	1450	1455	1456	rBV5	2736	4127	0.10%	0.020%
43	11.951	1484	1490	1495	rBV10	3461	8139	0.20%	0.040%
44	12.398	1560	1566	1569	rBV7	3366	5697	0.14%	0.028%
45	12.498	1576	1583	1594	rBV	69310	130861	3.25%	0.642%
46	12.716	1608	1620	1629	rBV	68036	127829	3.17%	0.627%
47	12.933	1649	1657	1662	rBV	2485	6752	0.17%	0.033%
48	13.510	1749	1755	1759	rVV2	17411	31855	0.79%	0.156%
49	13.545	1759	1761	1768	rVB7	5521	8780	0.22%	0.043%
50	13.722	1783	1791	1797	rVB6	8999	27879	0.69%	0.137%
51	13.845	1804	1812	1822	rBV5	14559	45776	1.14%	0.225%
52	13.986	1829	1836	1842	rBV3	29852	57273	1.42%	0.281%
53	14.039	1842	1845	1847	rVV2	20549	27168	0.67%	0.133%
54	14.075	1847	1851	1863	rVB	94111	161115	4.00%	0.790%
55	14.222	1870	1876	1880	rBV3	15752	26701	0.66%	0.131%
56	14.363	1894	1900	1909	rBV	101638	183344	4.55%	0.899%
57	14.545	1927	1931	1937	rVB9	3433	6000	0.15%	0.029%
58	14.669	1939	1952	1960	rBV	1693585	2570837	63.81%	12.611%
59	14.875	1982	1987	1995	rVB9	5723	13605	0.34%	0.067%
60	14.963	1998	2002	2003	rBV4	3847	4220	0.10%	0.021%
61	15.069	2013	2020	2027	rBV4	10171	22789	0.57%	0.112%
62	15.139	2027	2032	2038	rVB9	7993	15189	0.38%	0.075%
63	15.227	2042	2047	2053	rBV8	8826	17732	0.44%	0.087%
64	15.304	2053	2060	2071	rBV	100064	200637	4.98%	0.984%
65	15.439	2080	2083	2085	rBV4	4593	6009	0.15%	0.029%
66	15.486	2089	2091	2097	rVB7	6710	10452	0.26%	0.051%
67	15.663	2116	2121	2127	rVV	145943	226281	5.62%	1.110%
68	15.716	2128	2130	2135	rVB3	10656	15546	0.39%	0.076%
69	15.804	2141	2145	2151	rBV4	18218	37896	0.94%	0.186%
70	15.845	2151	2152	2155	rVV3	10904	11215	0.28%	0.055%
71	15.874	2155	2157	2162	rVB5	8343	11091	0.28%	0.054%
72	16.016	2178	2181	2191	rVB5	6317	12987	0.32%	0.064%
73	16.374	2235	2242	2243	rBV7	5025	9204	0.23%	0.045%
74	16.480	2257	2260	2262	rBV4	5128	5676	0.14%	0.028%
75	16.716	2292	2300	2301	rBV7	7833	15498	0.38%	0.076%
76	16.780	2306	2311	2317	rVV7	6919	13463	0.33%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014435.D
 Acq On : 31 Mar 2023 10:19
 Operator : CG/JU
 Sample : 02059-02DL2 25X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG1DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	17.074	2354	2361	2382	rBV	2534364	4029074	100.00%	19.765%
78	17.427	2413	2421	2427	rBV	2053367	2935180	72.85%	14.399%
79	17.527	2433	2438	2453	rVB2	155022	250402	6.21%	1.228%
80	18.033	2522	2524	2529	rVB6	9842	11175	0.28%	0.055%
81	18.468	2596	2598	2603	rBV6	7559	10911	0.27%	0.054%
82	19.757	2813	2817	2822	rBV	171643	231814	5.75%	1.137%
83	21.515	3111	3116	3126	rBV	1639486	2293781	56.93%	11.252%
84	24.033	3537	3544	3557	rVB2	929742	1999379	49.62%	9.808%




Sum of corrected areas: 20385316

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014435.D
Acq On : 31 Mar 2023 10:19
Operator : CG/JU
Sample : 02059-02DL2 25X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG1DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

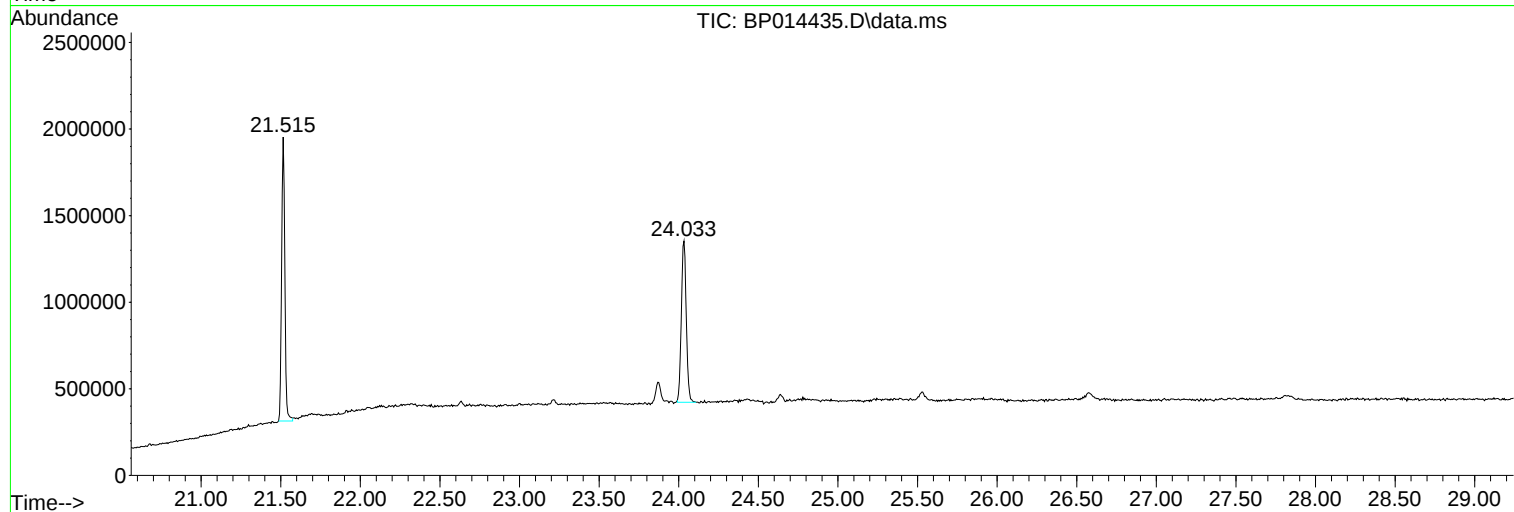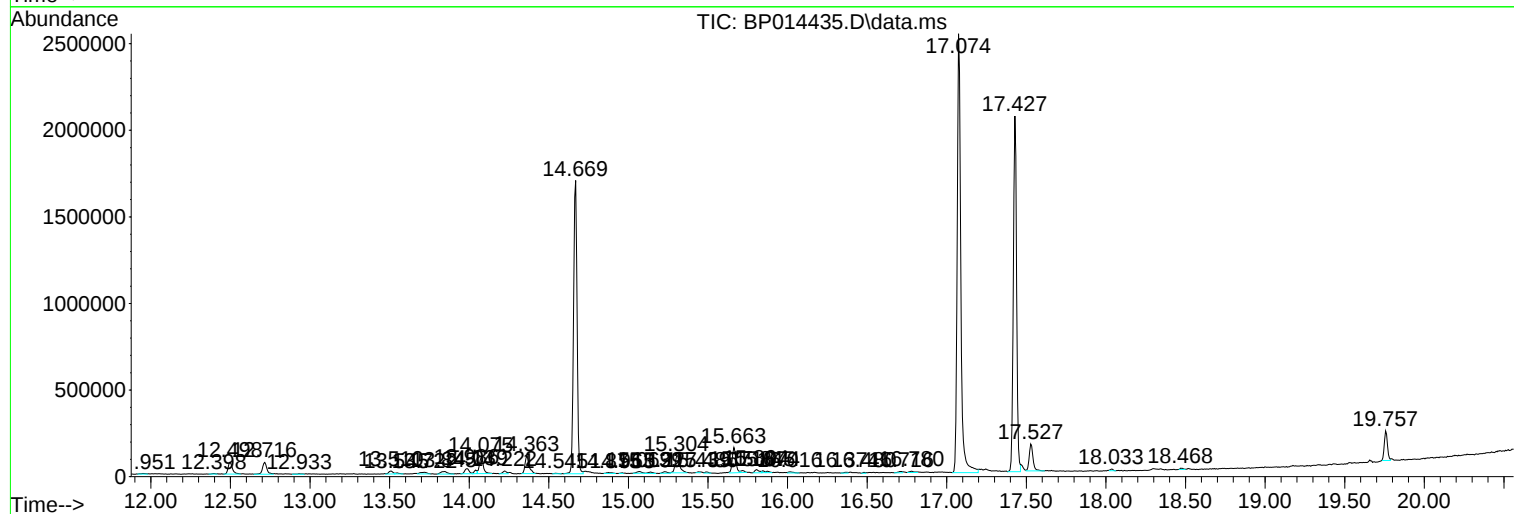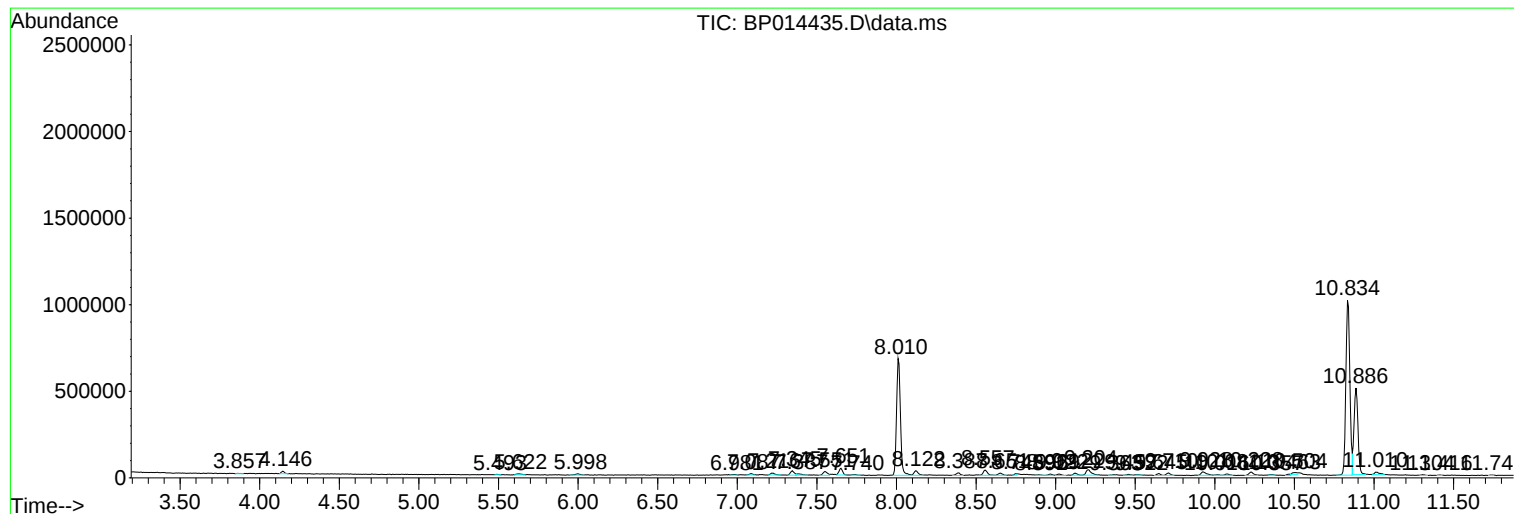

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014435.D
Acq On : 31 Mar 2023 10:19
Operator : CG/JU
Sample : 02059-02DL2 25X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG1DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014435.D
Acq On : 31 Mar 2023 10:19
Operator : CG/JU
Sample : 02059-02DL2 25X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG1DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc