

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014436.D
 Acq On : 31 Mar 2023 10:53
 Operator : CG/JU
 Sample : 02059-03DL2 25X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG5DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.146	159	163	172	rVB2	13388	19004	0.57%	0.099%
2	4.358	195	199	201	rBV5	2341	3546	0.11%	0.018%
3	5.487	387	391	395	rVB7	2687	4254	0.13%	0.022%
4	5.622	410	414	420	rBV3	5707	11211	0.34%	0.058%
5	5.993	472	477	482	rBV5	6006	9686	0.29%	0.050%
6	6.052	482	487	491	rBV3	9161	15122	0.46%	0.079%
7	6.475	555	559	562	rBV6	2940	3679	0.11%	0.019%
8	7.087	659	663	668	rBV6	6715	11176	0.34%	0.058%
9	7.222	678	686	690	rBV4	10901	20619	0.62%	0.107%
10	7.346	702	707	712	rBV	22436	39362	1.19%	0.204%
11	7.387	712	714	720	rVB5	7535	11478	0.35%	0.060%
12	7.552	737	742	749	rBV	19820	42396	1.28%	0.220%
13	7.652	754	759	765	rVV	34791	57130	1.73%	0.297%
14	7.734	768	773	779	rVB9	3680	8408	0.25%	0.044%
15	7.904	796	802	805	rBV8	2650	4063	0.12%	0.021%
16	8.010	813	820	830	rBV	664184	1110241	33.59%	5.765%
17	8.122	834	839	847	rVB	21643	39814	1.20%	0.207%
18	8.387	878	884	890	rBV2	13025	22453	0.68%	0.117%
19	8.499	900	903	907	rBV6	2887	4387	0.13%	0.023%
20	8.557	907	913	922	rVV2	25105	48002	1.45%	0.249%
21	8.646	923	928	935	rVB4	10671	19798	0.60%	0.103%
22	8.752	941	946	951	rBV8	9869	23343	0.71%	0.121%
23	8.810	955	956	960	rVB4	3334	4088	0.12%	0.021%
24	8.963	978	982	987	rBV5	6095	10492	0.32%	0.054%
25	9.016	987	991	997	rVB4	7078	11653	0.35%	0.061%
26	9.122	1003	1009	1016	rVB5	11632	23798	0.72%	0.124%
27	9.204	1016	1023	1033	rBV	31612	74912	2.27%	0.389%
28	9.363	1046	1050	1058	rVB	4100	9959	0.30%	0.052%
29	9.463	1060	1067	1071	rBV8	4889	11243	0.34%	0.058%
30	9.522	1071	1077	1079	rVV7	2372	4777	0.14%	0.025%
31	9.651	1094	1099	1103	rBV2	9243	14209	0.43%	0.074%
32	9.704	1103	1108	1113	rVB2	11445	20317	0.61%	0.106%
33	9.881	1133	1138	1140	rBV6	2092	3344	0.10%	0.017%
34	9.928	1140	1146	1154	rVV2	21040	48396	1.46%	0.251%
35	10.022	1157	1162	1166	rVV8	3577	8147	0.25%	0.042%
36	10.075	1166	1171	1182	rVB3	8777	16427	0.50%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014436.D
 Acq On : 31 Mar 2023 10:53
 Operator : CG/JU
 Sample : 02059-03DL2 25X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG5DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	10.228	1190	1197	1206	rBV5	16754	36971	1.12%	0.192%
38	10.346	1212	1217	1221	rBV8	3162	7182	0.22%	0.037%
39	10.404	1225	1227	1232	rVB6	2902	3339	0.10%	0.017%
40	10.463	1232	1237	1239	rBV4	7386	11170	0.34%	0.058%
41	10.504	1239	1244	1249	rBV4	10660	28458	0.86%	0.148%
42	10.834	1292	1300	1305	rBV	1024685	1743112	52.73%	9.052%
43	10.887	1305	1309	1317	rVB	409181	696321	21.06%	3.616%
44	11.022	1326	1332	1343	rBV5	11161	28774	0.87%	0.149%
45	11.298	1376	1379	1385	rVB8	3071	4180	0.13%	0.022%
46	11.404	1392	1397	1405	rBV8	2219	4756	0.14%	0.025%
47	12.051	1504	1507	1512	rVB7	2252	4085	0.12%	0.021%
48	12.245	1533	1540	1544	rVB9	3064	6536	0.20%	0.034%
49	12.498	1577	1583	1597	rVB	55391	107259	3.24%	0.557%
50	12.716	1611	1620	1628	rBV	54138	99809	3.02%	0.518%
51	13.475	1744	1749	1750	rBV5	2737	3837	0.12%	0.020%
52	13.510	1750	1755	1759	rVV3	12537	20823	0.63%	0.108%
53	13.710	1785	1789	1796	rVB7	6676	16296	0.49%	0.085%
54	13.839	1801	1811	1818	rBV7	11436	35108	1.06%	0.182%
55	13.987	1830	1836	1842	rBV2	24129	48529	1.47%	0.252%
56	14.039	1842	1845	1847	rVV2	14697	19404	0.59%	0.101%
57	14.075	1847	1851	1858	rVB	81133	130728	3.95%	0.679%
58	14.222	1871	1876	1886	rVB3	13839	30347	0.92%	0.158%
59	14.363	1894	1900	1909	rBV	91790	167319	5.06%	0.869%
60	14.545	1927	1931	1934	rBV6	7019	9228	0.28%	0.048%
61	14.669	1942	1952	1960	rBV	1610336	2460863	74.45%	12.779%
62	14.728	1960	1962	1971	rVB9	9248	20583	0.62%	0.107%
63	14.892	1982	1990	1996	rBV10	6478	15928	0.48%	0.083%
64	15.075	2014	2021	2026	rBV6	9438	19922	0.60%	0.103%
65	15.145	2028	2033	2039	rVB6	7718	14127	0.43%	0.073%
66	15.228	2043	2047	2052	rBV7	7270	14727	0.45%	0.076%
67	15.304	2052	2060	2075	rVV3	81893	183860	5.56%	0.955%
68	15.445	2079	2084	2085	rVV5	5949	8983	0.27%	0.047%
69	15.492	2089	2092	2098	rVB8	7030	11115	0.34%	0.058%
70	15.663	2115	2121	2126	rBV2	128044	193801	5.86%	1.006%
71	15.716	2128	2130	2135	rVB3	10574	14057	0.43%	0.073%
72	15.804	2141	2145	2150	rBV5	15052	29668	0.90%	0.154%
73	15.845	2150	2152	2155	rVV4	3236	4241	0.13%	0.022%
74	16.016	2179	2181	2186	rVB5	4511	6134	0.19%	0.032%
75	16.163	2204	2206	2210	rVB5	4183	4596	0.14%	0.024%
76	16.257	2220	2222	2226	rVB5	3156	4064	0.12%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014436.D
 Acq On : 31 Mar 2023 10:53
 Operator : CG/JU
 Sample : 02059-03DL2 25X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG5DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	16.363	2237	2240	2241	rBV3	6742	8199	0.25%	0.043%
78	16.492	2257	2262	2264	rBV6	3782	6339	0.19%	0.033%
79	16.522	2264	2267	2271	rVV6	2404	4180	0.13%	0.022%
80	16.704	2292	2298	2299	rBV6	7267	10677	0.32%	0.055%
81	16.780	2306	2311	2315	rBV8	6011	10444	0.32%	0.054%
82	16.939	2332	2338	2340	rBV7	4628	8271	0.25%	0.043%
83	16.975	2341	2344	2350	rVB8	2917	5356	0.16%	0.028%
84	17.075	2354	2361	2382	rBV	2152343	3305591	100.00%	17.166%
85	17.428	2414	2421	2427	rBV	1958843	2819150	85.28%	14.640%
86	17.528	2433	2438	2452	rVB	135023	224957	6.81%	1.168%
87	18.033	2521	2524	2528	rVB6	10101	11471	0.35%	0.060%
88	18.304	2565	2570	2575	rBV8	12232	27719	0.84%	0.144%
89	18.469	2596	2598	2604	rBV6	5877	6839	0.21%	0.036%
90	19.174	2716	2718	2723	rVB6	8372	7587	0.23%	0.039%
91	19.416	2756	2759	2764	rBV4	15380	24301	0.74%	0.126%
92	19.657	2796	2800	2805	rVB3	31271	41386	1.25%	0.215%
93	19.757	2813	2817	2823	rBV	176092	240227	7.27%	1.247%
94	21.516	3111	3116	3126	rBV	1744844	2394559	72.44%	12.435%
95	24.033	3537	3544	3556	rVB2	937534	2038348	61.66%	10.585%


Sum of corrected areas: 19256775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014436.D
Acq On : 31 Mar 2023 10:53
Operator : CG/JU
Sample : 02059-03DL2 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

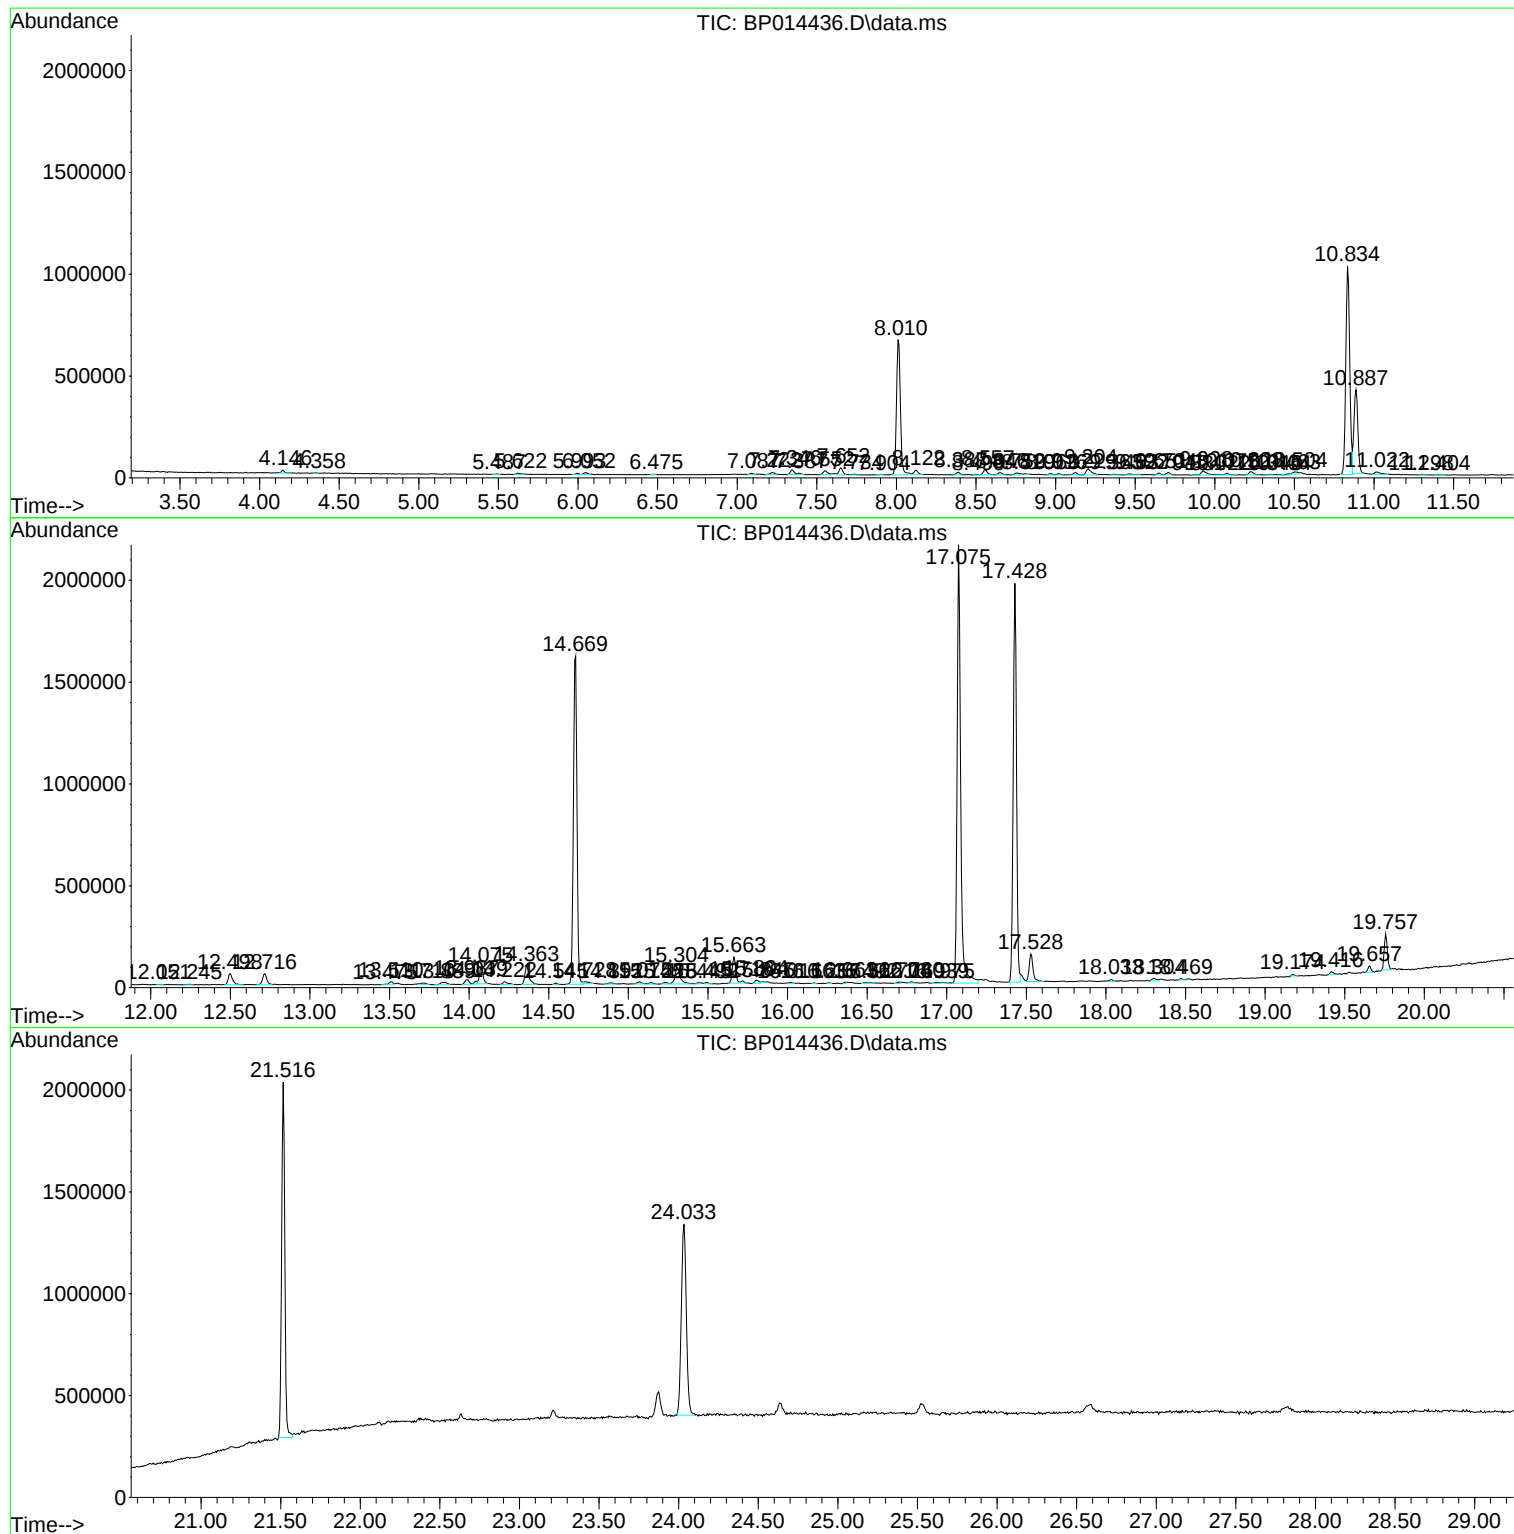

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014436.D
Acq On : 31 Mar 2023 10:53
Operator : CG/JU
Sample : 02059-03DL2 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014436.D
Acq On : 31 Mar 2023 10:53
Operator : CG/JU
Sample : 02059-03DL2 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------