

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.146	159	163	169	rVB2	11555	17081	0.43%	0.089%
2	5.622	408	414	417	rBV7	6690	11232	0.28%	0.059%
3	5.999	471	478	483	rBV5	9130	16744	0.42%	0.087%
4	6.046	483	486	491	rVB6	5272	6925	0.17%	0.036%
5	6.975	635	644	647	rBV6	4032	9765	0.25%	0.051%
6	7.087	659	663	669	rVV3	7836	13244	0.33%	0.069%
7	7.146	669	673	679	rVB9	5159	10161	0.26%	0.053%
8	7.222	679	686	692	rBV2	13267	24188	0.61%	0.126%
9	7.346	702	707	712	rBV2	19724	36318	0.91%	0.190%
10	7.387	712	714	720	rVB4	6306	10094	0.25%	0.053%
11	7.558	735	743	747	rBV3	16843	32586	0.82%	0.170%
12	7.616	749	753	755	rVV3	11602	17862	0.45%	0.093%
13	7.652	755	759	767	rVV	37076	63983	1.61%	0.334%
14	7.728	767	772	778	rVB9	2888	6727	0.17%	0.035%
15	8.010	814	820	833	rBV	583558	978025	24.58%	5.110%
16	8.122	833	839	848	rVV	26117	47974	1.21%	0.251%
17	8.387	878	884	891	rBV3	13043	24260	0.61%	0.127%
18	8.557	908	913	919	rBV3	26255	46518	1.17%	0.243%
19	8.652	925	929	936	rBV3	13433	21430	0.54%	0.112%
20	8.763	940	948	955	rBV10	8119	23367	0.59%	0.122%
21	8.963	978	982	988	rBV5	7296	13366	0.34%	0.070%
22	9.016	988	991	999	rVB2	7128	10227	0.26%	0.053%
23	9.122	1003	1009	1016	rVB2	14533	26072	0.66%	0.136%
24	9.205	1017	1023	1027	rBV3	26429	56063	1.41%	0.293%
25	9.381	1051	1053	1058	rVB6	4070	5903	0.15%	0.031%
26	9.457	1062	1066	1070	rBV5	5912	9964	0.25%	0.052%
27	9.516	1073	1076	1081	rVB7	3163	4803	0.12%	0.025%
28	9.646	1093	1098	1104	rVB	10763	17940	0.45%	0.094%
29	9.710	1104	1109	1114	rVB	15788	24642	0.62%	0.129%
30	9.928	1140	1146	1156	rVV6	16522	43174	1.09%	0.226%
31	10.016	1156	1161	1165	rVV8	3958	8580	0.22%	0.045%
32	10.075	1167	1171	1175	rVV4	7725	12141	0.31%	0.063%
33	10.228	1191	1197	1205	rBV5	19537	36128	0.91%	0.189%
34	10.357	1211	1219	1220	rBV8	4174	6220	0.16%	0.033%
35	10.463	1232	1237	1240	rBV6	6953	11447	0.29%	0.060%
36	10.516	1240	1246	1248	rBV5	10991	23037	0.58%	0.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	10.834	1288	1300	1305	rBV	906786	1576050	39.61%	8.235%
38	10.887	1305	1309	1323	rVV	502542	868548	21.83%	4.538%
39	11.022	1326	1332	1339	rBV7	10337	25760	0.65%	0.135%
40	11.122	1346	1349	1353	rVB6	2668	4163	0.10%	0.022%
41	11.310	1376	1381	1382	rBV5	3374	5245	0.13%	0.027%
42	11.940	1482	1488	1489	rBV6	2895	4398	0.11%	0.023%
43	12.240	1534	1539	1549	rVB6	5442	14358	0.36%	0.075%
44	12.393	1560	1565	1570	rBV9	3215	6972	0.18%	0.036%
45	12.498	1577	1583	1597	rVB	76498	141857	3.57%	0.741%
46	12.716	1610	1620	1632	rBV	72596	137544	3.46%	0.719%
47	13.181	1695	1699	1705	rBV9	2985	6163	0.15%	0.032%
48	13.475	1740	1749	1750	rBV6	7091	12282	0.31%	0.064%
49	13.504	1750	1754	1761	rVB2	16239	27771	0.70%	0.145%
50	13.698	1781	1787	1790	rBV6	9208	18447	0.46%	0.096%
51	13.845	1801	1812	1818	rBV5	19191	55773	1.40%	0.291%
52	13.987	1829	1836	1841	rBV2	35262	67836	1.71%	0.354%
53	14.045	1841	1846	1847	rVV2	21228	27796	0.70%	0.145%
54	14.075	1847	1851	1858	rVB	80751	126719	3.19%	0.662%
55	14.222	1870	1876	1879	rBV2	17988	29793	0.75%	0.156%
56	14.363	1893	1900	1913	rBV	87879	172253	4.33%	0.900%
57	14.540	1926	1930	1934	rBV5	8444	13077	0.33%	0.068%
58	14.663	1940	1951	1959	rBV	1486010	2286707	57.48%	11.948%
59	14.734	1959	1963	1965	rVV4	4767	6959	0.17%	0.036%
60	14.887	1982	1989	1994	rBV5	8513	21595	0.54%	0.113%
61	14.963	1999	2002	2005	rVB5	3672	5464	0.14%	0.029%
62	15.063	2014	2019	2026	rVV4	12007	25269	0.64%	0.132%
63	15.145	2028	2033	2038	rVB4	8919	16661	0.42%	0.087%
64	15.234	2043	2048	2052	rBV7	9123	13454	0.34%	0.070%
65	15.310	2052	2061	2074	rVV3	101141	227711	5.72%	1.190%
66	15.439	2077	2083	2085	rVV6	9119	15280	0.38%	0.080%
67	15.492	2088	2092	2101	rVB5	17610	25959	0.65%	0.136%
68	15.663	2114	2121	2127	rBV	126771	192203	4.83%	1.004%
69	15.710	2127	2129	2134	rVB5	12040	18286	0.46%	0.096%
70	15.804	2141	2145	2149	rBV6	17898	33617	0.84%	0.176%
71	16.004	2173	2179	2180	rBV5	6421	7896	0.20%	0.041%
72	16.157	2202	2205	2206	rBV3	4491	3997	0.10%	0.021%
73	16.239	2214	2219	2220	rBV5	3379	4205	0.11%	0.022%
74	16.257	2220	2222	2227	rVB6	4839	6583	0.17%	0.034%
75	16.363	2236	2240	2242	rBV3	14806	22189	0.56%	0.116%
76	16.486	2258	2261	2265	rBV5	3525	4454	0.11%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	16.528	2265	2268	2272	rVV6	4566	6080	0.15%	0.032%
78	16.704	2294	2298	2300	rBV4	9346	13549	0.34%	0.071%
79	16.781	2307	2311	2315	rBV4	7977	10633	0.27%	0.056%
80	16.875	2322	2327	2332	rVB8	6478	11164	0.28%	0.058%
81	16.934	2333	2337	2339	rBV5	4735	5750	0.14%	0.030%
82	17.075	2355	2361	2373	rBV	2643806	3978463	100.00%	20.788%
83	17.210	2382	2384	2388	rBV5	6327	7786	0.20%	0.041%
84	17.428	2415	2421	2427	rBV	1928763	2677442	67.30%	13.990%
85	17.528	2433	2438	2447	rBV	127287	202029	5.08%	1.056%
86	17.622	2452	2454	2459	rBV6	3941	5918	0.15%	0.031%
87	17.904	2498	2502	2506	rVB7	6948	12049	0.30%	0.063%
88	17.939	2506	2508	2511	rVB4	3877	4598	0.12%	0.024%
89	18.298	2565	2569	2573	rBV4	13248	25001	0.63%	0.131%
90	18.480	2596	2600	2603	rBV4	10282	15196	0.38%	0.079%
91	18.663	2628	2631	2635	rBV5	5856	11007	0.28%	0.058%
92	19.175	2716	2718	2722	rBV5	11862	13276	0.33%	0.069%
93	19.657	2797	2800	2803	rBV5	15535	20967	0.53%	0.110%
94	19.757	2813	2817	2825	rBV	143528	215264	5.41%	1.125%
95	21.516	3111	3116	3126	rBV	1518221	2085145	52.41%	10.895%
96	24.033	3538	3544	3555	rVB2	851635	1807254	45.43%	9.443%




Sum of corrected areas: 19138056

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

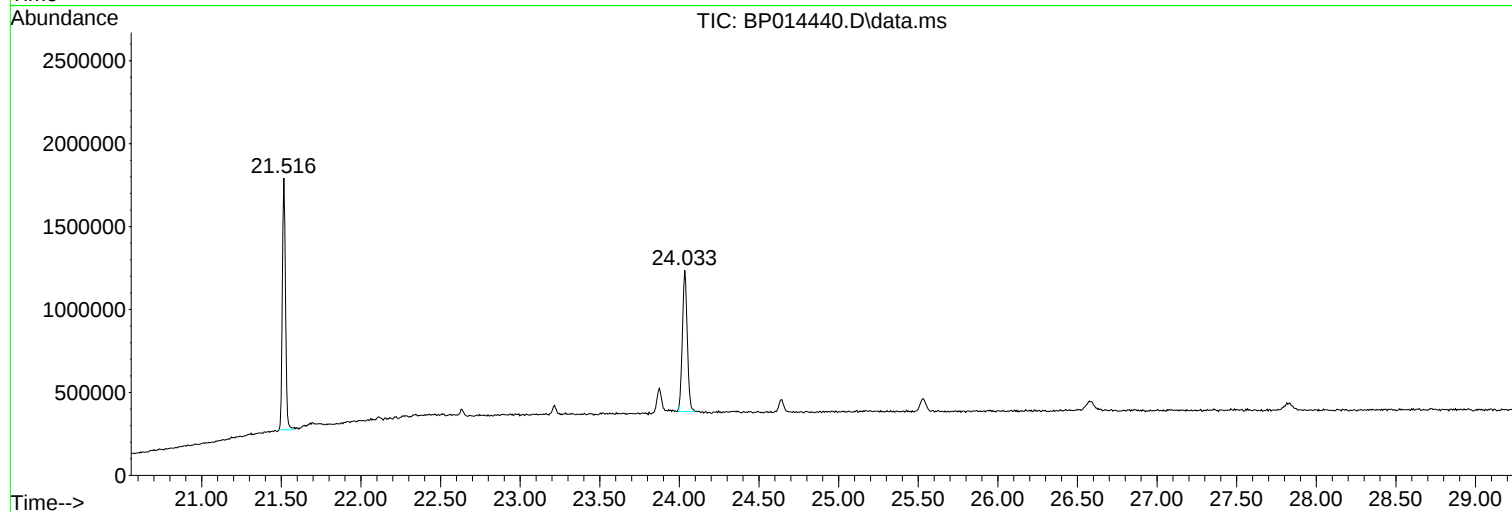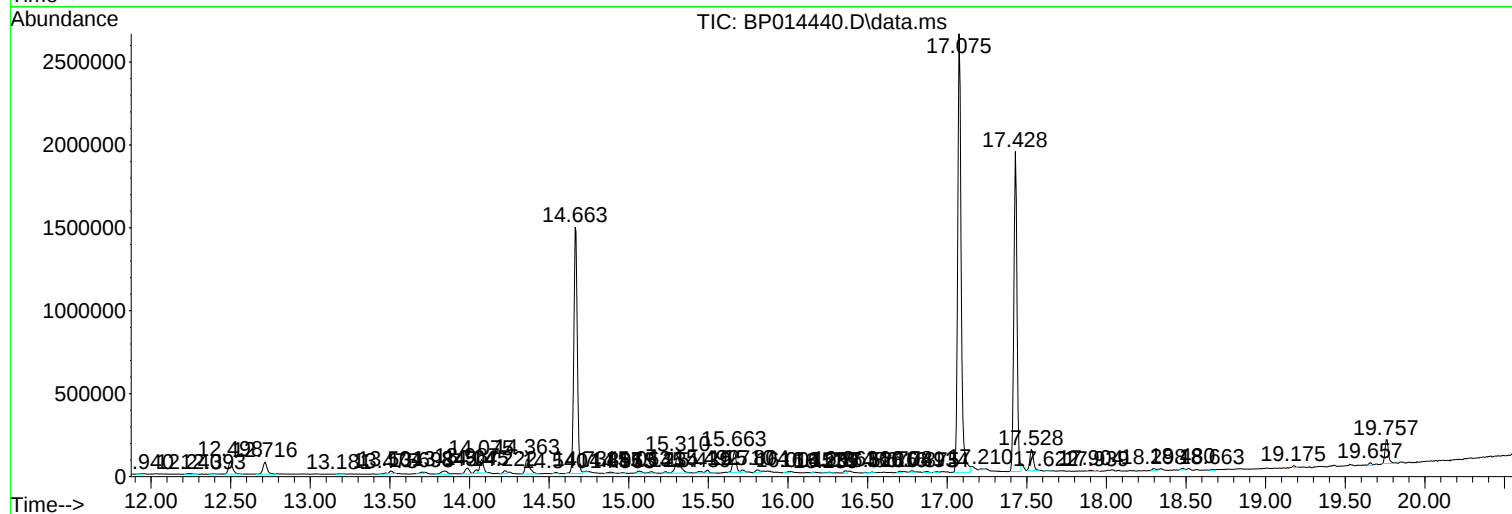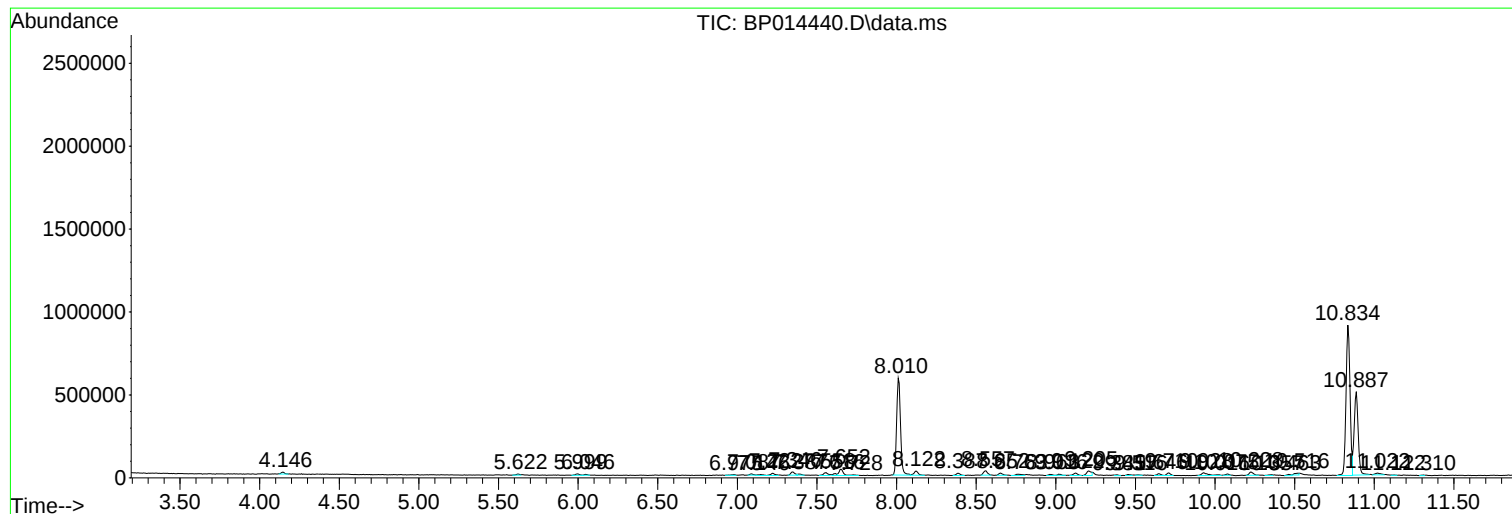

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc