

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014460.D
 Acq On : 01 Apr 2023 00:59
 Operator : CG/JU
 Sample : PB151752BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK752

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	41	rVB	48876	65722	1.19%	0.121%
2	3.828	107	109	130	rBV	188969	350763	6.35%	0.643%
3	4.140	159	162	169	rVB2	12755	20961	0.38%	0.038%
4	7.187	671	680	691	rBV	857408	1494990	27.05%	2.741%
5	7.340	699	706	722	rVB	707637	1102496	19.95%	2.021%
6	7.546	734	741	758	rBV	885004	1474805	26.68%	2.704%
7	8.010	813	820	830	rBV	724615	1141639	20.65%	2.093%
8	8.740	936	944	961	rBV	1099332	1919229	34.72%	3.519%
9	9.193	1014	1021	1039	rBV	916257	1534481	27.76%	2.813%
10	9.916	1134	1144	1156	rBV	806070	1381169	24.99%	2.532%
11	10.463	1227	1237	1268	rBV	929453	2020776	36.56%	3.705%
12	10.834	1293	1300	1314	rBV	1047611	1790063	32.39%	3.282%
13	10.999	1320	1328	1349	rBV2	79601	220689	3.99%	0.405%
14	11.704	1442	1448	1450	rBV6	3591	5762	0.10%	0.011%
15	12.440	1567	1573	1582	rBV5	14218	32276	0.58%	0.059%
16	13.640	1772	1777	1783	rVB10	4920	10543	0.19%	0.019%
17	14.075	1844	1851	1865	rBV	2332163	3212757	58.12%	5.891%
18	14.363	1892	1900	1914	rBV	2422352	3576631	64.71%	6.558%
19	14.534	1927	1929	1937	rVB9	3366	5607	0.10%	0.010%
20	14.669	1945	1952	1965	rVB	1773525	2594595	46.94%	4.757%
21	14.904	1986	1992	2019	rBV	449344	1275656	23.08%	2.339%
22	15.663	2114	2121	2132	rBV	3061808	4503220	81.47%	8.257%
23	15.792	2136	2143	2158	rVV	986695	1486789	26.90%	2.726%
24	15.904	2158	2162	2166	rVB2	16436	24250	0.44%	0.044%
25	17.428	2415	2421	2431	rBV	2207707	3126832	56.57%	5.733%
26	17.528	2432	2438	2455	rVV	3509896	5102797	92.32%	9.356%
27	19.333	2742	2745	2749	rBV2	48343	60498	1.09%	0.111%
28	19.404	2755	2757	2762	rVB	31919	36731	0.66%	0.067%
29	19.757	2811	2817	2826	rBV	4098353	5527374	100.00%	10.134%
30	21.516	3111	3116	3127	rBV	1819480	2736694	49.51%	5.018%
31	23.874	3510	3517	3526	rVB2	2091096	4278072	77.40%	7.844%
32	24.039	3539	3545	3558	rVB2	1120536	2425443	43.88%	4.447%




Sum of corrected areas: 54540310

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014460.D
Acq On : 01 Apr 2023 00:59
Operator : CG/JU
Sample : PB151752BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK752

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

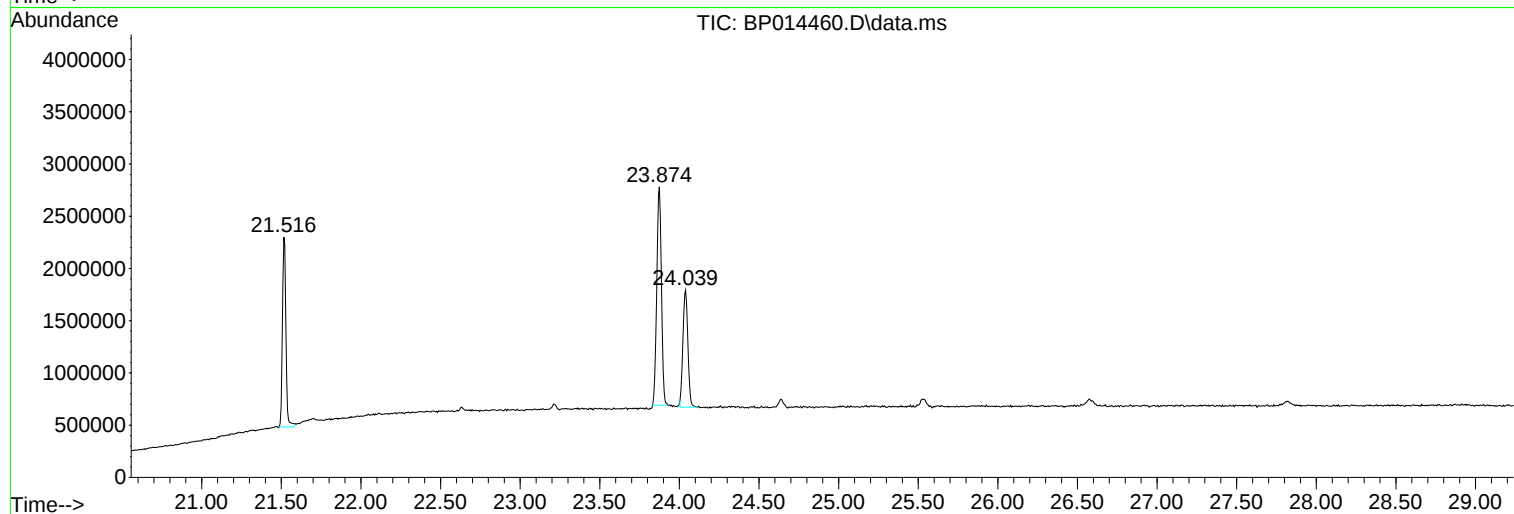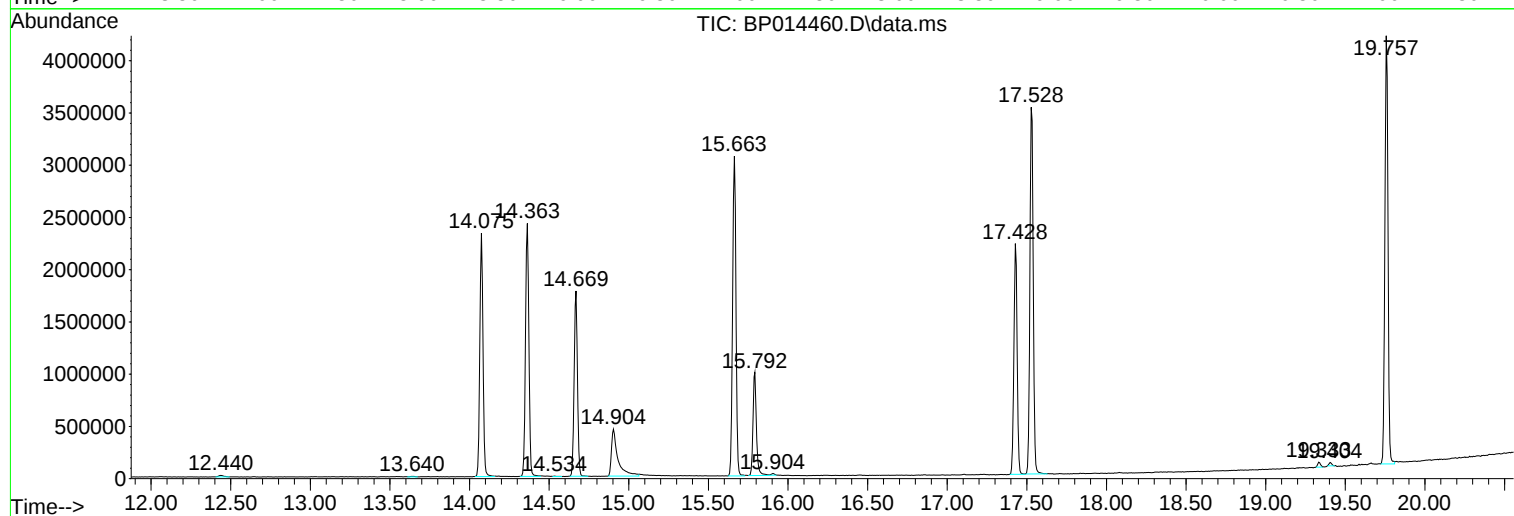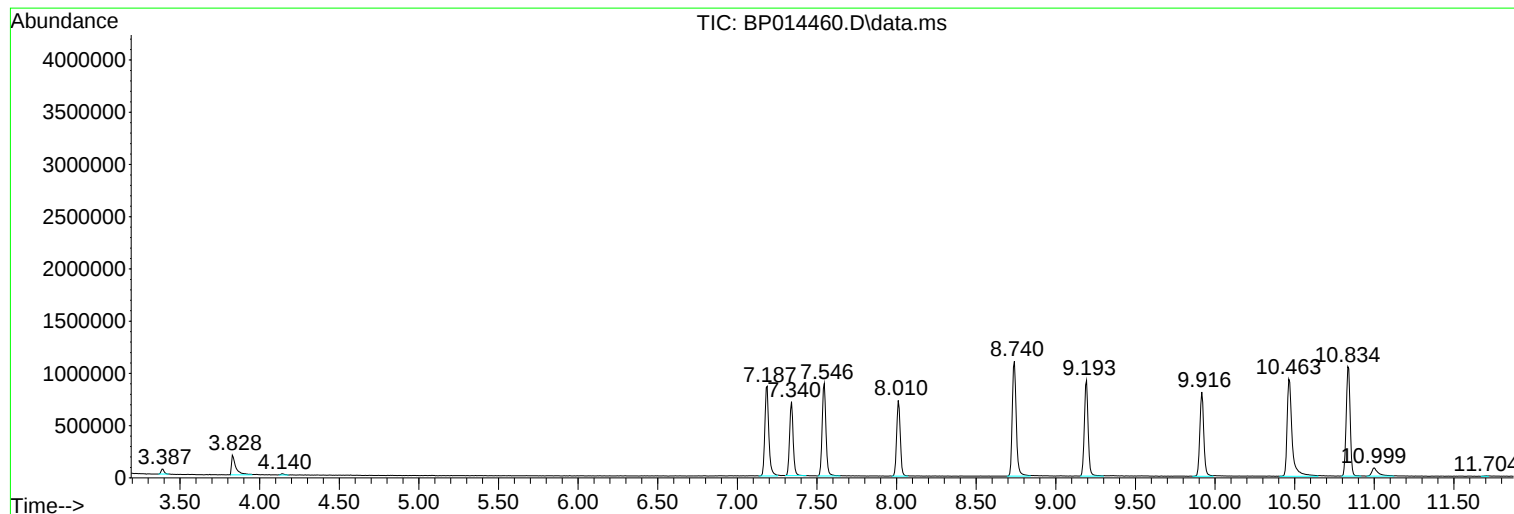

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014460.D
Acq On : 01 Apr 2023 00:59
Operator : CG/JU
Sample : PB151752BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK752

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014460.D
Acq On : 01 Apr 2023 00:59
Operator : CG/JU
Sample : PB151752BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK752

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------