

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014461.D
 Acq On : 01 Apr 2023 01:33
 Operator : CG/JU
 Sample : PB151754BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	42	rVB	45339	67680	1.26%	0.131%
2	3.828	106	109	126	rBV	174725	316852	5.88%	0.612%
3	4.146	158	163	166	rBV	9852	13035	0.24%	0.025%
4	7.181	671	679	698	rBV	819080	1452141	26.94%	2.803%
5	7.340	698	706	717	rBV	648691	1039403	19.28%	2.006%
6	7.546	732	741	753	rBV	852850	1399885	25.97%	2.702%
7	8.010	811	820	831	rBV	645244	1036530	19.23%	2.000%
8	8.740	935	944	961	rBV	1034266	1871779	34.72%	3.612%
9	9.193	1013	1021	1033	rBV	854717	1445947	26.82%	2.791%
10	9.916	1137	1144	1164	rBV	759138	1324851	24.58%	2.557%
11	10.463	1229	1237	1260	rBV	904654	1943377	36.05%	3.751%
12	10.834	1291	1300	1311	rBV	976813	1645909	30.53%	3.177%
13	10.999	1321	1328	1352	rBV2	73824	207058	3.84%	0.400%
14	12.434	1567	1572	1585	rBV4	14087	35119	0.65%	0.068%
15	14.075	1842	1851	1865	rBV	2254759	3115830	57.80%	6.013%
16	14.363	1892	1900	1912	rBV	2327982	3486242	64.67%	6.728%
17	14.669	1945	1952	1964	rBV	1641144	2428757	45.06%	4.687%
18	14.904	1984	1992	2010	rBV	423161	1172977	21.76%	2.264%
19	15.663	2114	2121	2137	rBV	3039462	4374674	81.16%	8.443%
20	15.792	2137	2143	2157	rVV	933191	1410071	26.16%	2.721%
21	15.904	2158	2162	2171	rVB4	16915	33713	0.63%	0.065%
22	17.104	2362	2366	2370	rBV7	6397	10904	0.20%	0.021%
23	17.428	2414	2421	2431	rBV	2023484	2897584	53.75%	5.592%
24	17.528	2432	2438	2451	rVV2	3392285	4959427	92.00%	9.571%
25	19.333	2742	2745	2750	rVB4	42626	57389	1.06%	0.111%
26	19.404	2754	2757	2761	rVV2	35227	47197	0.88%	0.091%
27	19.757	2811	2817	2827	rBV	4012704	5390412	100.00%	10.403%
28	21.516	3111	3116	3123	rBV	1756373	2461249	45.66%	4.750%
29	23.874	3510	3517	3526	rVB2	1944535	4038299	74.92%	7.794%
30	24.033	3538	3544	3554	rVB2	1007955	2130706	39.53%	4.112%




Sum of corrected areas: 51814997

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014461.D
Acq On : 01 Apr 2023 01:33
Operator : CG/JU
Sample : PB151754BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK754

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

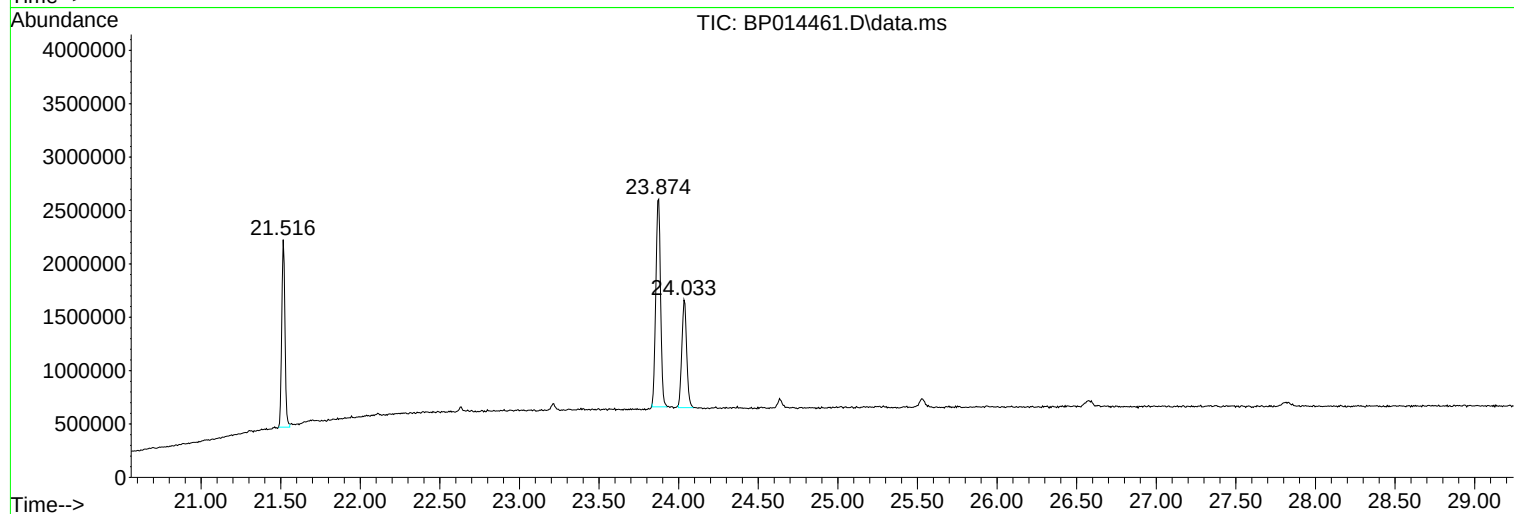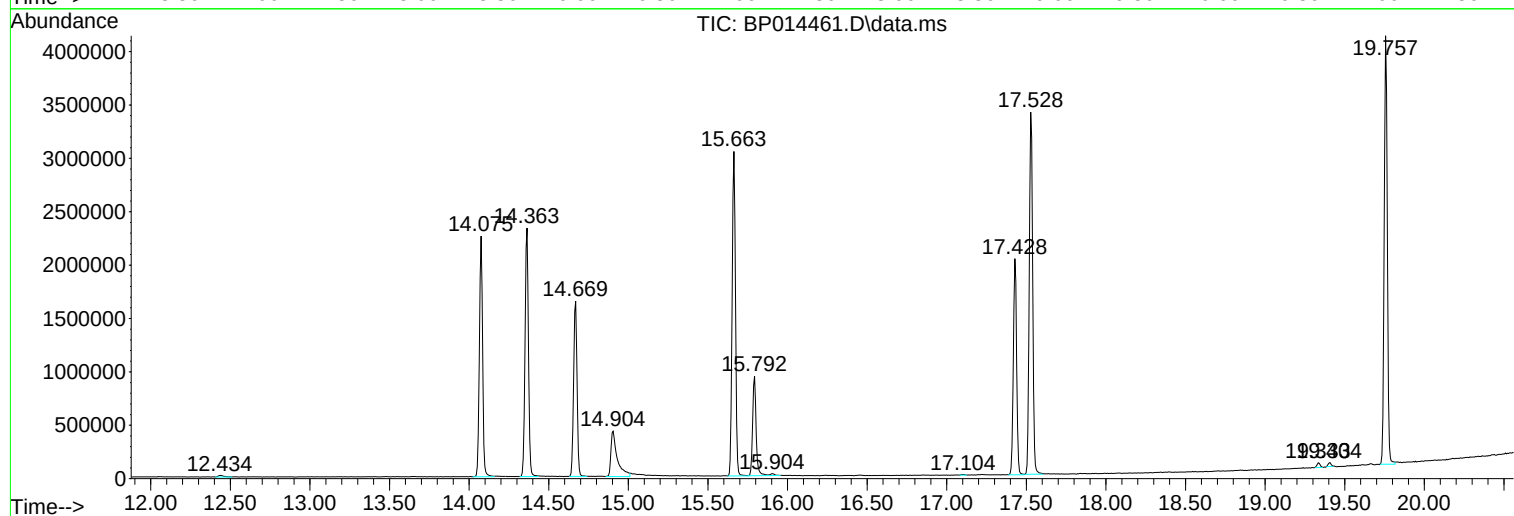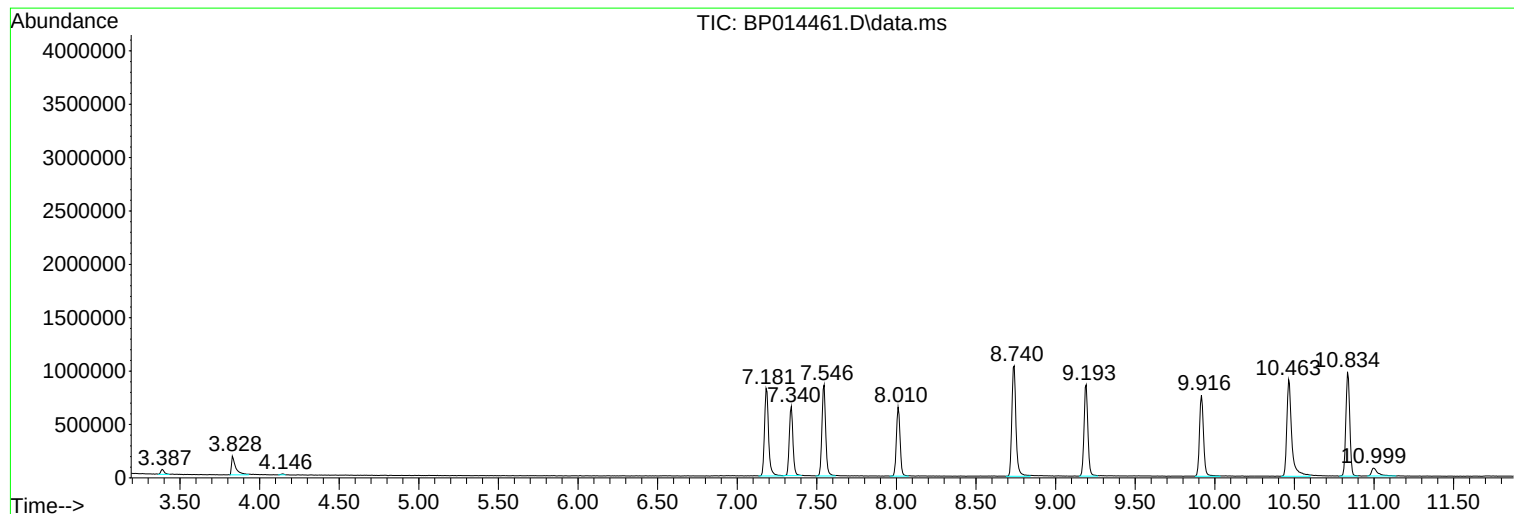

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014461.D
Acq On : 01 Apr 2023 01:33
Operator : CG/JU
Sample : PB151754BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK754

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014461.D
Acq On : 01 Apr 2023 01:33
Operator : CG/JU
Sample : PB151754BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK754

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------