

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014465.D
 Acq On : 01 Apr 2023 03:48
 Operator : CG/JU
 Sample : 02092-14
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	41	rVB	35916	51077	0.91%	0.103%
2	3.846	110	112	121	rBV	45637	89378	1.59%	0.180%
3	4.046	140	146	149	rBV2	13085	21912	0.39%	0.044%
4	4.146	157	163	167	rBV	14653	20947	0.37%	0.042%
5	4.252	177	181	186	rVB6	9102	15088	0.27%	0.030%
6	5.081	317	322	326	rBV	11042	15280	0.27%	0.031%
7	6.393	538	545	551	rBV4	8757	16687	0.30%	0.034%
8	7.187	673	680	691	rBV	142946	276308	4.92%	0.556%
9	7.340	699	706	723	rBV	661829	1082154	19.26%	2.176%
10	7.546	734	741	760	rBV	621943	1072413	19.08%	2.156%
11	8.011	813	820	832	rBV	661774	1058764	18.84%	2.129%
12	8.293	863	868	883	rVB	8581	26870	0.48%	0.054%
13	8.740	936	944	958	rBV	482602	877526	15.61%	1.764%
14	9.187	1013	1020	1035	rBV	880577	1526339	27.16%	3.069%
15	9.340	1038	1046	1055	rVB7	16595	33347	0.59%	0.067%
16	9.558	1079	1083	1087	rVB2	8123	11948	0.21%	0.024%
17	9.916	1136	1144	1160	rBV	757519	1318244	23.46%	2.651%
18	10.463	1230	1237	1266	rBV	852561	1803095	32.08%	3.626%
19	10.834	1293	1300	1309	rBV	987013	1658264	29.51%	3.334%
20	10.993	1321	1327	1344	rBV	96434	231896	4.13%	0.466%
21	11.669	1438	1442	1449	rBV9	6348	15710	0.28%	0.032%
22	12.057	1504	1508	1515	rVB7	4057	8183	0.15%	0.016%
23	12.434	1565	1572	1581	rBV3	17383	34304	0.61%	0.069%
24	13.463	1744	1747	1753	rVB6	6946	11343	0.20%	0.023%
25	13.640	1772	1777	1782	rBV9	3719	7830	0.14%	0.016%
26	14.075	1842	1851	1864	rBV	2316668	3214684	57.20%	6.464%
27	14.175	1866	1868	1876	rVB9	6741	11784	0.21%	0.024%
28	14.363	1892	1900	1913	rBV	2405048	3612800	64.29%	7.264%
29	14.528	1926	1928	1935	rVB8	4332	6911	0.12%	0.014%
30	14.663	1945	1951	1959	rBV	1604370	2454203	43.67%	4.935%
31	14.940	1991	1998	2010	rBV5	44220	160084	2.85%	0.322%
32	15.481	2086	2090	2095	rBV7	5936	8320	0.15%	0.017%
33	15.663	2114	2121	2133	rBV	3252932	4569980	81.32%	9.189%
34	15.792	2137	2143	2154	rVV	941608	1465766	26.08%	2.947%
35	15.904	2158	2162	2168	rVB3	19610	32216	0.57%	0.065%
36	16.028	2178	2183	2189	rBV	82726	128921	2.29%	0.259%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014465.D
 Acq On : 01 Apr 2023 03:48
 Operator : CG/JU
 Sample : 02092-14
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.428	2415	2421	2430	rBV	2030391	2906180	51.71%	5.843%
38	17.528	2432	2438	2453	rVB2	3717018	5261811	93.63%	10.580%
39	18.075	2529	2531	2535	rVB5	13014	14907	0.27%	0.030%
40	18.298	2564	2569	2575	rBV3	50583	96060	1.71%	0.193%
41	19.333	2741	2745	2751	rBV4	55396	81537	1.45%	0.164%
42	19.404	2754	2757	2766	rVB	49410	84622	1.51%	0.170%
43	19.757	2811	2817	2826	rBV	4343213	5619956	100.00%	11.300%
44	21.516	3111	3116	3125	rBV	1774008	2404329	42.78%	4.834%
45	23.874	3510	3517	3526	rVB2	2084016	4241486	75.47%	8.528%
46	24.039	3539	3545	3553	rVB	990626	2072168	36.87%	4.167%




Sum of corrected areas: 49733632

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014465.D
Acq On : 01 Apr 2023 03:48
Operator : CG/JU
Sample : 02092-14
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

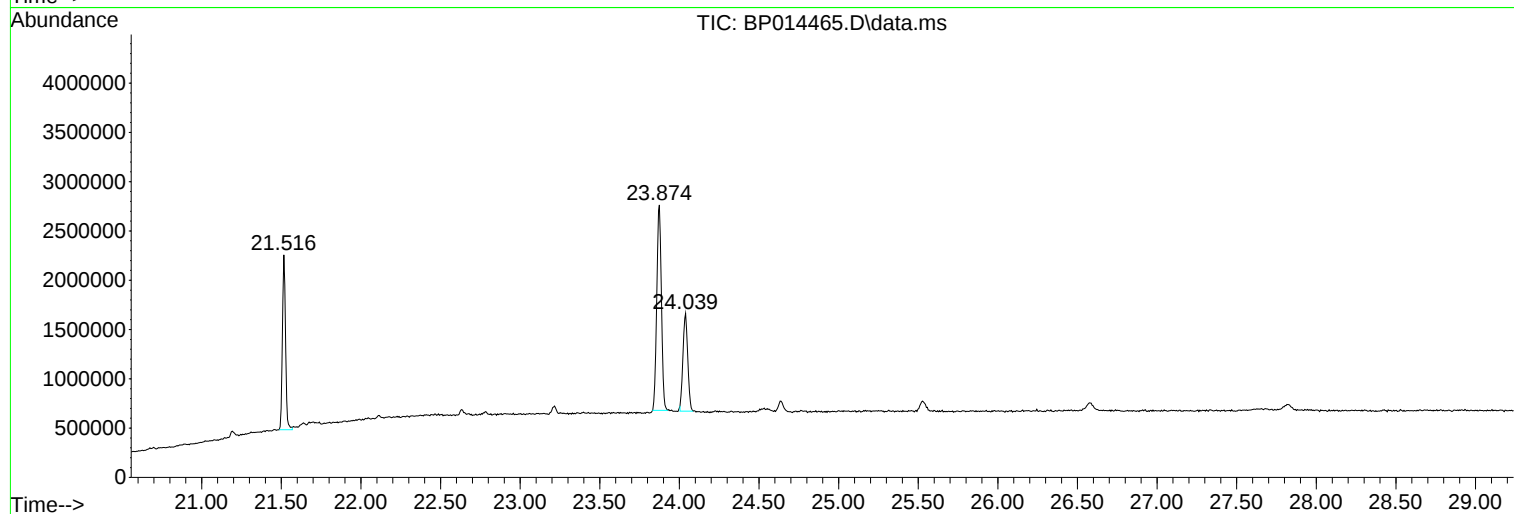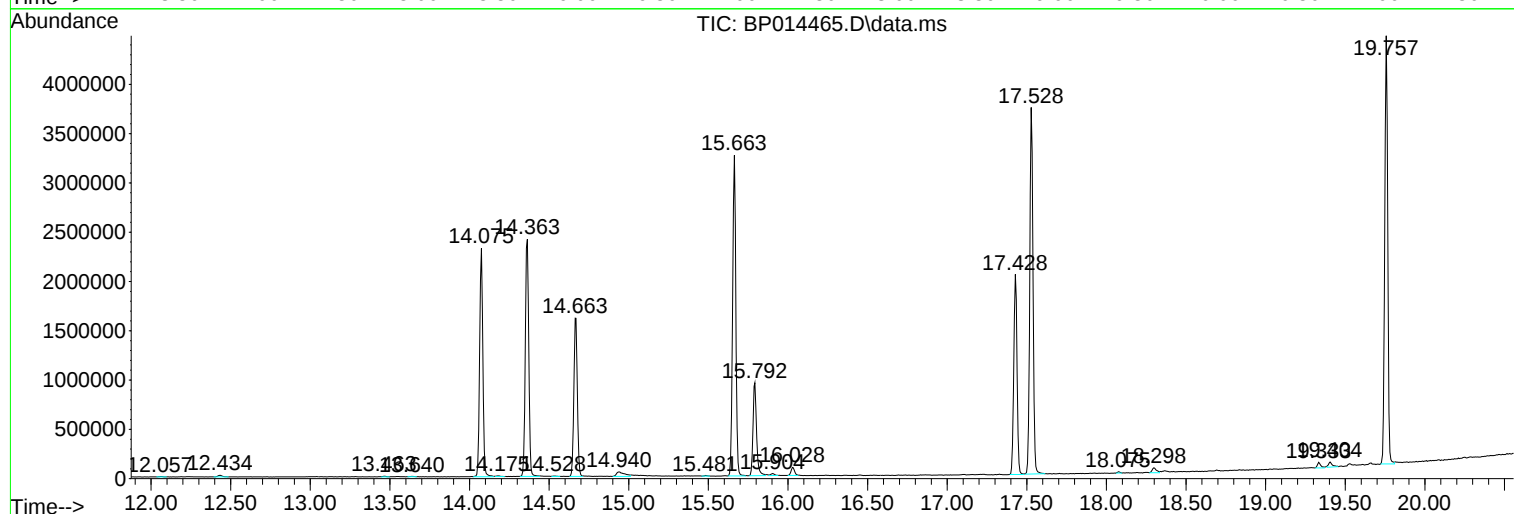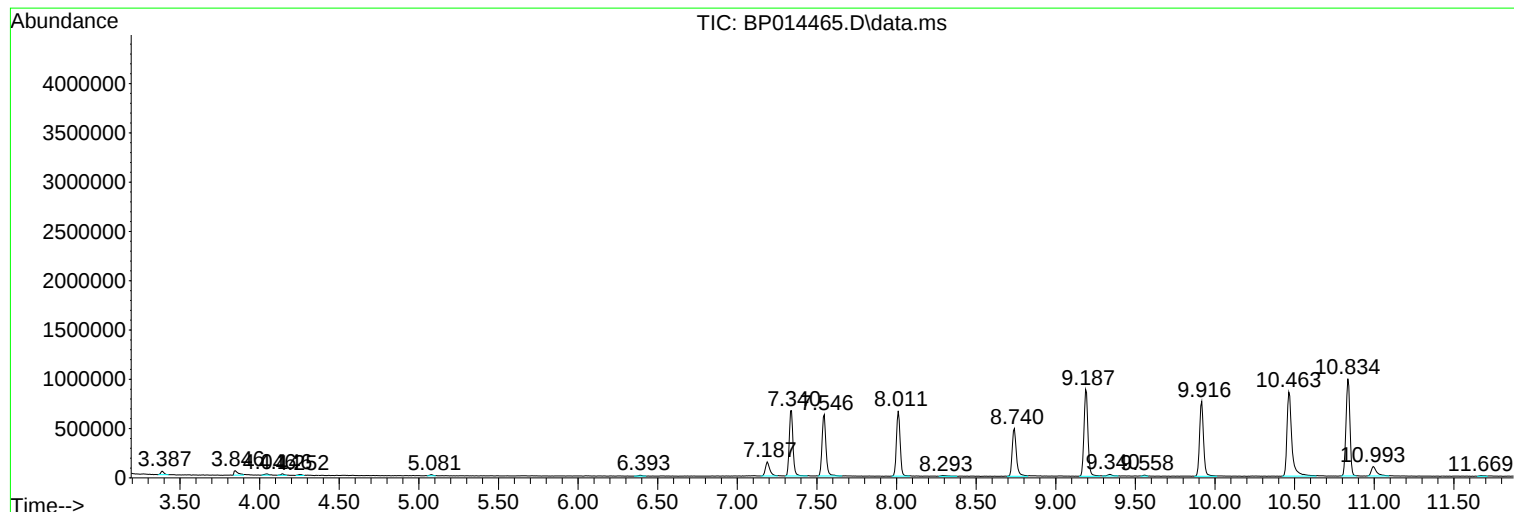

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014465.D
Acq On : 01 Apr 2023 03:48
Operator : CG/JU
Sample : 02092-14
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014465.D
Acq On : 01 Apr 2023 03:48
Operator : CG/JU
Sample : 02092-14
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc