

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014466.D
 Acq On : 01 Apr 2023 04:22
 Operator : CG/JU
 Sample : 02093-09
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	31	34	42	rVB	33523	48729	0.92%	0.100%
2	3.846	110	112	123	rBV	44414	90992	1.71%	0.188%
3	4.040	140	145	152	rBV	13459	23156	0.44%	0.048%
4	4.146	158	163	170	rVB2	12374	21779	0.41%	0.045%
5	4.252	178	181	188	rVB7	8798	13691	0.26%	0.028%
6	4.528	224	228	232	rBV7	4214	5514	0.10%	0.011%
7	5.075	317	321	327	rBV2	12411	20875	0.39%	0.043%
8	6.393	539	545	552	rVB5	9860	15886	0.30%	0.033%
9	7.187	672	680	690	rBV	145063	281883	5.31%	0.581%
10	7.340	699	706	721	rBV	666612	1097361	20.67%	2.262%
11	7.546	733	741	757	rBV	638946	1093922	20.60%	2.255%
12	8.010	814	820	831	rBV	631612	1013306	19.09%	2.089%
13	8.287	863	867	873	rBV8	7177	13324	0.25%	0.027%
14	8.740	935	944	962	rBV	474339	889430	16.75%	1.834%
15	9.187	1013	1020	1037	rBV	904183	1543658	29.07%	3.182%
16	9.346	1041	1047	1053	rVB7	13749	26647	0.50%	0.055%
17	9.557	1079	1083	1091	rVB2	11235	18825	0.35%	0.039%
18	9.916	1134	1144	1157	rBV	775302	1321671	24.89%	2.725%
19	10.251	1196	1201	1204	rBV7	2919	6041	0.11%	0.012%
20	10.463	1229	1237	1266	rBV	871226	1830287	34.47%	3.773%
21	10.834	1293	1300	1316	rVB	944286	1607769	30.28%	3.315%
22	10.993	1316	1327	1344	rBV2	94808	249778	4.70%	0.515%
23	12.245	1538	1540	1546	rVB7	4362	6039	0.11%	0.012%
24	12.434	1565	1572	1578	rBV3	15062	32313	0.61%	0.067%
25	13.269	1709	1714	1717	rBV7	4114	5430	0.10%	0.011%
26	13.463	1743	1747	1754	rBV9	5325	8967	0.17%	0.018%
27	13.551	1755	1762	1768	rVB2	15136	24461	0.46%	0.050%
28	13.645	1773	1778	1784	rVB10	5165	10214	0.19%	0.021%
29	14.075	1839	1851	1863	rBV	2293324	3233560	60.90%	6.666%
30	14.304	1885	1890	1892	rBV6	3581	5493	0.10%	0.011%
31	14.363	1892	1900	1917	rVV	2400471	3605314	67.91%	7.433%
32	14.669	1945	1952	1961	rBV	1587029	2364829	44.54%	4.875%
33	14.939	1992	1998	2001	rBV4	38101	77716	1.46%	0.160%
34	15.492	2087	2092	2096	rVB5	5697	8790	0.17%	0.018%
35	15.604	2107	2111	2114	rBV5	5078	6257	0.12%	0.013%
36	15.663	2114	2121	2136	rVV	3196790	4579711	86.26%	9.442%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014466.D
 Acq On : 01 Apr 2023 04:22
 Operator : CG/JU
 Sample : 02093-09
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.792	2136	2143	2158	rVV	863620	1367260	25.75%	2.819%
38	15.904	2158	2162	2170	rVB3	15450	32636	0.61%	0.067%
39	16.034	2178	2184	2192	rVB	80182	120908	2.28%	0.249%
40	17.428	2415	2421	2431	rBV	1962619	2716307	51.16%	5.600%
41	17.528	2432	2438	2454	rVV	3562372	5157028	97.13%	10.632%
42	18.075	2528	2531	2537	rBV8	15266	23450	0.44%	0.048%
43	18.298	2565	2569	2578	rBV3	40627	79504	1.50%	0.164%
44	19.333	2742	2745	2751	rBV3	48571	65149	1.23%	0.134%
45	19.404	2754	2757	2767	rVB2	44056	74900	1.41%	0.154%
46	19.757	2811	2817	2825	rBV	4115850	5309345	100.00%	10.946%
47	21.516	3111	3116	3126	rBV	1569755	2167994	40.83%	4.470%
48	23.874	3510	3517	3525	rVB	2137803	4162815	78.41%	8.582%
49	24.033	3539	3544	3554	rVB2	951318	2023805	38.12%	4.172%




Sum of corrected areas: 48504719

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

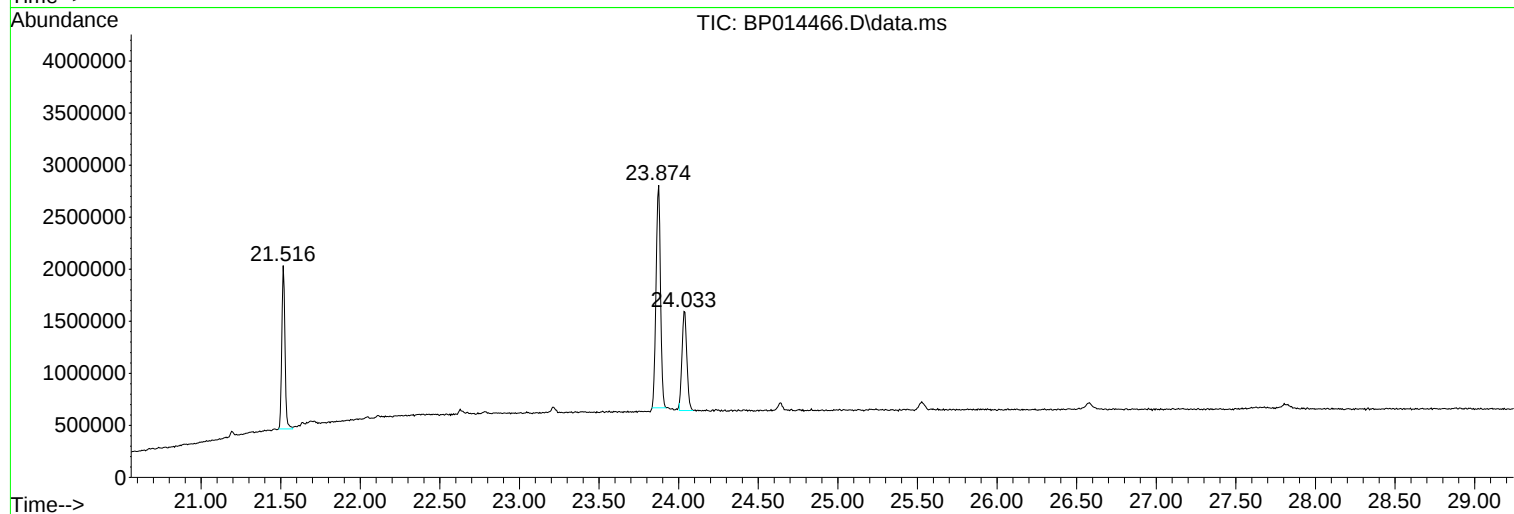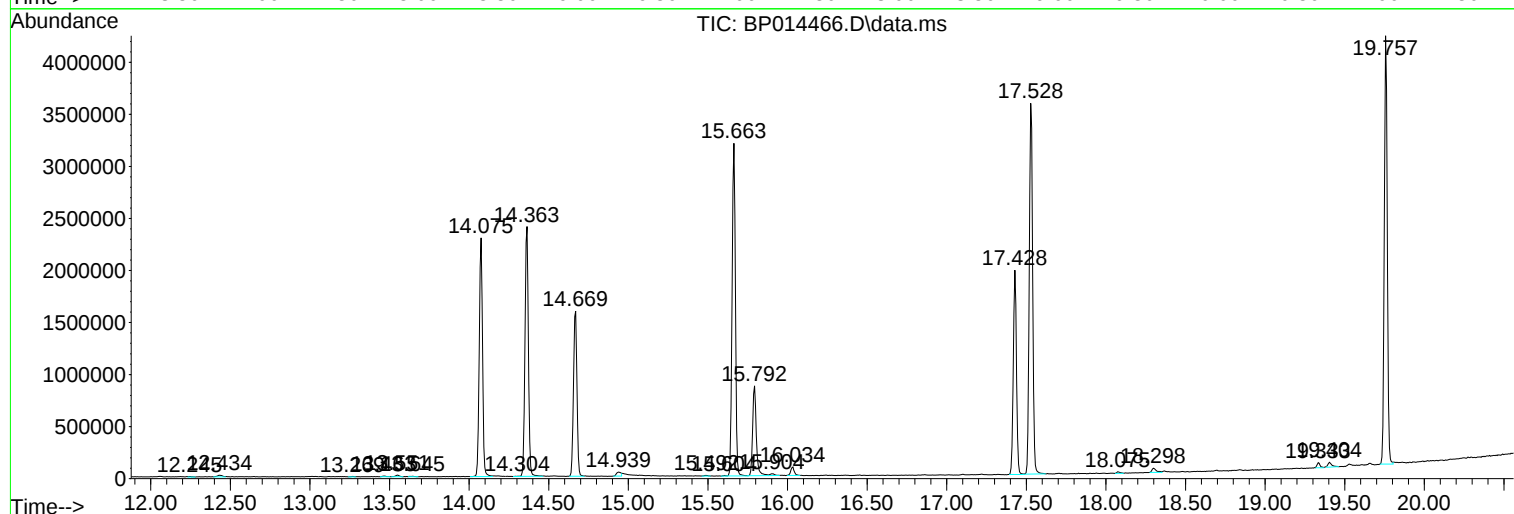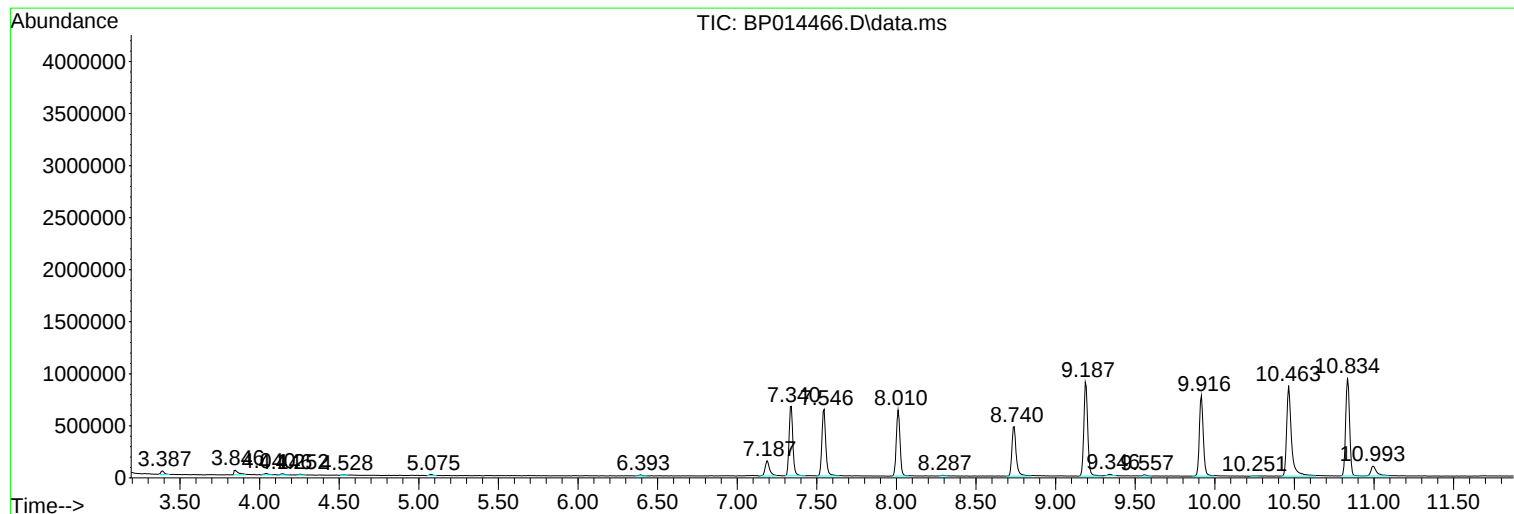

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------