

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005120.D
 Acq On : 31 Mar 2021 11:35
 Operator : CG/JU
 Sample : M1817-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PHC-326FB-002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	38	rVB	44564	53565	2.43%	0.498%
2	4.375	214	219	226	rBV	56260	74538	3.39%	0.693%
3	4.822	289	295	297	rBV	35817	45883	2.09%	0.427%
4	4.858	297	301	308	rVB	56620	79402	3.61%	0.739%
5	5.311	370	378	391	rBV	618704	855623	38.88%	7.960%
6	6.887	637	646	659	rBV	494120	789282	35.87%	7.343%
7	7.710	777	786	794	rBV	113437	172912	7.86%	1.609%
8	8.869	975	983	992	rBV	382981	625095	28.41%	5.815%
9	10.499	1250	1260	1266	rBV	132930	215519	9.79%	2.005%
10	12.981	1674	1682	1689	rBV	937335	1311401	59.59%	12.200%
11	13.822	1820	1825	1834	rVB	33868	52022	2.36%	0.484%
12	14.363	1911	1917	1924	rBV	189857	278530	12.66%	2.591%
13	15.198	2051	2059	2067	rBV	21478	39987	1.82%	0.372%
14	15.863	2165	2172	2180	rBV	745180	1025113	46.58%	9.537%
15	17.122	2380	2386	2392	rBV	251896	343017	15.59%	3.191%
16	18.028	2532	2540	2548	rBV	271239	401953	18.27%	3.739%
17	18.092	2548	2551	2557	rVB	27762	40713	1.85%	0.379%
18	18.292	2581	2585	2590	rBV7	13817	23026	1.05%	0.214%
19	18.757	2660	2664	2668	rVB	19070	22630	1.03%	0.211%
20	19.145	2727	2730	2738	rVB7	17322	28630	1.30%	0.266%
21	19.263	2743	2750	2764	rBV2	136459	218812	9.94%	2.036%
22	19.698	2818	2824	2829	rBV	1873596	2200588	100.00%	20.473%
23	20.445	2944	2951	2954	rBV4	41811	84525	3.84%	0.786%
24	20.898	3024	3028	3030	rBV2	21225	28791	1.31%	0.268%
25	20.933	3030	3034	3041	rVV2	139077	247906	11.27%	2.306%
26	21.004	3042	3046	3052	rVB	138792	164432	7.47%	1.530%
27	21.133	3065	3068	3071	rVB	21730	23324	1.06%	0.217%
28	21.216	3077	3082	3087	rBV	320232	428990	19.49%	3.991%
29	21.304	3087	3097	3106	rVV10	126132	421249	19.14%	3.919%
30	23.498	3464	3470	3479	rVB2	231521	451530	20.52%	4.201%




Sum of corrected areas: 10748988

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005120.D
Acq On : 31 Mar 2021 11:35
Operator : CG/JU
Sample : M1817-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

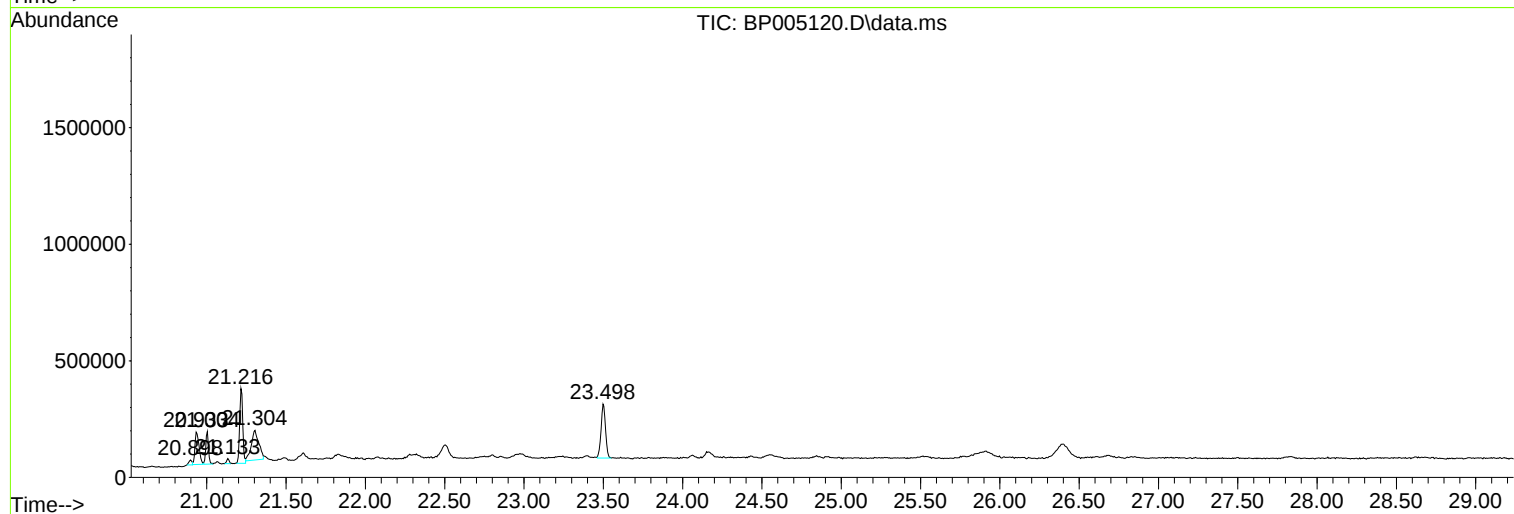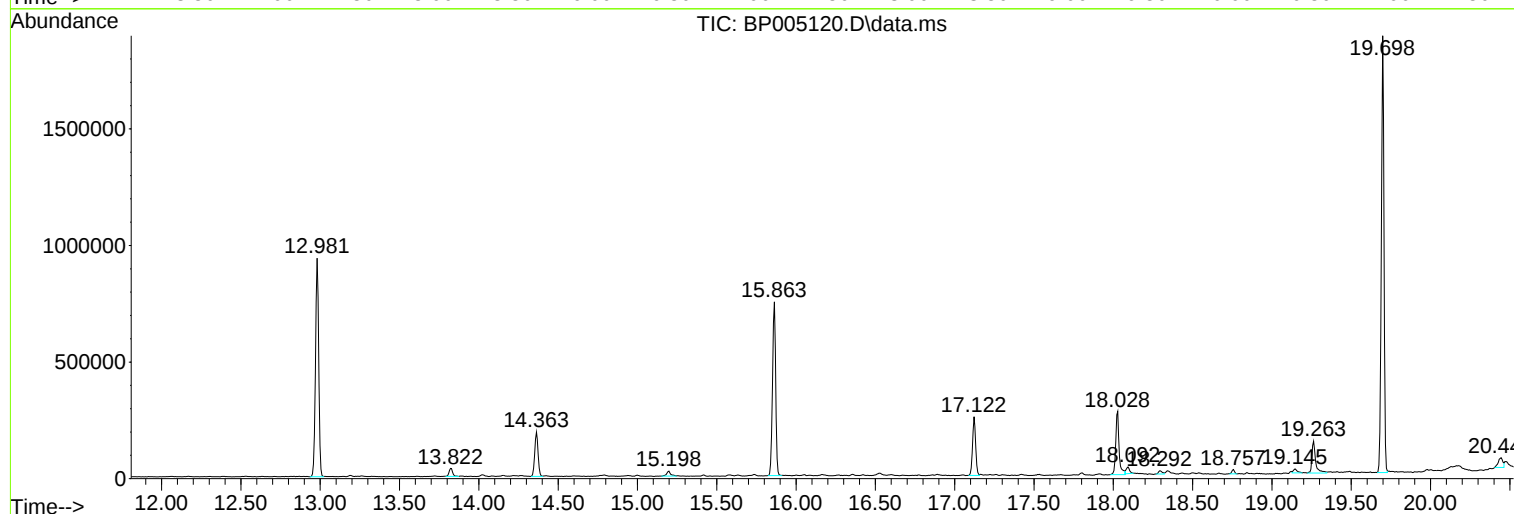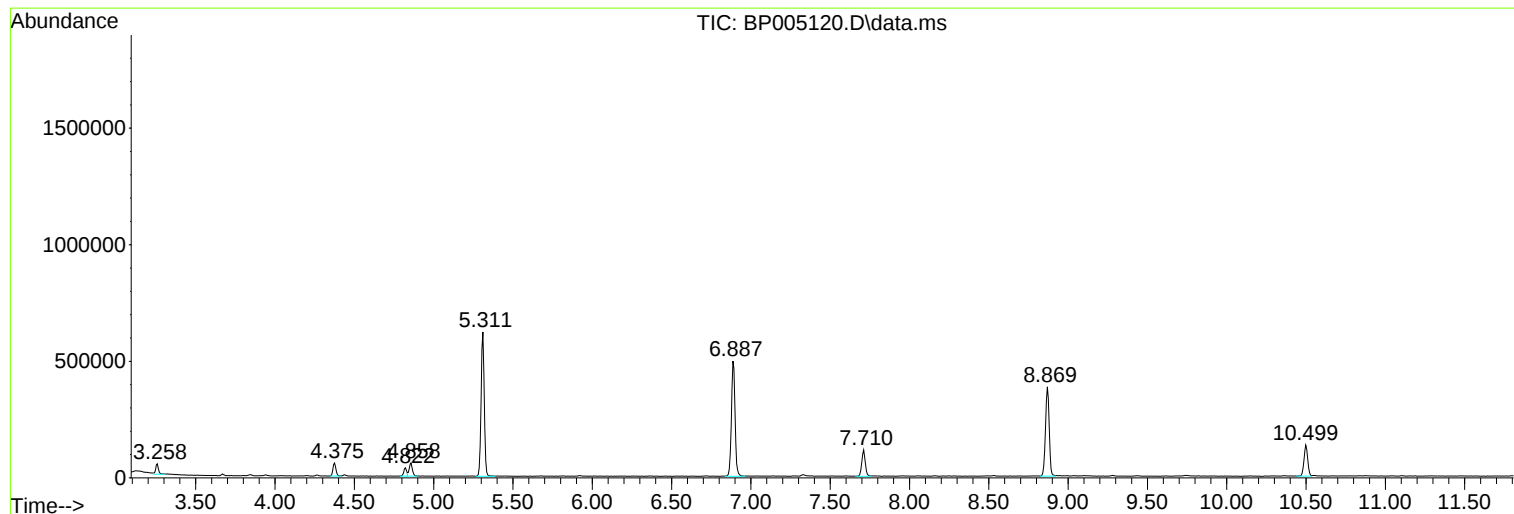

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005120.D
Acq On : 31 Mar 2021 11:35
Operator : CG/JU
Sample : M1817-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005120.D
Acq On : 31 Mar 2021 11:35
Operator : CG/JU
Sample : M1817-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------