

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005121.D
 Acq On : 31 Mar 2021 12:09
 Operator : CG/JU
 Sample : M1817-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PHC-326FB-002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.858	296	301	307	rVB	18684	26467	1.77%	0.276%
2	5.305	370	377	388	rBV	484829	704713	47.13%	7.351%
3	6.887	638	646	660	rBV	478072	753955	50.42%	7.864%
4	7.710	779	786	793	rBV	116972	183295	12.26%	1.912%
5	8.869	975	983	992	rBV	287184	467696	31.28%	4.878%
6	10.498	1253	1260	1267	rBV	145417	239787	16.04%	2.501%
7	12.981	1673	1682	1692	rBV	719354	1030576	68.92%	10.750%
8	13.822	1820	1825	1833	rVB2	14775	25102	1.68%	0.262%
9	14.081	1864	1869	1875	rBV	13010	22974	1.54%	0.240%
10	14.363	1910	1917	1924	rVB	230600	329193	22.01%	3.434%
11	15.857	2165	2171	2179	rBV	564531	803385	53.73%	8.380%
12	17.122	2378	2386	2390	rBV	276648	395656	26.46%	4.127%
13	17.163	2390	2393	2400	rVB	72827	99805	6.67%	1.041%
14	17.251	2405	2408	2414	rVB	21195	31809	2.13%	0.332%
15	18.022	2531	2539	2548	rBV3	153107	242613	16.22%	2.531%
16	18.180	2561	2566	2570	rBV2	20824	34102	2.28%	0.356%
17	19.016	2704	2708	2716	rVB9	11680	22484	1.50%	0.235%
18	19.139	2722	2729	2736	rBV	149267	211716	14.16%	2.208%
19	19.263	2743	2750	2759	rBV2	67025	127096	8.50%	1.326%
20	19.492	2785	2789	2798	rVB	123581	171463	11.47%	1.788%
21	19.698	2816	2824	2829	rBV	1285617	1495365	100.00%	15.598%
22	19.974	2868	2871	2880	rVB3	26145	48183	3.22%	0.503%
23	20.321	2926	2930	2934	rBV5	12381	18214	1.22%	0.190%
24	20.933	3030	3034	3042	rVV3	164174	238440	15.95%	2.487%
25	20.998	3043	3045	3053	rVB	34181	43162	2.89%	0.450%
26	21.216	3076	3082	3086	rBV2	381509	562264	37.60%	5.865%
27	21.251	3086	3088	3095	rVB	61939	75898	5.08%	0.792%
28	21.333	3099	3102	3105	rBV2	25685	31324	2.09%	0.327%
29	21.363	3105	3107	3111	rBV4	15281	17692	1.18%	0.185%
30	21.821	3179	3185	3193	rBV2	169054	305034	20.40%	3.182%
31	22.510	3299	3302	3307	rBV2	41604	53554	3.58%	0.559%
32	22.804	3347	3352	3356	rBV3	94222	174959	11.70%	1.825%
33	23.398	3449	3453	3460	rVB	53083	99274	6.64%	1.035%
34	23.498	3464	3470	3477	rVV2	228310	429301	28.71%	4.478%
35	23.715	3504	3507	3514	rVB6	44415	70573	4.72%	0.736%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005121.D
Acq On : 31 Mar 2021 12:09
Operator : CG/JU
Sample : M1817-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 9587124

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005121.D
Acq On : 31 Mar 2021 12:09
Operator : CG/JU
Sample : M1817-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

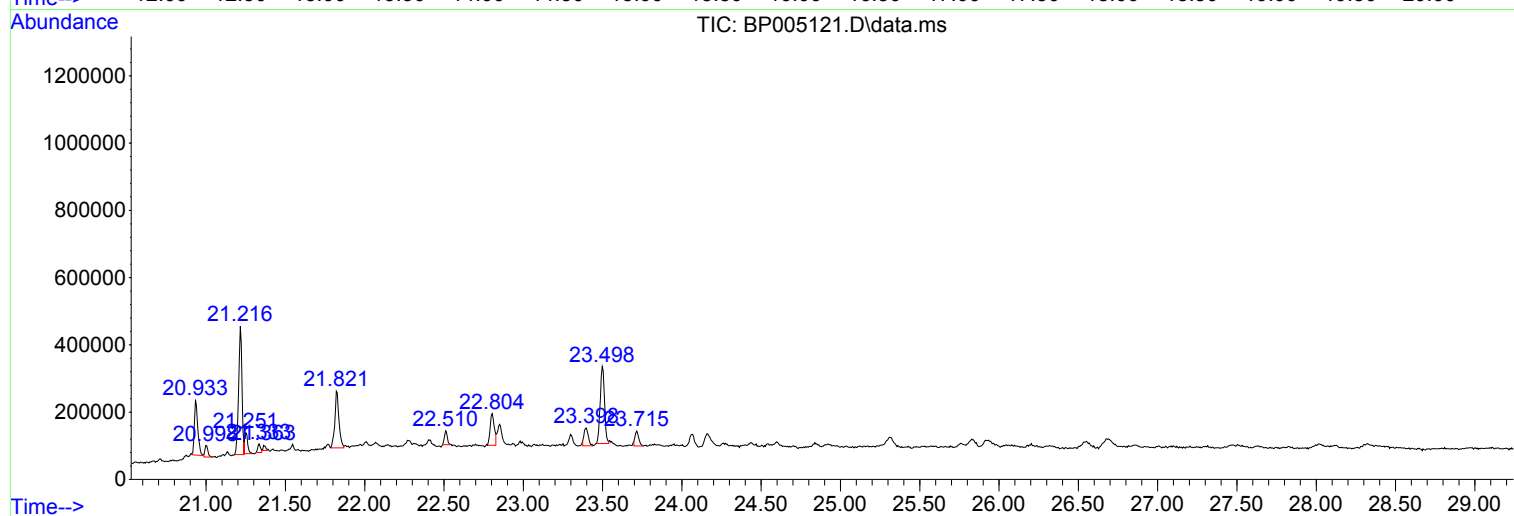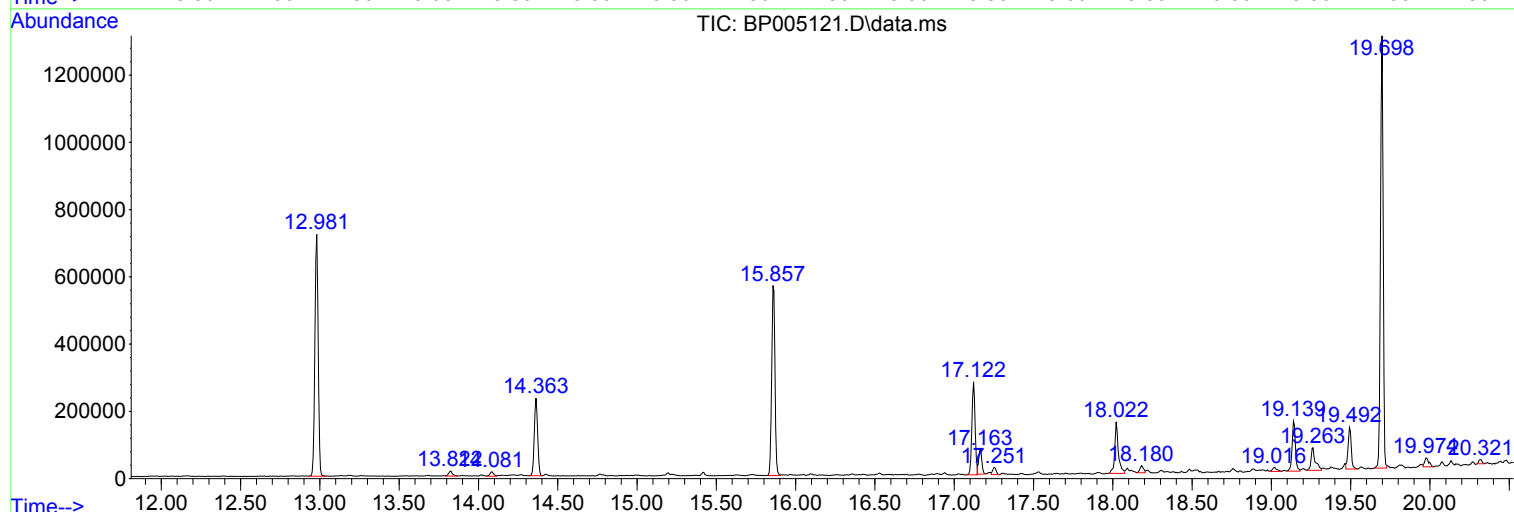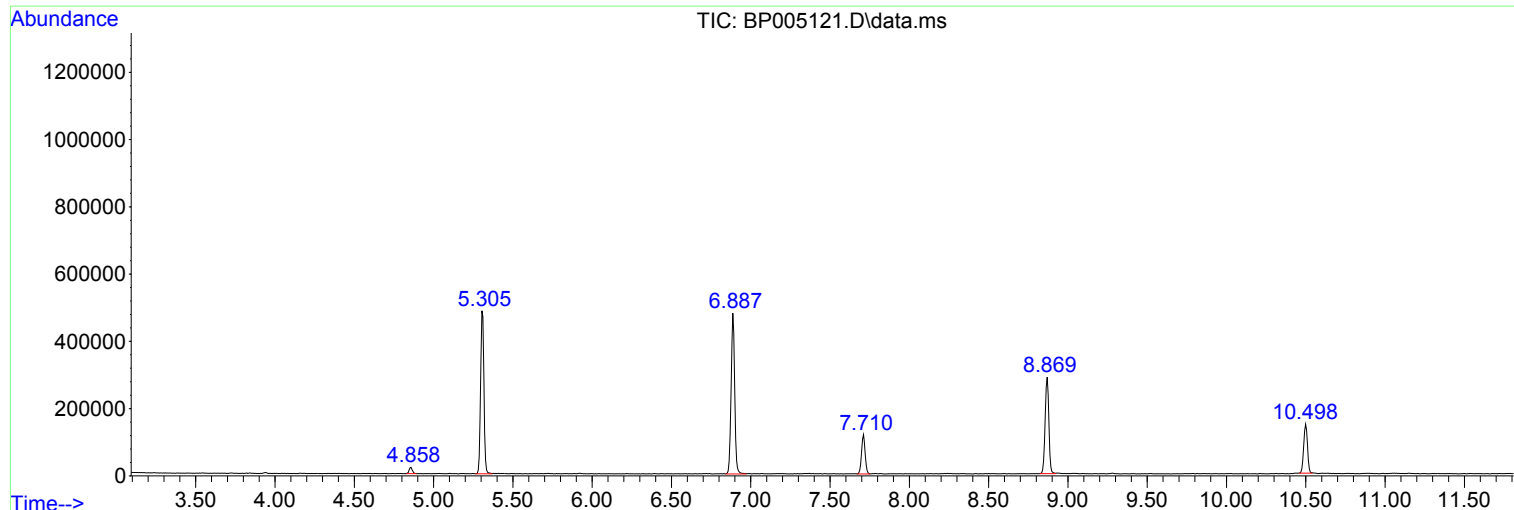

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005121.D
Acq On : 31 Mar 2021 12:09
Operator : CG/JU
Sample : M1817-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005121.D
Acq On : 31 Mar 2021 12:09
Operator : CG/JU
Sample : M1817-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------