

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005123.D
 Acq On : 31 Mar 2021 13:17
 Operator : CG/JU
 Sample : M1817-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PHC-326FB-003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.311	370	378	385	rBV	553383	802113	10.60%	1.243%
2	6.887	635	646	661	rVB	533407	951655	12.58%	1.474%
3	7.711	776	786	791	rBV2	155557	298932	3.95%	0.463%
4	8.216	865	872	876	rBV2	45688	89378	1.18%	0.138%
5	8.811	962	973	977	rBV4	36517	80744	1.07%	0.125%
6	8.869	977	983	991	rVV	339605	571021	7.55%	0.885%
7	9.681	1115	1121	1131	rBV5	48343	112964	1.49%	0.175%
8	9.922	1154	1162	1168	rBV	203309	346838	4.59%	0.537%
9	10.010	1171	1177	1183	rVV	75834	131379	1.74%	0.204%
10	10.499	1252	1260	1265	rBV	197456	331797	4.39%	0.514%
11	11.334	1389	1402	1410	rBV	209269	353933	4.68%	0.548%
12	12.981	1675	1682	1690	rVB	795726	1152546	15.24%	1.786%
13	14.363	1911	1917	1924	rBV	293290	424204	5.61%	0.657%
14	15.634	2125	2133	2138	rBV2	70822	118478	1.57%	0.184%
15	15.722	2142	2148	2154	rVB3	59866	104230	1.38%	0.161%
16	15.863	2166	2172	2177	rBV	594705	843897	11.16%	1.307%
17	16.534	2281	2286	2295	rVB8	38650	76547	1.01%	0.119%
18	17.122	2381	2386	2391	rBV	319667	495064	6.54%	0.767%
19	17.163	2391	2393	2401	rVB	93217	118982	1.57%	0.184%
20	17.734	2487	2490	2494	rVB	83875	105102	1.39%	0.163%
21	18.034	2536	2541	2545	rBV	653775	913649	12.08%	1.416%
22	18.245	2574	2577	2581	rVB2	102761	128100	1.69%	0.198%
23	18.298	2581	2586	2591	rBV	590470	843909	11.16%	1.307%
24	18.510	2615	2622	2626	rBV	2746438	3875293	51.23%	6.004%
25	18.545	2626	2628	2635	rVB	380492	404285	5.34%	0.626%
26	18.869	2679	2683	2685	rBV	233768	307779	4.07%	0.477%
27	18.916	2685	2691	2699	rVB	3270248	4456147	58.91%	6.904%
28	19.057	2712	2715	2718	rVB	109409	119346	1.58%	0.185%
29	19.151	2725	2731	2737	rBV2	558643	1243126	16.43%	1.926%
30	19.198	2737	2739	2744	rVB	314526	374027	4.94%	0.579%
31	19.275	2747	2752	2755	rBV2	475085	758210	10.02%	1.175%
32	19.428	2775	2778	2782	rVB2	108723	148365	1.96%	0.230%
33	19.498	2787	2790	2799	rVB	364516	524116	6.93%	0.812%
34	19.604	2805	2808	2813	rVB2	217292	265107	3.50%	0.411%
35	19.657	2813	2817	2820	rBV	247109	347310	4.59%	0.538%
36	19.698	2820	2824	2828	rVB	1185723	1407932	18.61%	2.181%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005123.D
 Acq On : 31 Mar 2021 13:17
 Operator : CG/JU
 Sample : M1817-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PHC-326FB-003

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.816	2838	2844	2846	rBV3	176627	290506	3.84%	0.450%
38	19.975	2868	2871	2874	rBV2	202824	256914	3.40%	0.398%
39	20.133	2894	2898	2903	rVB	584416	696729	9.21%	1.079%
40	20.192	2903	2908	2912	rVV3	454131	595258	7.87%	0.922%
41	20.245	2914	2917	2923	rVB3	278514	322319	4.26%	0.499%
42	20.410	2941	2945	2951	rVB2	403874	524046	6.93%	0.812%
43	20.604	2975	2978	2981	rBV2	156467	196765	2.60%	0.305%
44	20.704	2990	2995	2999	rVB2	1803910	2204092	29.14%	3.415%
45	20.763	3002	3005	3009	rVB2	411508	451947	5.97%	0.700%
46	20.857	3016	3021	3024	rBV	1071225	1460102	19.30%	2.262%
47	20.939	3031	3035	3038	rBV2	1076236	1520323	20.10%	2.355%
48	21.033	3044	3051	3056	rVB4	796390	1334518	17.64%	2.068%
49	21.122	3062	3066	3071	rBV2	363000	435613	5.76%	0.675%
50	21.251	3078	3088	3093	rVB3	1637262	2698641	35.67%	4.181%
51	21.310	3095	3098	3100	rBV	128438	132164	1.75%	0.205%
52	21.386	3108	3111	3117	rVB	310183	379670	5.02%	0.588%
53	21.622	3146	3151	3157	rVB	2937430	3603260	47.63%	5.582%
54	21.692	3158	3163	3170	rVB2	2688260	3540367	46.80%	5.485%
55	21.998	3211	3215	3219	rBV	488993	643260	8.50%	0.997%
56	22.104	3230	3233	3238	rVB	214253	269084	3.56%	0.417%
57	22.263	3255	3260	3267	rBV	1383379	2088689	27.61%	3.236%
58	22.727	3334	3339	3345	rVB	1792291	2787534	36.85%	4.319%
59	23.721	3503	3508	3517	rVB	481577	996100	13.17%	1.543%
60	24.157	3575	3582	3592	rVB	1270403	2992570	39.56%	4.636%
61	24.316	3603	3609	3617	rVB	866867	1897119	25.08%	2.939%
62	24.398	3618	3623	3631	rVB	497360	1037117	13.71%	1.607%
63	24.798	3678	3691	3710	rVB	2356838	7564524	100.00%	11.720%




Sum of corrected areas: 64545736

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005123.D
Acq On : 31 Mar 2021 13:17
Operator : CG/JU
Sample : M1817-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

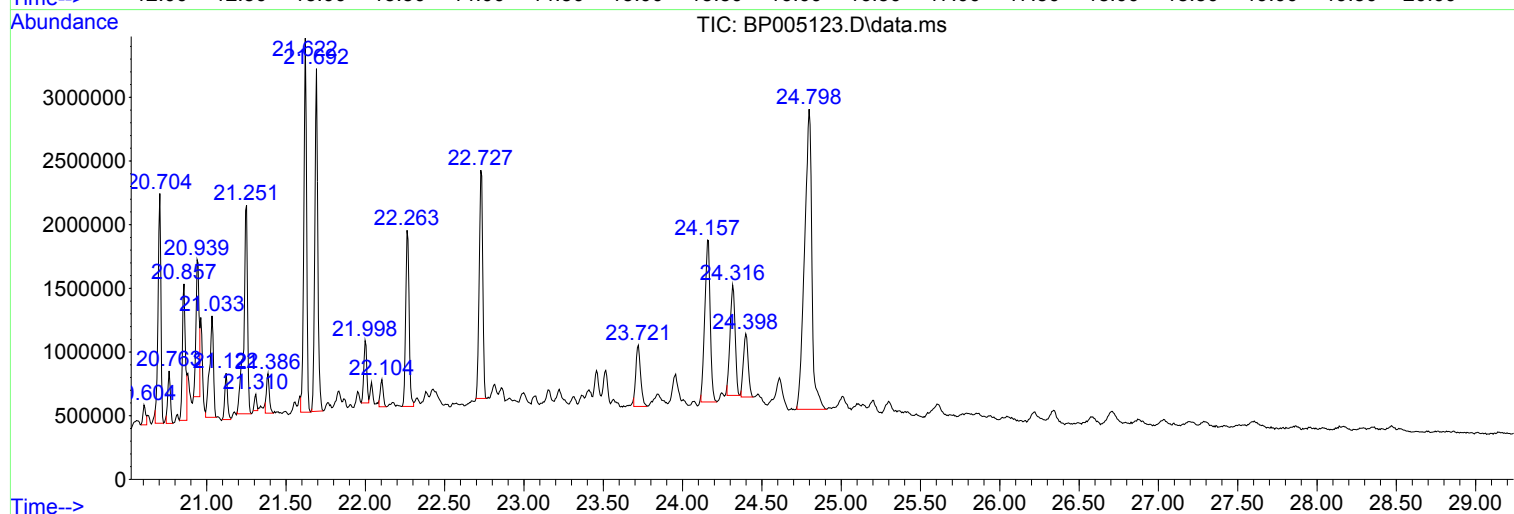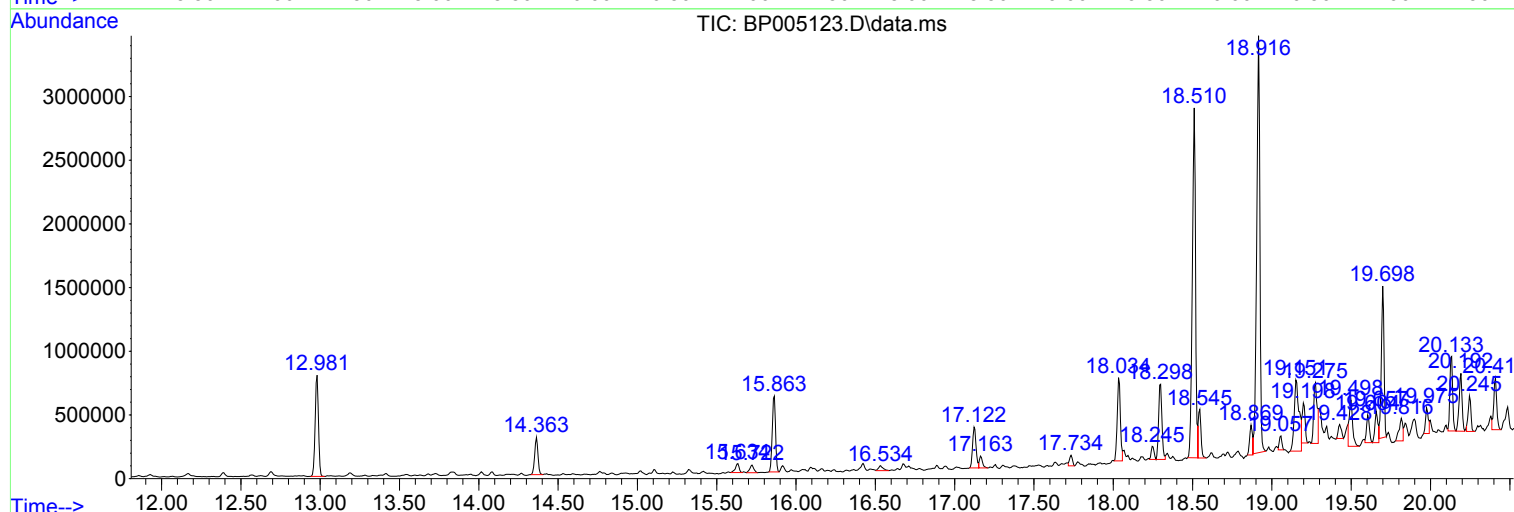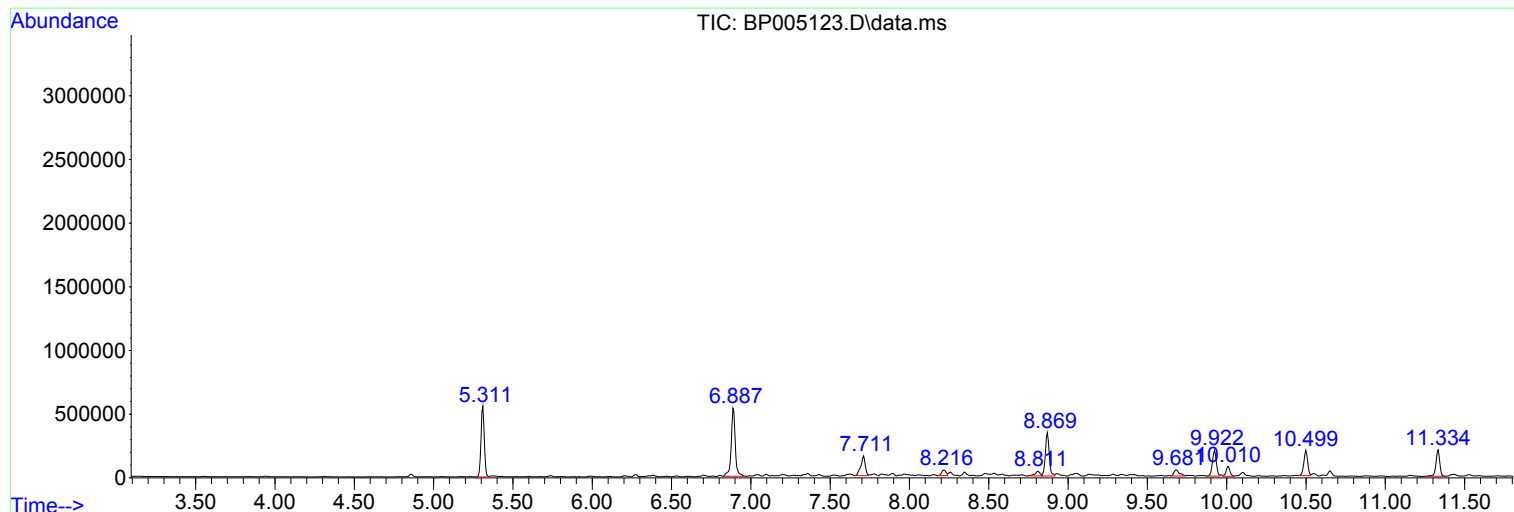

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005123.D
Acq On : 31 Mar 2021 13:17
Operator : CG/JU
Sample : M1817-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
Data File : BP005123.D
Acq On : 31 Mar 2021 13:17
Operator : CG/JU
Sample : M1817-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PHC-326FB-003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------