
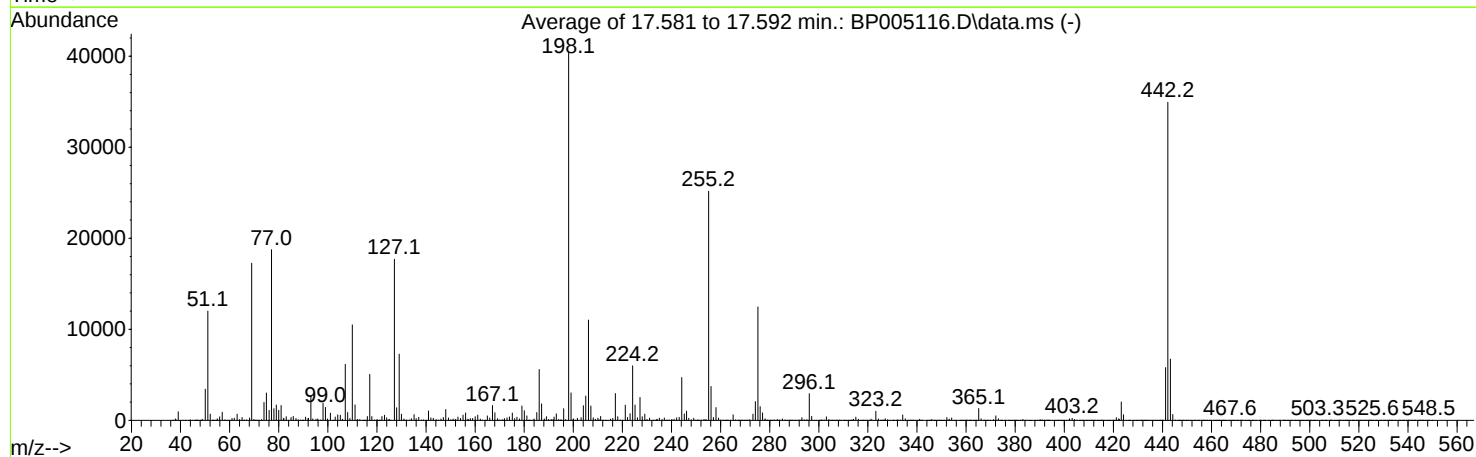


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005116.D
 Acq On : 31 Mar 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 26 10:07:03 2021

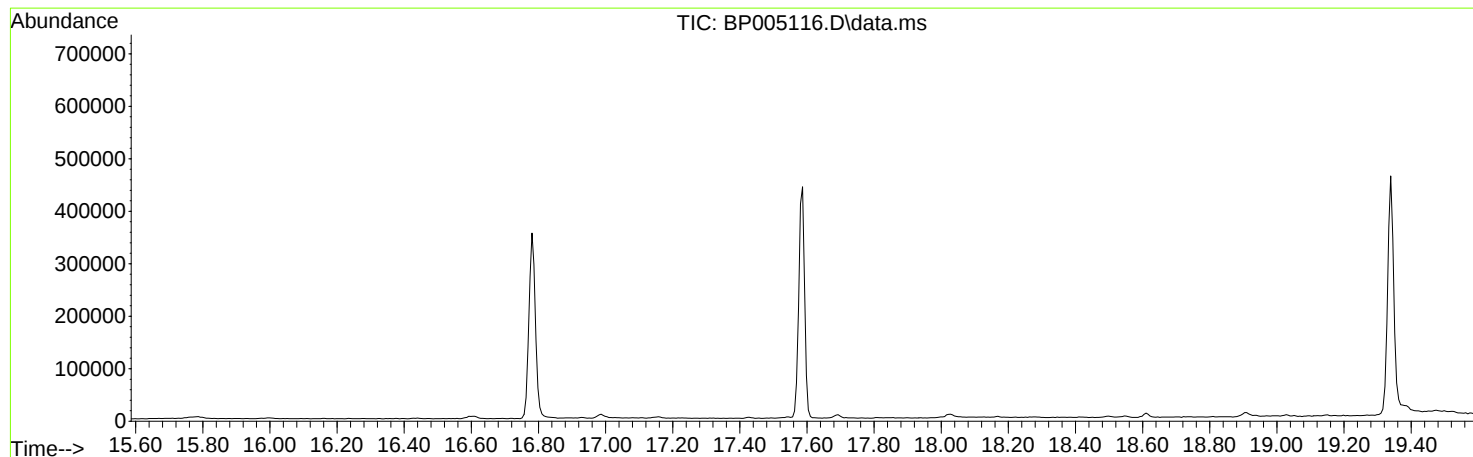

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	12002	PASS
68	69	0.00	2	1.5	267	PASS
69	198	0.00	100	42.7	17260	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	43.8	17699	PASS
197	198	0.00	2	0.2	86	PASS
198	198	100	100	100.0	40405	PASS
199	198	5	9	7.5	3033	PASS
275	198	10	60	30.8	12456	PASS
365	198	1	100	3.2	1306	PASS
441	198	0.01	100	14.4	5801	PASS
442	442	100	100	100.0	34947	PASS
443	442	15	24	19.3	6736	PASS

Instrument :
BNA_P
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2021	BNA_P	<u>BP005116.D</u>
Compound Name	Response	Retention Time
DDT	152471	20.53
DDD	4149	20.11
DDE	638	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4787	157258	3.04

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005116.D
 Acq On : 31 Mar 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 31 11:39:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 10:07:03 2021
 Response via : Initial Calibration

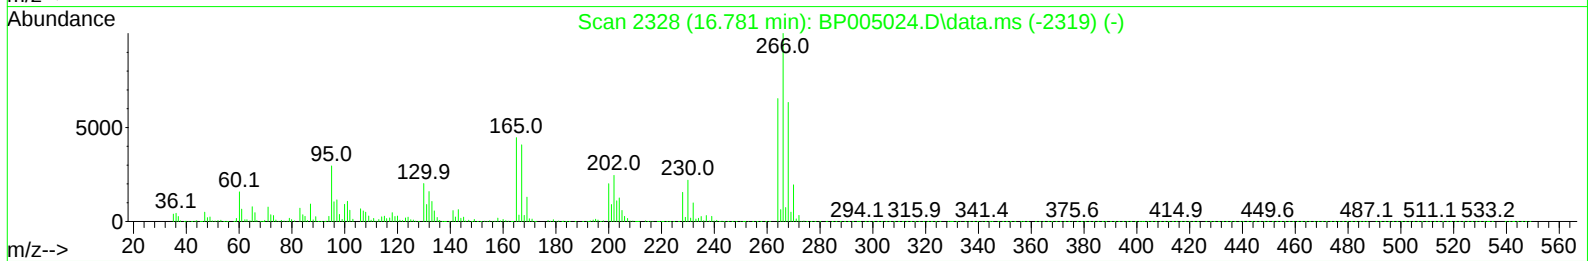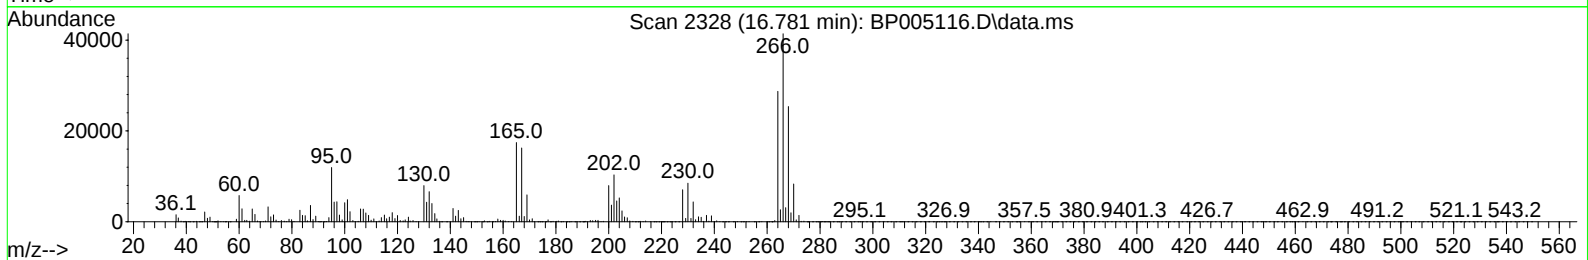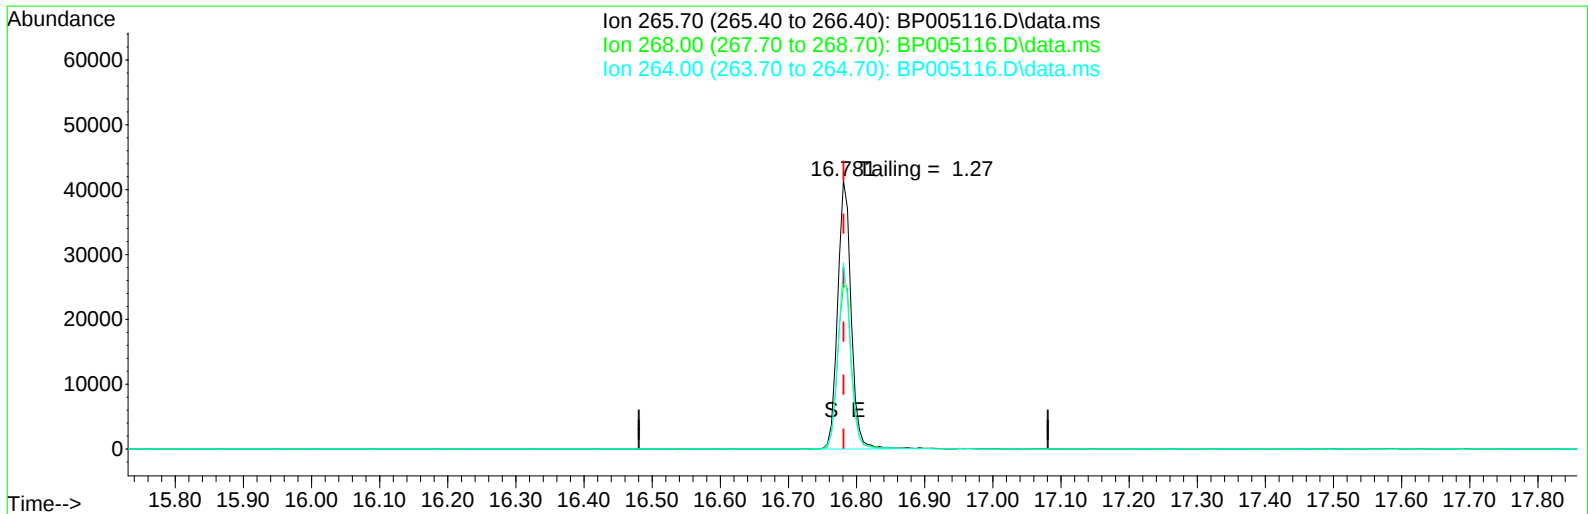

TIC: BP005116.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.000) 15473.55 ng




response 56841

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.27
264.00	63.30	69.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033121\
 Data File : BP005116.D
 Acq On : 31 Mar 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 31 11:39:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 10:07:03 2021
 Response via : Initial Calibration

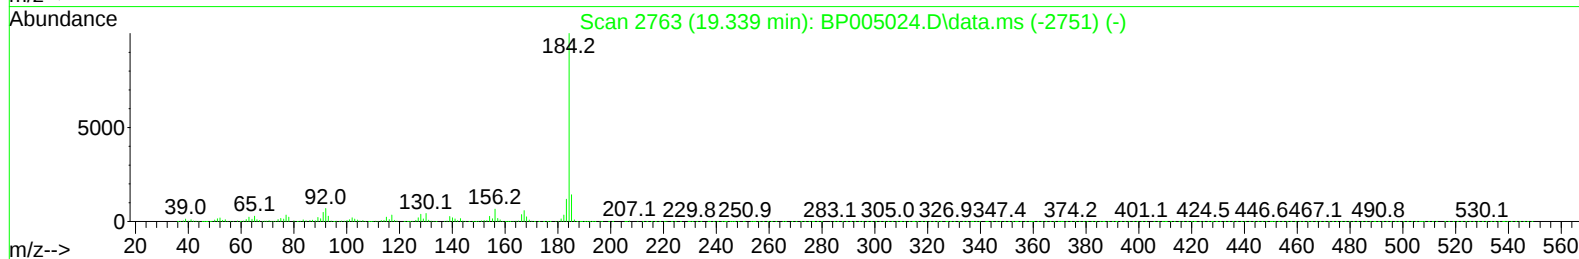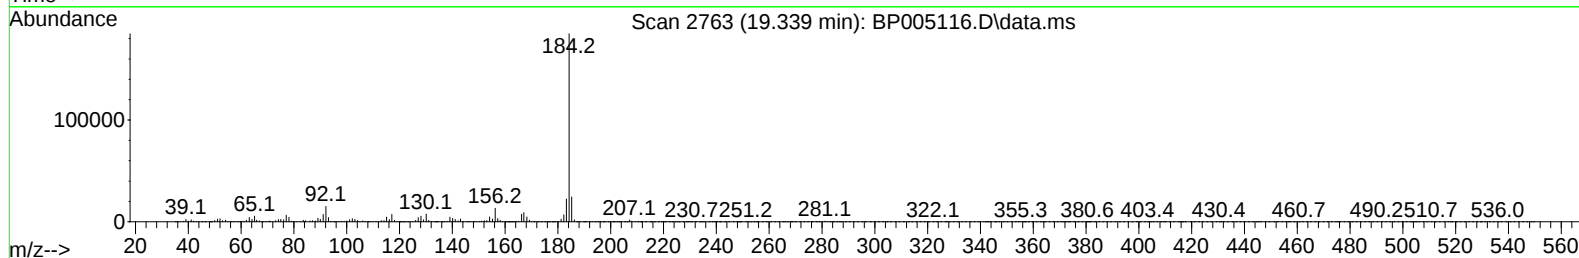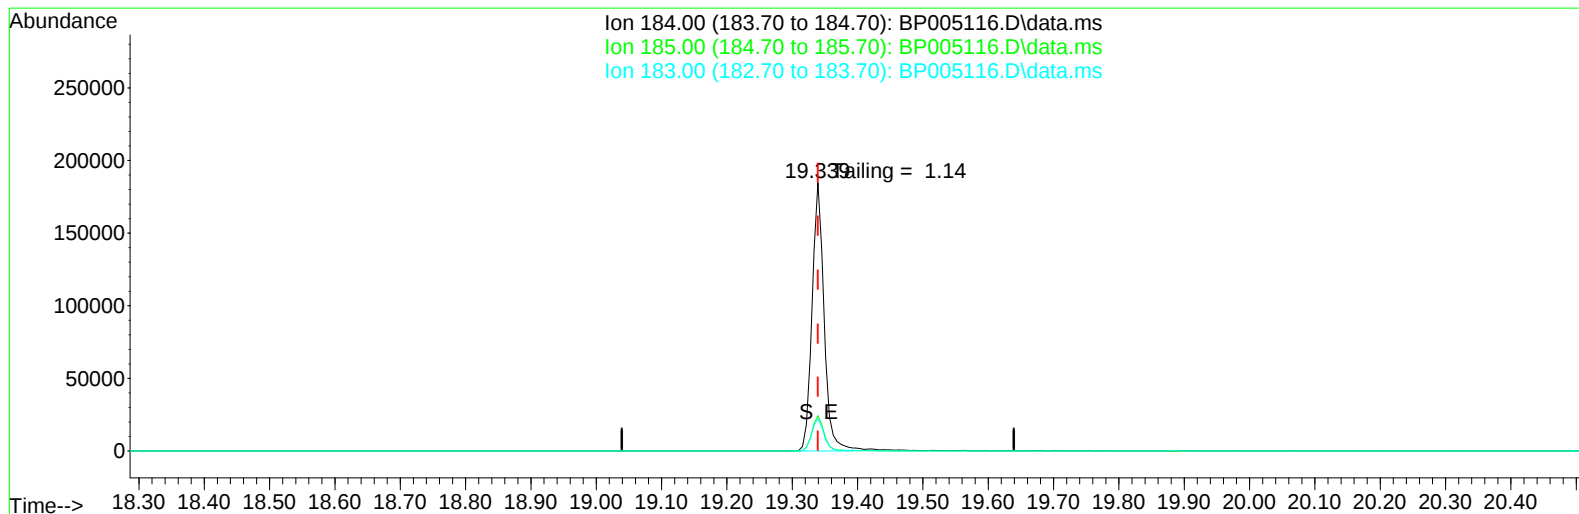

TIC: BP005116.D\data.ms

(77) Benzidine

19.339min (-0.000) 1688.04 ng

response 241290

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.18
183.00	12.00	12.05
0.00	0.00	0.00