
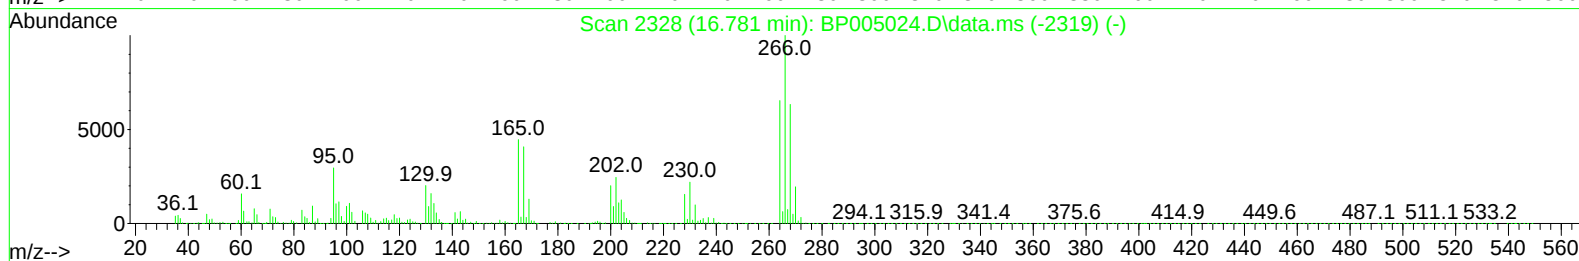
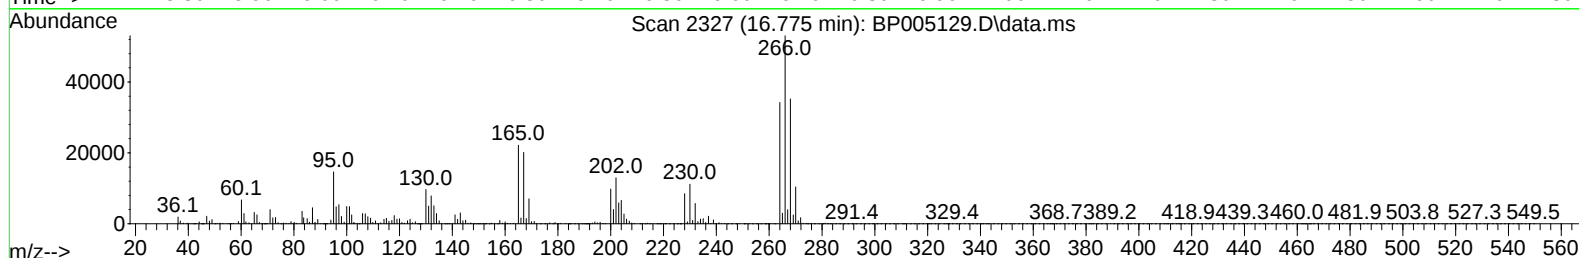


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
Data File : BP005129.D
Acq On : 01 Apr 2021 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 11:12:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 10:07:03 2021
Response via : Initial Calibration

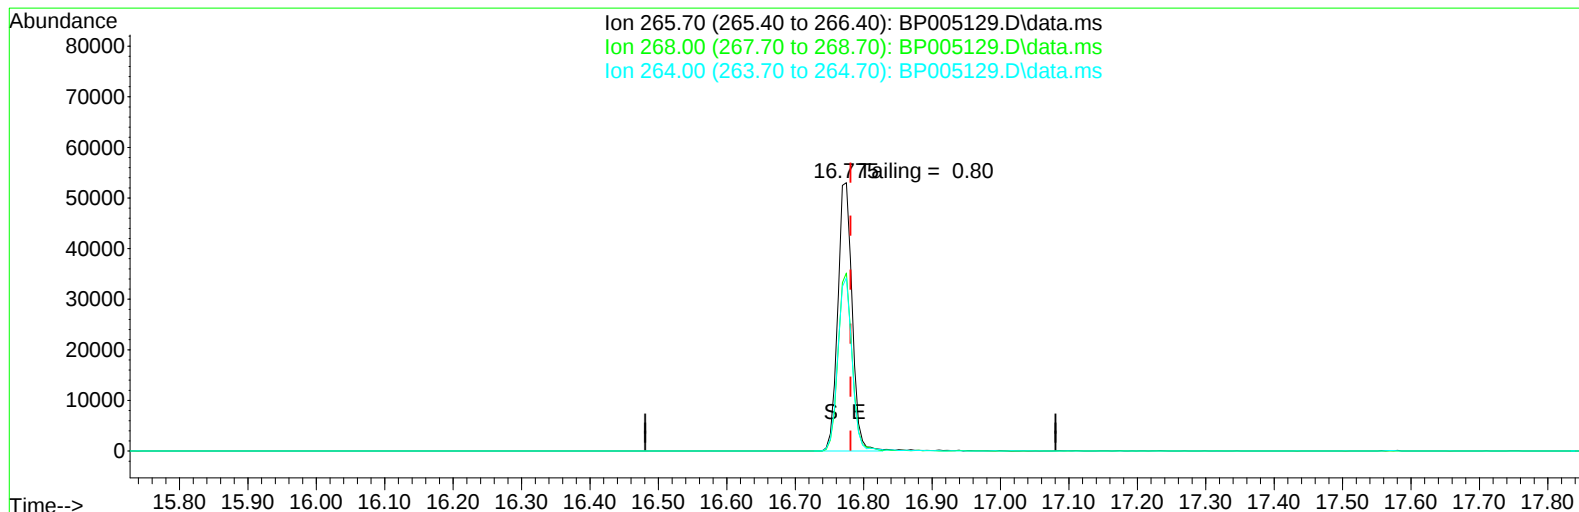

TIC: BP005129.D\data.ms

(70) Pentachlorophenol (C)




16.775min (-0.006) 818626.36 ng

response 77468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	66.38
264.00	63.30	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
 Data File : BP005129.D
 Acq On : 01 Apr 2021 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 11:12:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 10:07:03 2021
 Response via : Initial Calibration

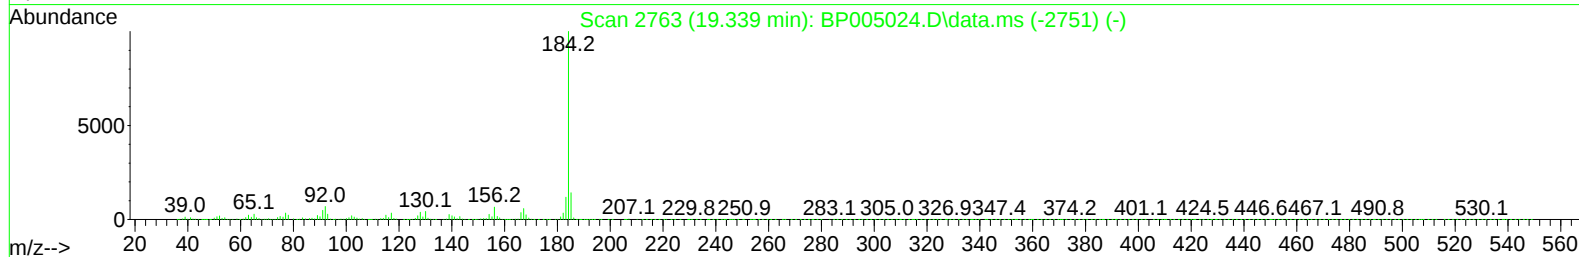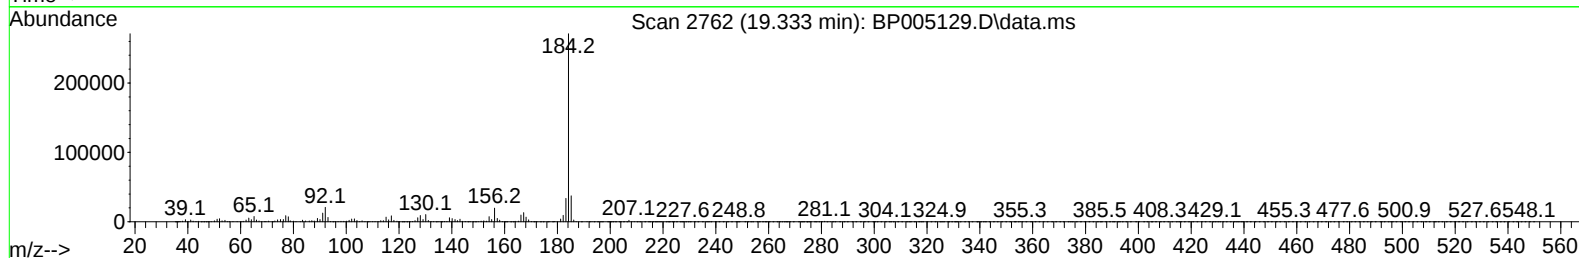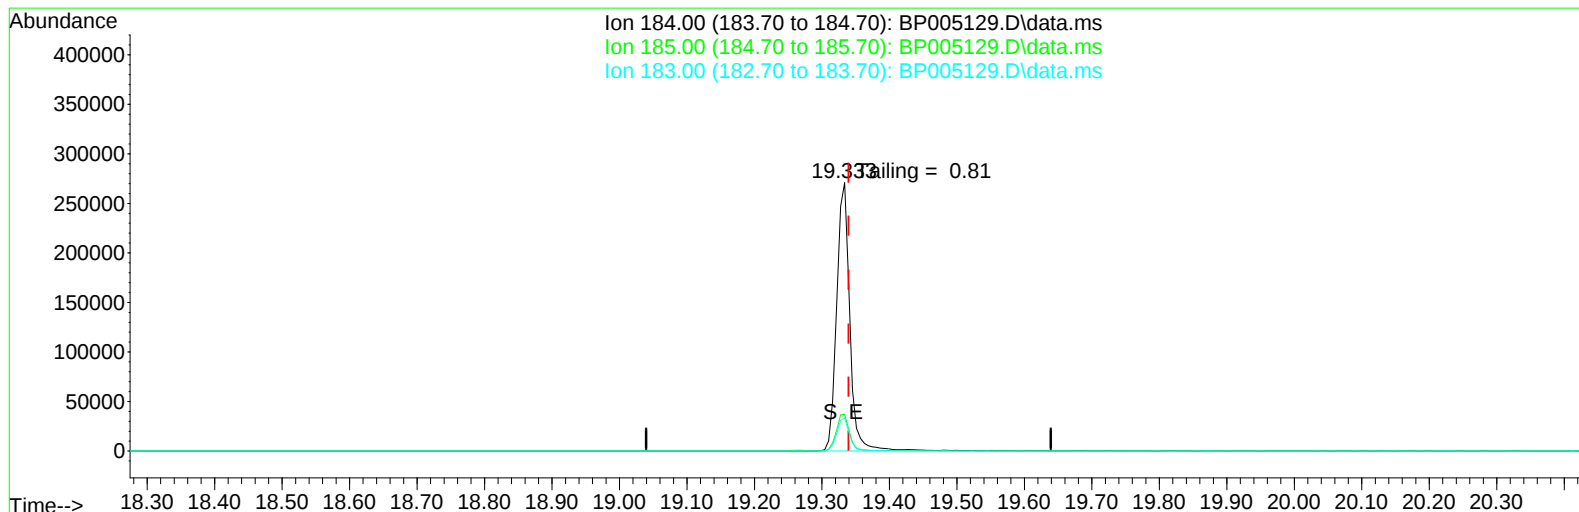

TIC: BP005129.D\data.ms

(77) Benzidine**19.333min (-0.006) 296815.20 ng****response 364683**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.75
183.00	12.00	12.45
0.00	0.00	0.00