

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
 Data File : BP005131.D
 Acq On : 01 Apr 2021 12:17
 Operator : CG/JU
 Sample : PB135470BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135470BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.305	371	377	386	rBV	605400	835415	44.34%	10.526%
2	6.887	634	646	657	rBV	543909	834511	44.30%	10.514%
3	7.705	779	785	795	rVB	99990	161999	8.60%	2.041%
4	8.869	976	983	992	rBV	308363	522186	27.72%	6.579%
5	10.499	1253	1260	1269	rBV	126303	211205	11.21%	2.661%
6	12.981	1675	1682	1690	rBV	762143	1125845	59.76%	14.185%
7	14.363	1910	1917	1925	rBV	186438	275054	14.60%	3.465%
8	15.863	2165	2172	2188	rBV	613097	878460	46.63%	11.068%
9	17.122	2380	2386	2395	rBV	239326	340276	18.06%	4.287%
10	18.022	2535	2539	2550	rBV6	10736	19695	1.05%	0.248%
11	19.698	2818	2824	2832	rBV	1585299	1883948	100.00%	23.736%
12	20.957	3034	3038	3041	rBV2	15402	19099	1.01%	0.241%
13	21.004	3043	3046	3051	rVV	21535	28155	1.49%	0.355%
14	21.222	3078	3083	3089	rBV	326644	399649	21.21%	5.035%
15	23.504	3465	3471	3479	rVB2	207900	401471	21.31%	5.058%




Sum of corrected areas: 7936968

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
Data File : BP005131.D
Acq On : 01 Apr 2021 12:17
Operator : CG/JU
Sample : PB135470BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135470BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

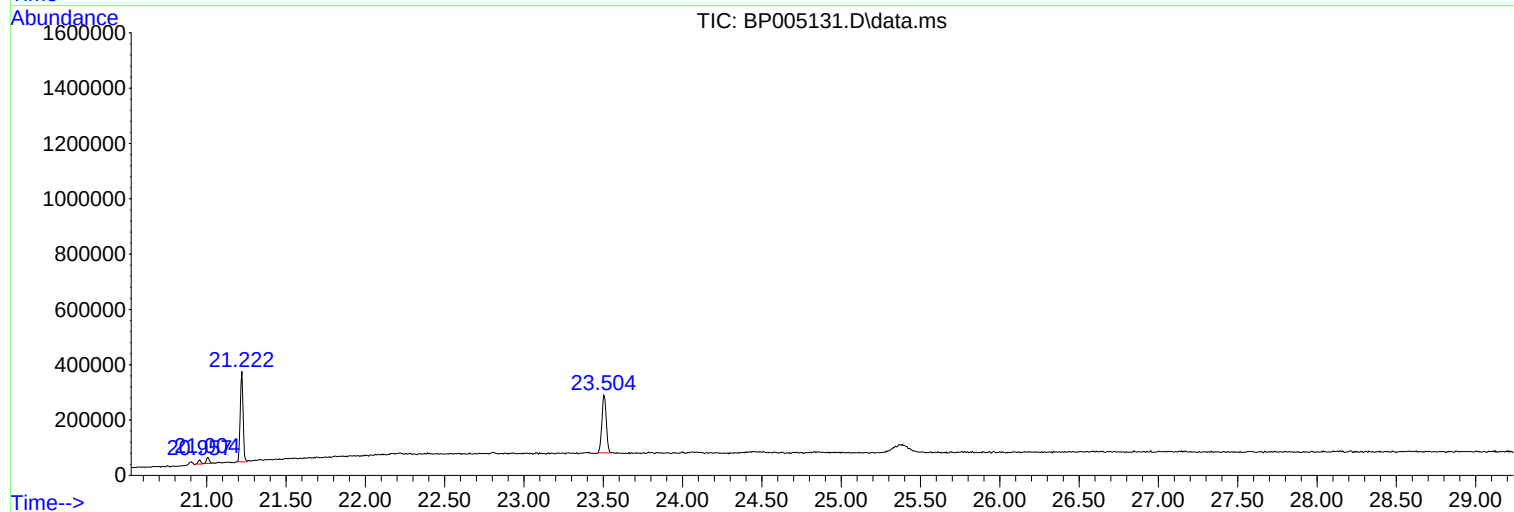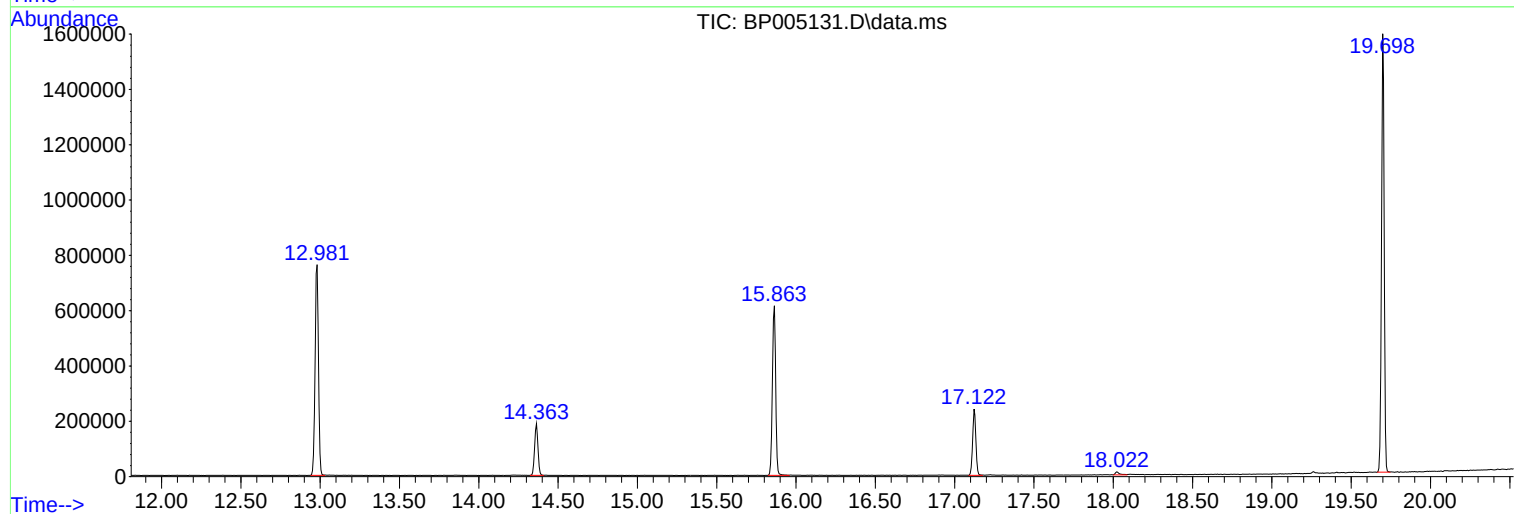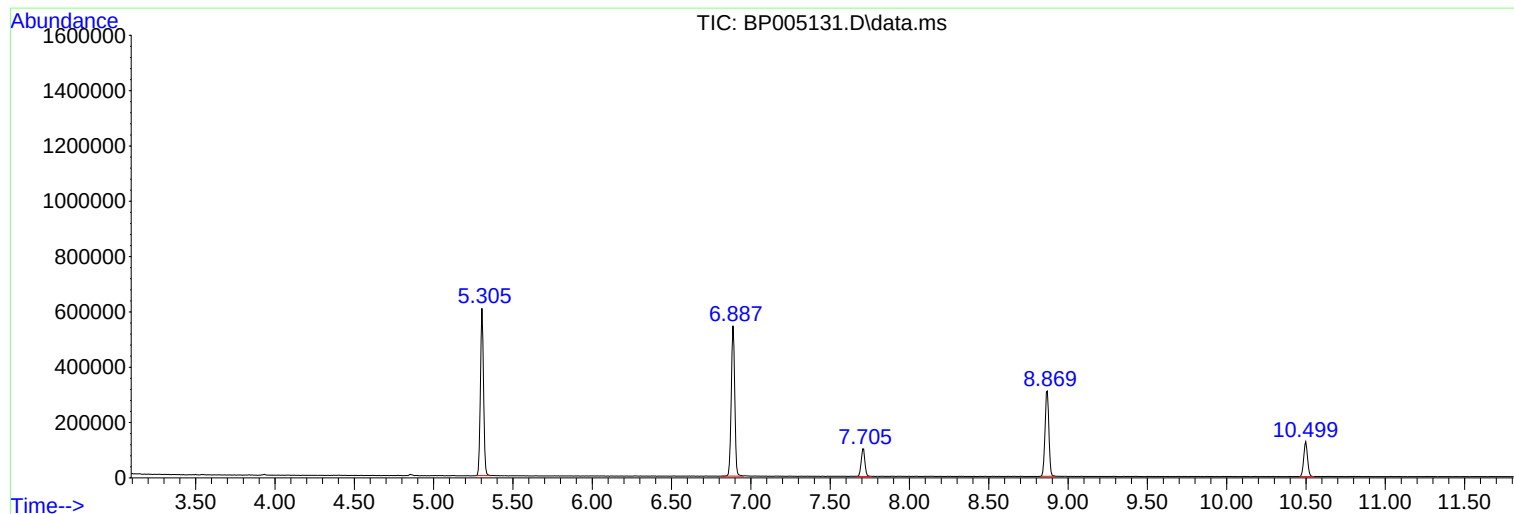

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
Data File : BP005131.D
Acq On : 01 Apr 2021 12:17
Operator : CG/JU
Sample : PB135470BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135470BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
Data File : BP005131.D
Acq On : 01 Apr 2021 12:17
Operator : CG/JU
Sample : PB135470BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135470BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------