
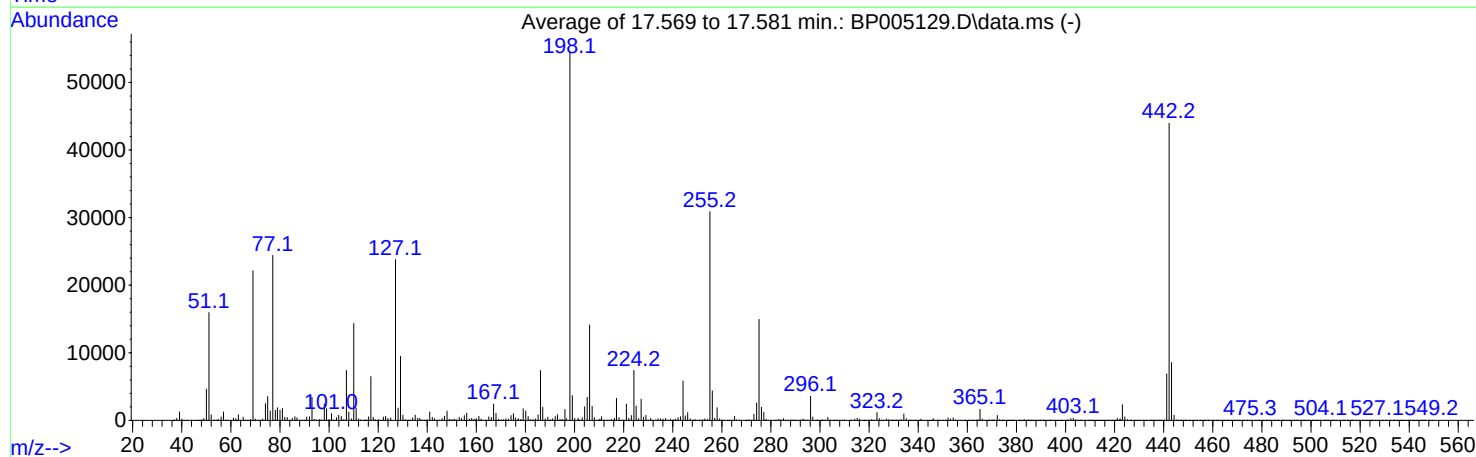


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
 Data File : BP005129.D
 Acq On : 01 Apr 2021 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 01 12:23:57 2021

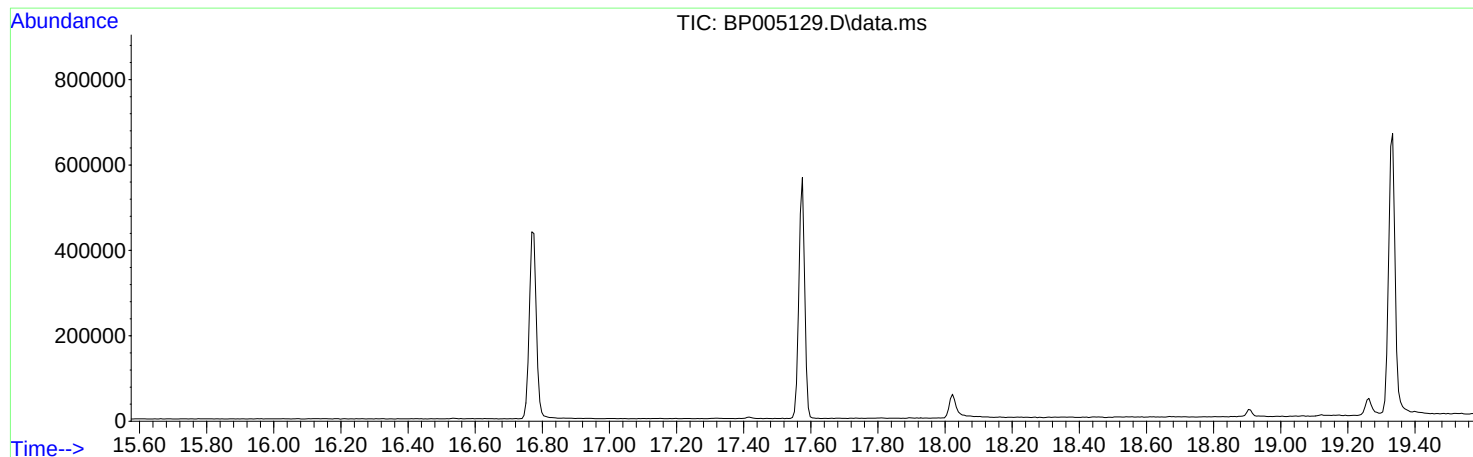




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	15958	PASS
68	69	0.00	2	0.5	117	PASS
69	198	0.00	100	40.7	22132	PASS
70	69	0.00	2	0.8	186	PASS
127	198	10	80	43.7	23795	PASS
197	198	0.00	2	0.4	237	PASS
198	198	100	100	100.0	54429	PASS
199	198	5	9	6.7	3636	PASS
275	198	10	60	27.5	14949	PASS
365	198	1	100	3.0	1640	PASS
441	198	0.01	100	12.6	6869	PASS
442	442	100	100	100.0	43965	PASS
443	442	15	24	19.4	8536	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
Data File : BP005129.D
Acq On : 01 Apr 2021 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 01 11:12:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 10:07:03 2021
Response via : Initial Calibration

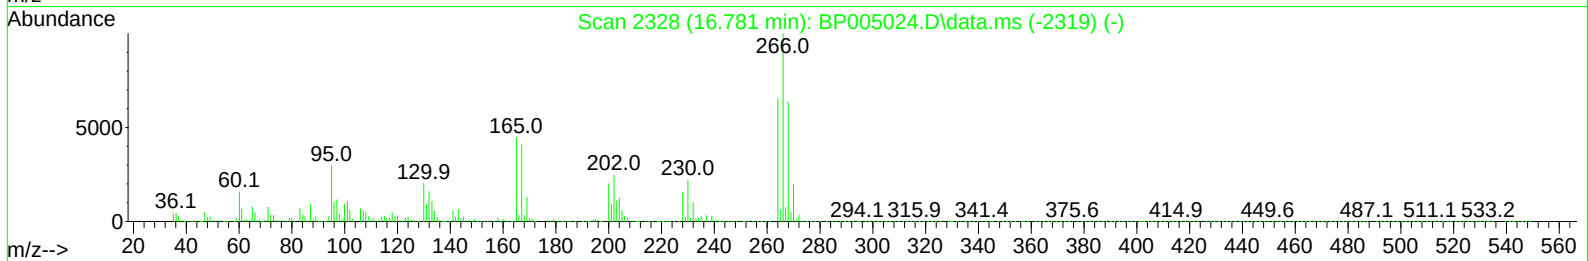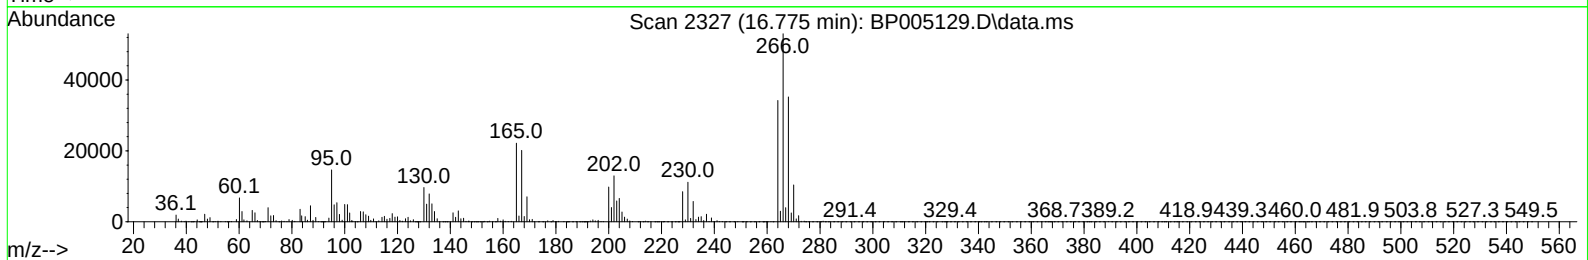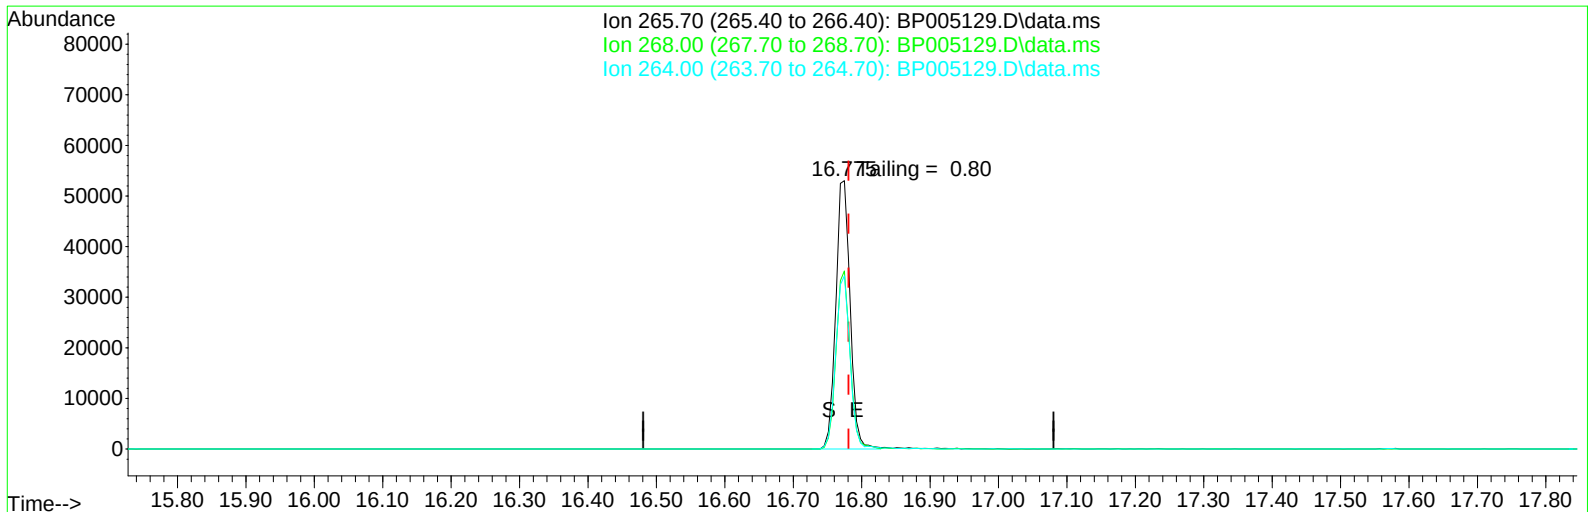

TIC: BP005129.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.006) 818626.36 ng




response 77468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	66.38
264.00	63.30	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040121\
 Data File : BP005129.D
 Acq On : 01 Apr 2021 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 11:12:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 10:07:03 2021
 Response via : Initial Calibration

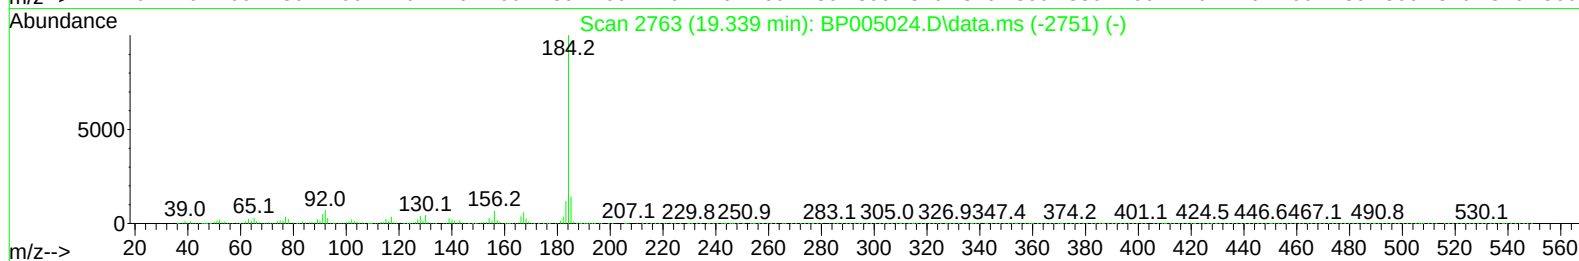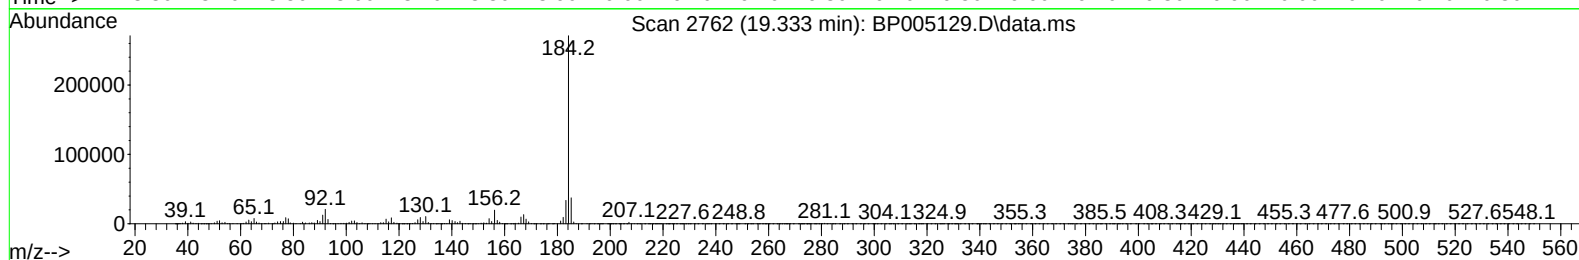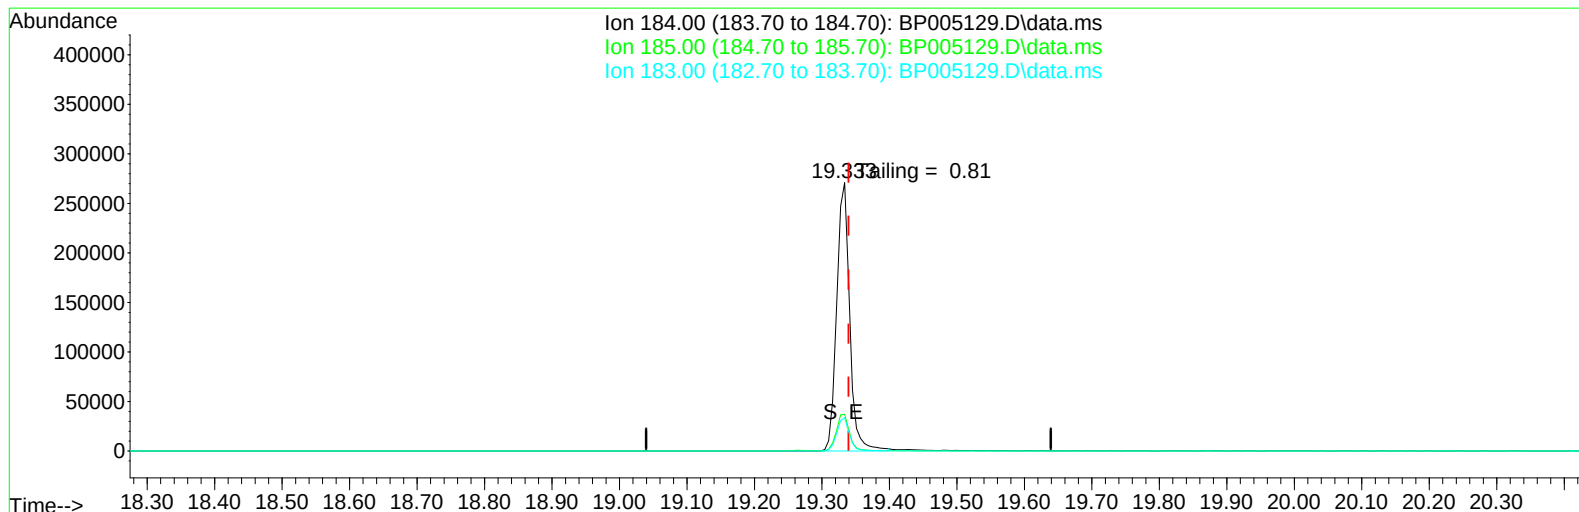

TIC: BP005129.D\data.ms

(77) Benzidine

19.333min (-0.006) 296815.20 ng

response 364683

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.75
183.00	12.00	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/1/2021	BNA_P	BP005129.D
Compound Name	Response	Retention Time
DDT	204209	20.53
DDD	3303	20.1
DDE	398	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3701	207910	1.78

Instrument :
BNA_P
ClientSampleId :
DFTPP