

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040122\
 Data File : BP009653.D
 Acq On : 01 Apr 2022 12:14
 Operator : CG/JU
 Sample : PB143765BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143765BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.340	393	400	428	rBV	4340828	7642992	51.19%	11.154%
2	6.928	662	670	701	rBV	4057991	7640040	51.17%	11.149%
3	7.728	799	806	824	rBV	835797	1513428	10.14%	2.209%
4	8.893	994	1004	1023	rBV	2539548	4990669	33.43%	7.283%
5	10.522	1273	1281	1309	rBV	913942	1884192	12.62%	2.750%
6	12.999	1693	1702	1722	rBV	6802387	10850807	72.68%	15.835%
7	14.381	1930	1937	1958	rVB	1420094	2488576	16.67%	3.632%
8	15.887	2184	2193	2217	rBV	4598016	7834233	52.47%	11.433%
9	17.151	2401	2408	2423	rBV	1681409	2883026	19.31%	4.207%
10	19.733	2841	2847	2857	rBV	11501905	14929839	100.00%	21.787%
11	21.269	3103	3108	3119	rBV	2071375	3135007	21.00%	4.575%
12	23.645	3506	3512	3526	rVB2	1188549	2732041	18.30%	3.987%




Sum of corrected areas: 68524850

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040122\
Data File : BP009653.D
Acq On : 01 Apr 2022 12:14
Operator : CG/JU
Sample : PB143765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

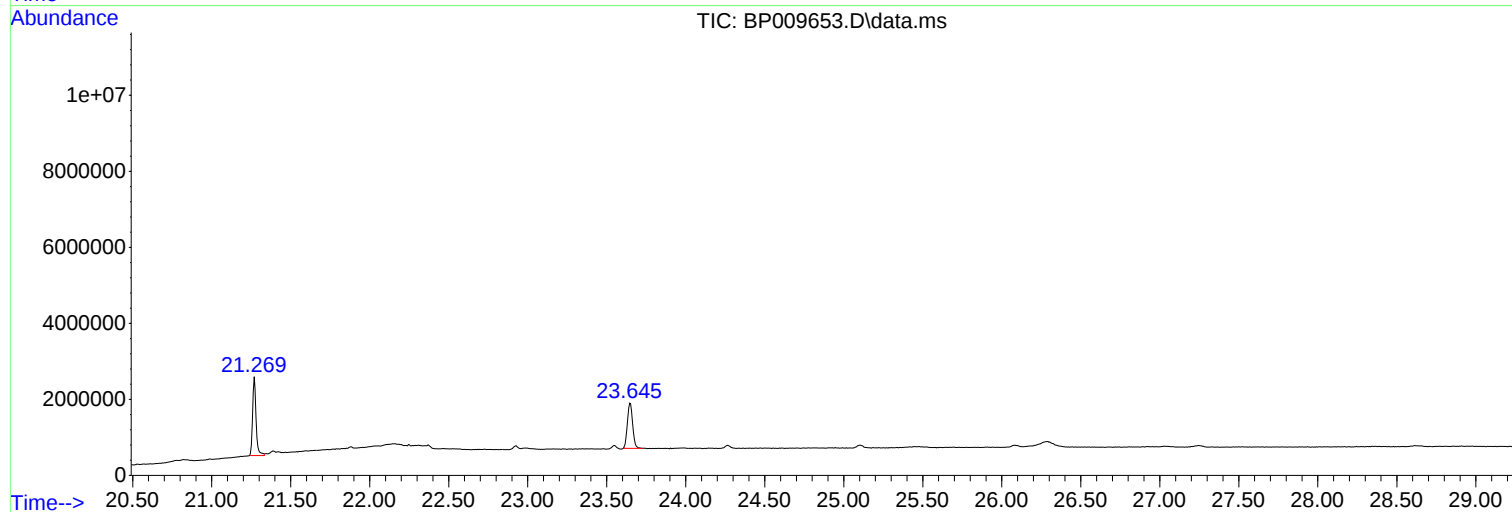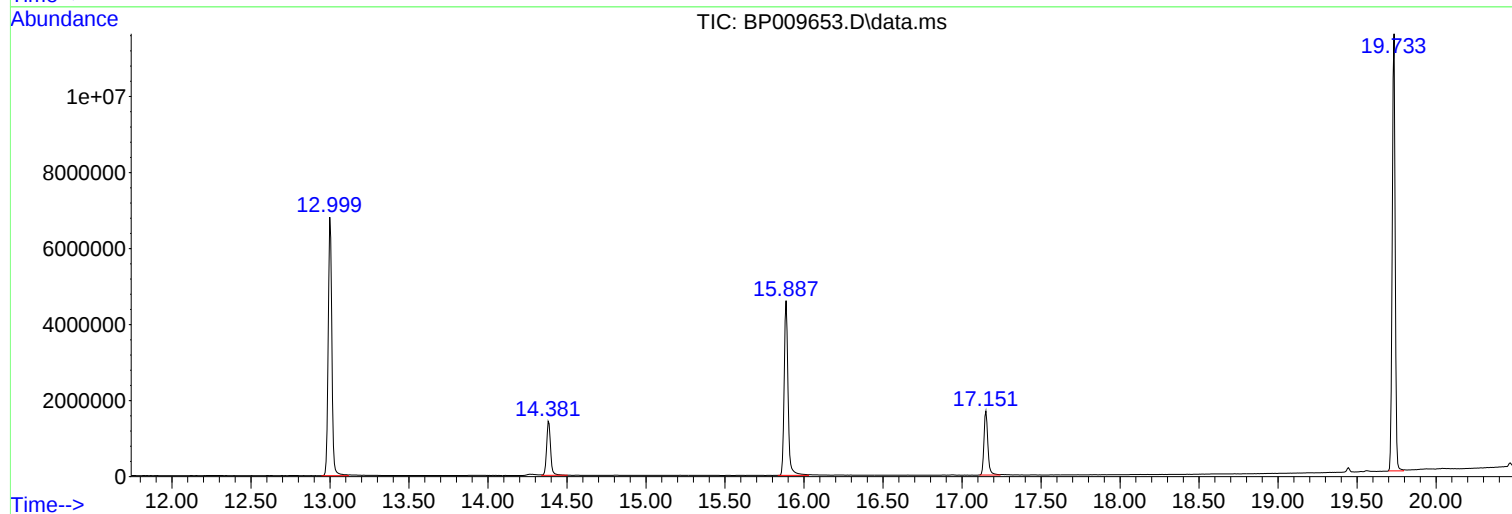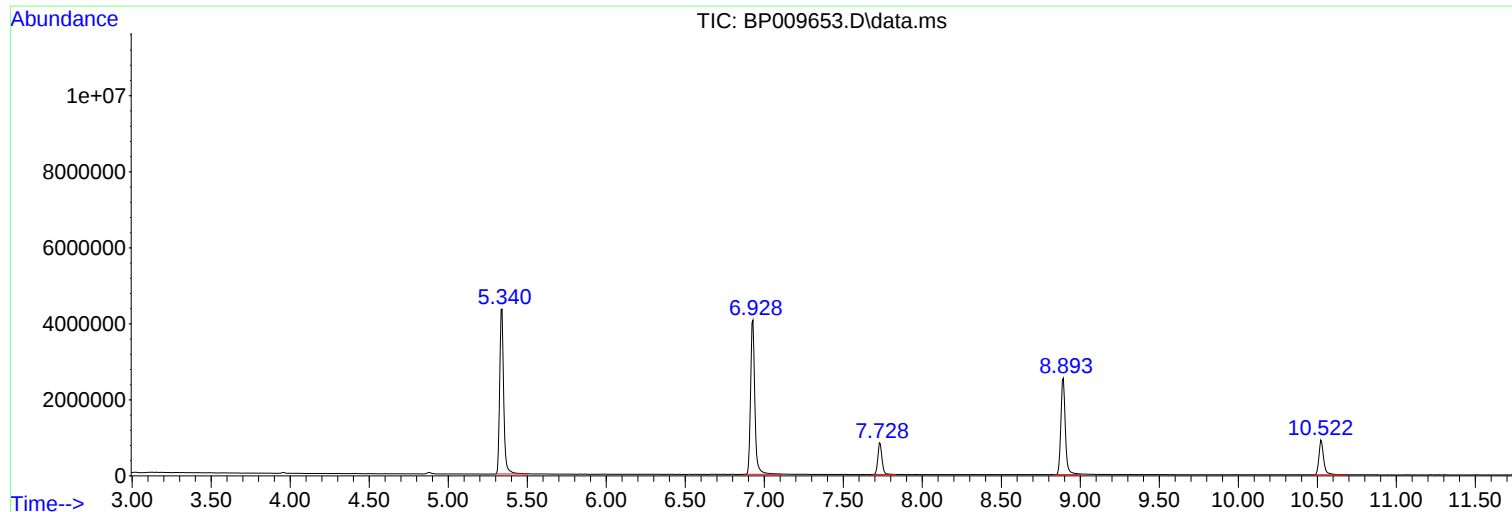

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040122\
Data File : BP009653.D
Acq On : 01 Apr 2022 12:14
Operator : CG/JU
Sample : PB143765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040122\
Data File : BP009653.D
Acq On : 01 Apr 2022 12:14
Operator : CG/JU
Sample : PB143765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------