
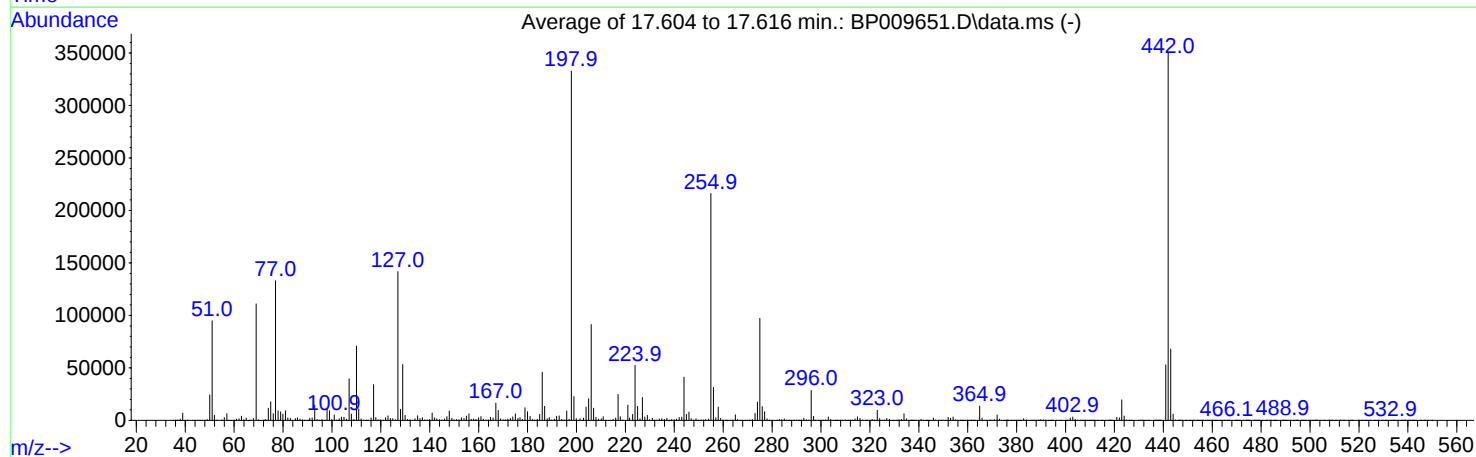


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040122\  
 Data File : BP009651.D  
 Acq On : 01 Apr 2022 10:29  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Mar 31 04:36:51 2022

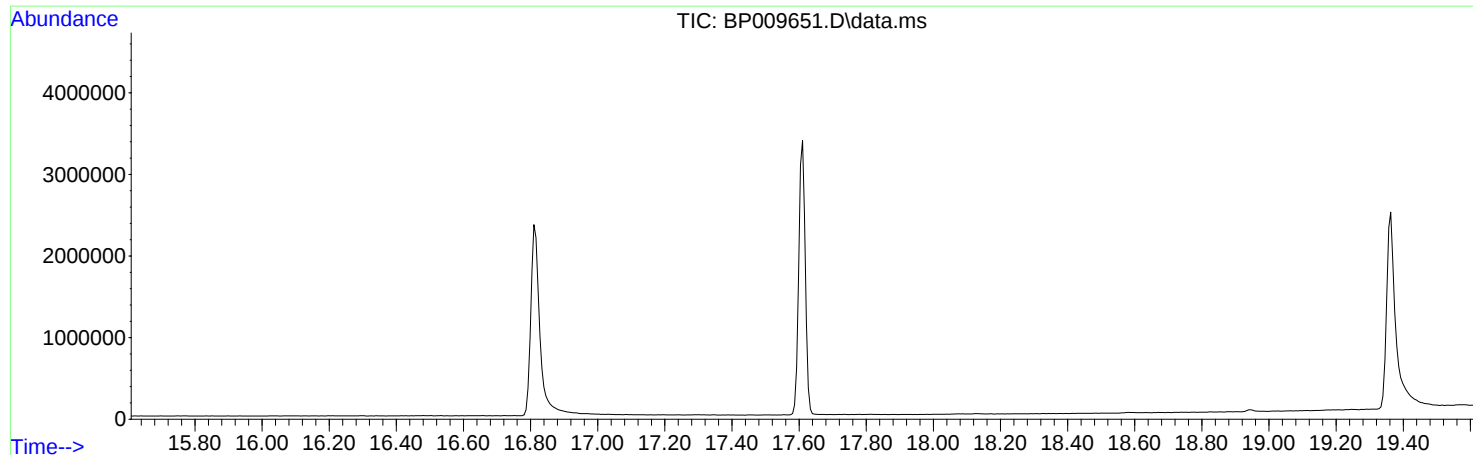




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 28.5         | 94836      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 1654       | PASS                |
| 69             | 198             | 0.00            | 100             | 33.4         | 111022     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 575        | PASS                |
| 127            | 198             | 10              | 80              | 42.6         | 141800     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 1024       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 332772     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 22792      | PASS                |
| 275            | 198             | 10              | 60              | 29.2         | 97103      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 13539      | PASS                |
| 441            | 198             | 0.01            | 100             | 15.9         | 52909      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 350488     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 67979      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040122\  
Data File : BP009651.D  
Acq On : 01 Apr 2022 10:29  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Apr 01 23:39:22 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 31 04:36:51 2022  
Response via : Initial Calibration

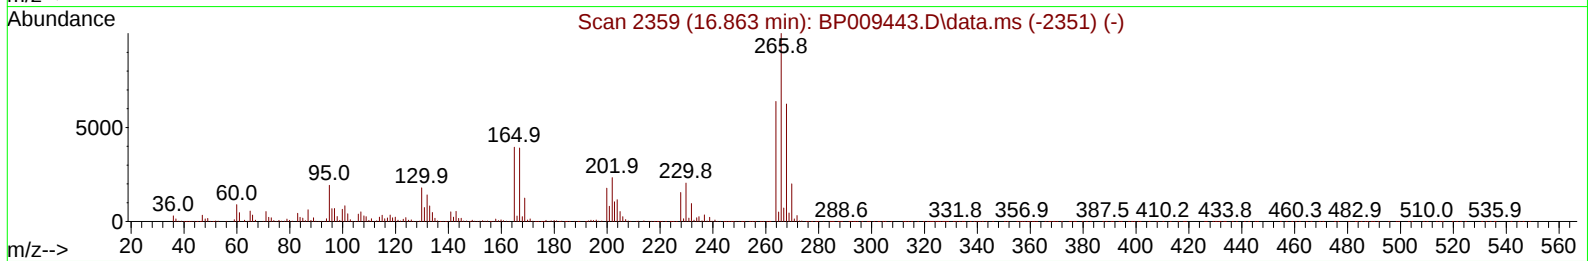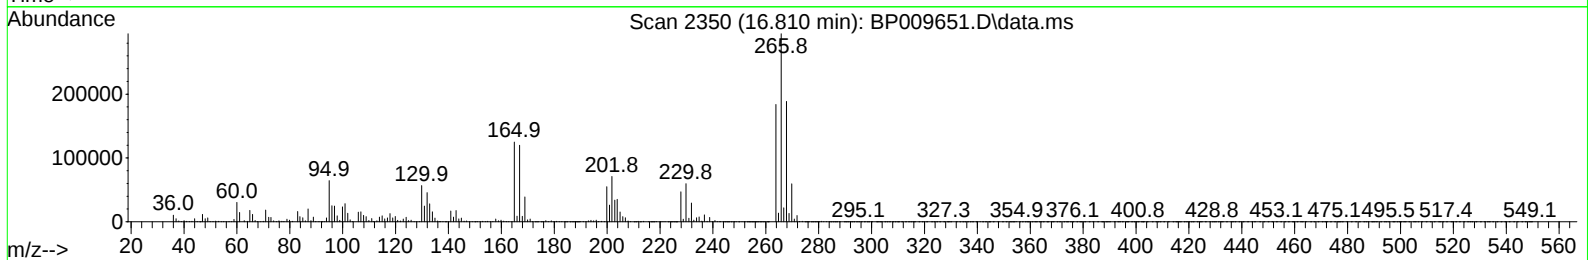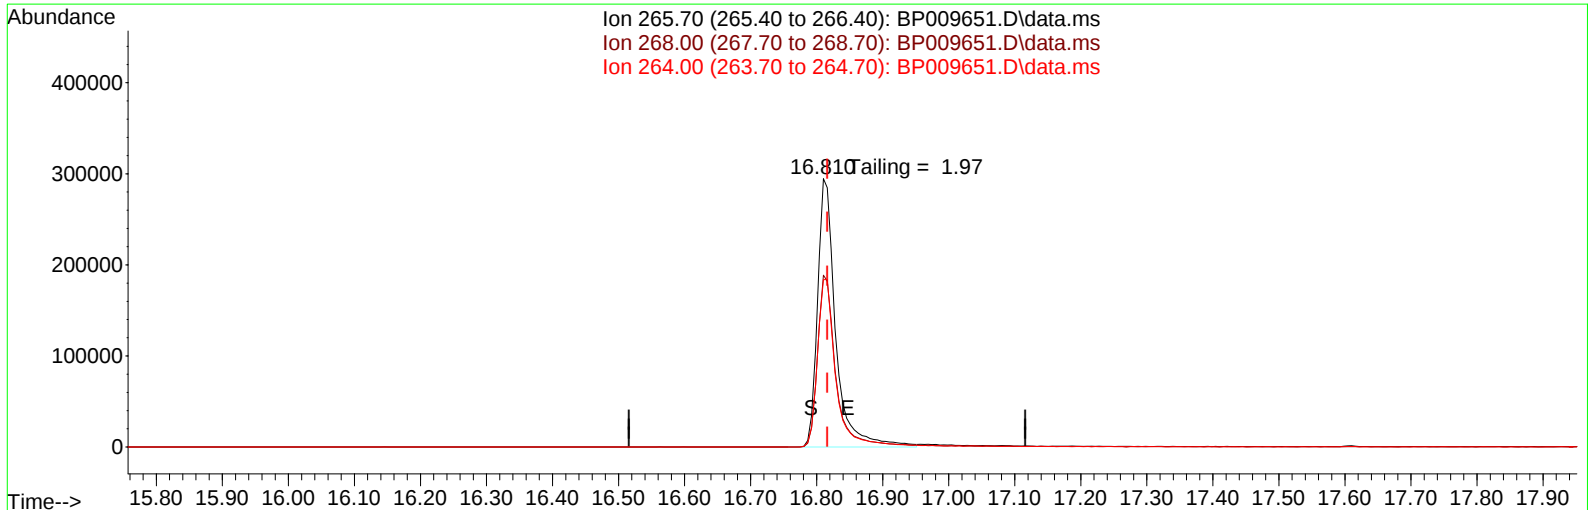

TIC: BP009651.D\data.ms

**(70) Pentachlorophenol (C)**

**16.810min (-0.006) 377135.50 ng**




**response 564993**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.30  | 64.04  |
| 264.00 | 63.60  | 62.39  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040122\  
 Data File : BP009651.D  
 Acq On : 01 Apr 2022 10:29  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 01 23:39:22 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Mar 31 04:36:51 2022  
 Response via : Initial Calibration

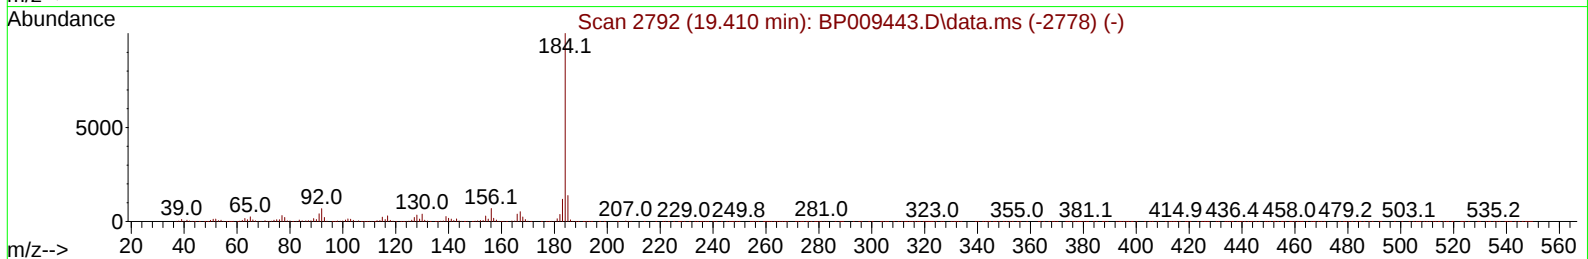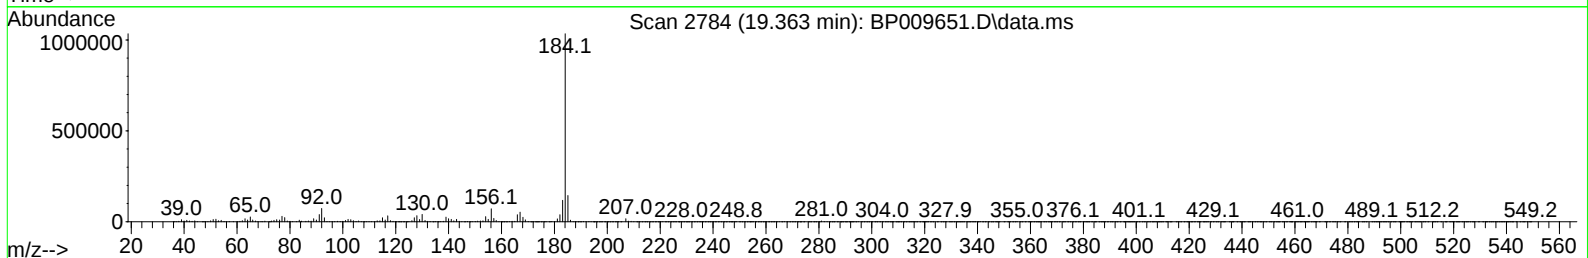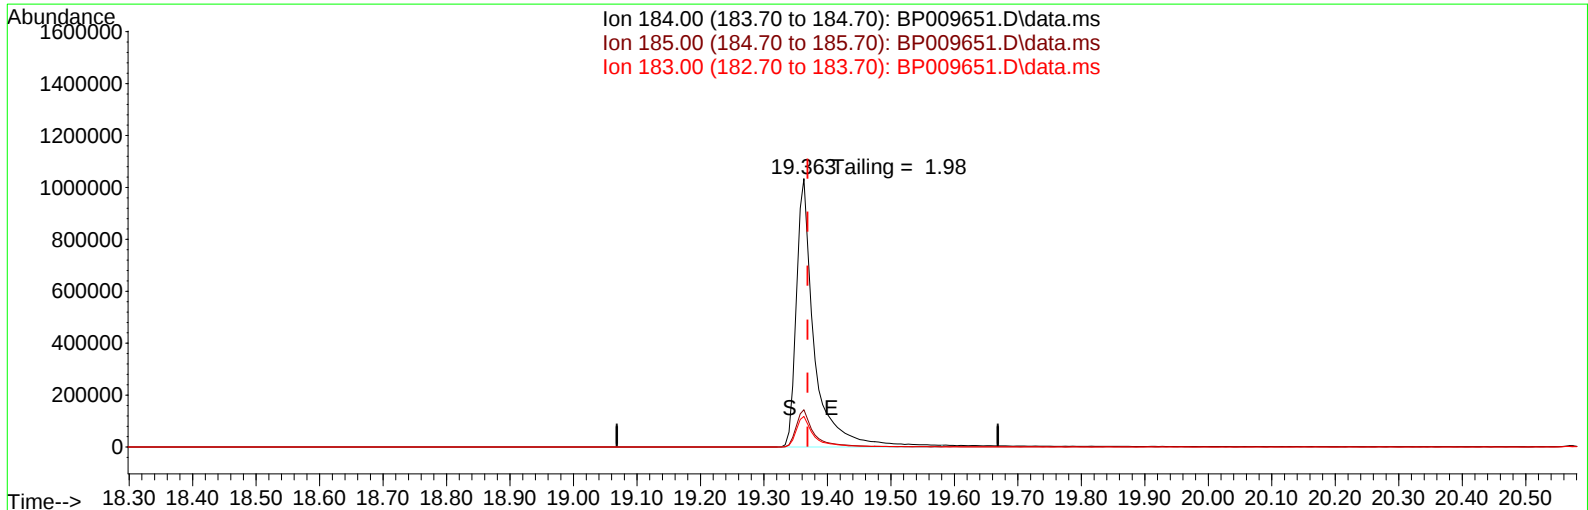

TIC: BP009651.D\data.ms

**(77) Benzidine**

**19.363min (-0.006) 162918.85 ng**

**response 2052585**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 13.93  |
| 183.00 | 11.70  | 11.40  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/1/2022      | BNA_P            | <u>BP009651.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1140651          | 20.569             |
| DDD           | 21672            | 20.145             |
| DDE           | 2482             | 19.639             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 24154         | 1164805          | 2.07               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP