

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040125\
 Data File : BP024206.D
 Acq On : 01 Apr 2025 10:37
 Operator : RC/JU
 Sample : PB166622BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	40	rVB	113081	157438	1.47%	0.149%
2	3.675	96	100	121	rBV	1370315	2114843	19.81%	2.000%
3	3.993	150	154	160	rVB	42144	60220	0.56%	0.057%
4	6.922	642	652	665	rBV	1734821	2616129	24.51%	2.475%
5	7.081	672	679	691	rBV	1416877	2197979	20.59%	2.079%
6	7.281	706	713	724	rBV	1764512	2657616	24.90%	2.514%
7	7.740	781	791	801	rBV	1256217	1975552	18.51%	1.869%
8	8.446	902	911	933	rBV	2122649	3360844	31.49%	3.179%
9	8.893	979	987	999	rBV	1467130	2472429	23.16%	2.339%
10	9.604	1099	1108	1131	rBV	1248025	1969675	18.45%	1.863%
11	10.146	1192	1200	1219	rBV	1919168	3186827	29.86%	3.014%
12	10.522	1256	1264	1277	rVB	1904360	2994744	28.06%	2.833%
13	10.657	1277	1287	1302	rBV	1823458	3384518	31.71%	3.201%
14	11.181	1369	1376	1384	rBV4	9364	20420	0.19%	0.019%
15	12.116	1526	1535	1543	rBV2	30454	60713	0.57%	0.057%
16	13.357	1737	1746	1753	rVB	49437	71412	0.67%	0.068%
17	13.787	1809	1819	1830	rBV	3771079	5242237	49.11%	4.959%
18	14.069	1859	1867	1882	rBV2	4138620	6213871	58.22%	5.878%
19	14.381	1912	1920	1930	rBV	2869618	4250728	39.82%	4.021%
20	14.592	1949	1956	1972	rBV	1376286	2207428	20.68%	2.088%
21	14.804	1988	1992	2001	rVB6	9239	18780	0.18%	0.018%
22	15.386	2084	2091	2099	rBV	5413538	7805669	73.13%	7.383%
23	15.510	2106	2112	2127	rBV	1589351	2214664	20.75%	2.095%
24	15.628	2129	2132	2140	rVB	25437	46424	0.43%	0.044%
25	16.122	2212	2216	2222	rVB6	7220	12633	0.12%	0.012%
26	16.186	2222	2227	2234	rBV6	8404	14538	0.14%	0.014%
27	16.516	2279	2283	2288	rBV5	8929	12460	0.12%	0.012%
28	16.857	2336	2341	2346	rVB5	8379	12698	0.12%	0.012%
29	16.963	2354	2359	2364	rBV2	14261	26541	0.25%	0.025%
30	17.180	2390	2396	2406	rBV2	3648787	5121438	47.98%	4.844%
31	17.286	2407	2414	2437	rVB	5570828	8827082	82.70%	8.349%
32	17.886	2513	2516	2523	rVB7	13525	21864	0.20%	0.021%
33	18.127	2553	2557	2564	rBV2	31246	48395	0.45%	0.046%
34	19.210	2737	2741	2746	rBV	69773	98339	0.92%	0.093%
35	19.286	2749	2754	2759	rVV	59184	90460	0.85%	0.086%
36	19.369	2764	2768	2773	rVB2	97238	121008	1.13%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040125\
Data File : BP024206.D
Acq On : 01 Apr 2025 10:37
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Title : SVOA CALIBRATION

37	19.616	2806	2810	2813	rBV	225739	252400	2.36%	0.239%
38	19.669	2813	2819	2827	rVB	7865808	10673775	100.00%	10.096%
39	20.486	2955	2958	2962	rBV3	55507	74718	0.70%	0.071%
40	20.710	2993	2996	3002	rBV	165187	196272	1.84%	0.186%
41	21.639	3147	3154	3167	rBV	3488342	5896197	55.24%	5.577%
42	24.780	3679	3688	3704	rVB	4139336	10648088	99.76%	10.072%
43	25.015	3718	3728	3740	rVB	2112968	5829027	54.61%	5.514%
44	25.180	3753	3756	3768	rVB	239709	442323	4.14%	0.418%




Sum of corrected areas: 105721416

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040125\
Data File : BP024206.D
Acq On : 01 Apr 2025 10:37
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

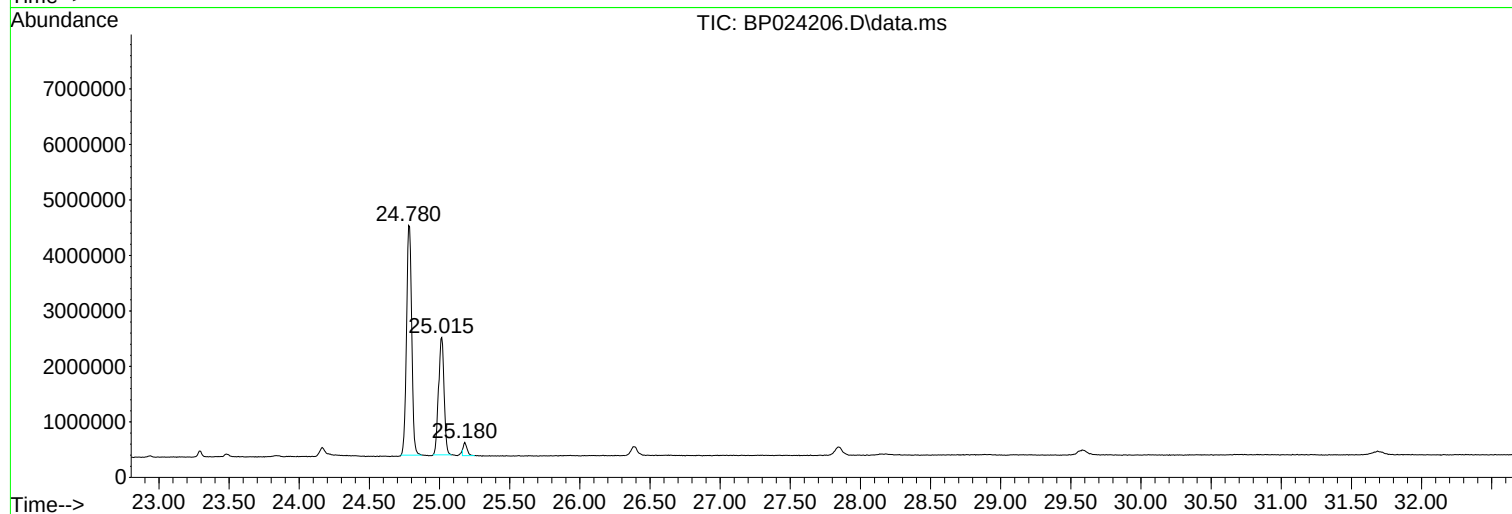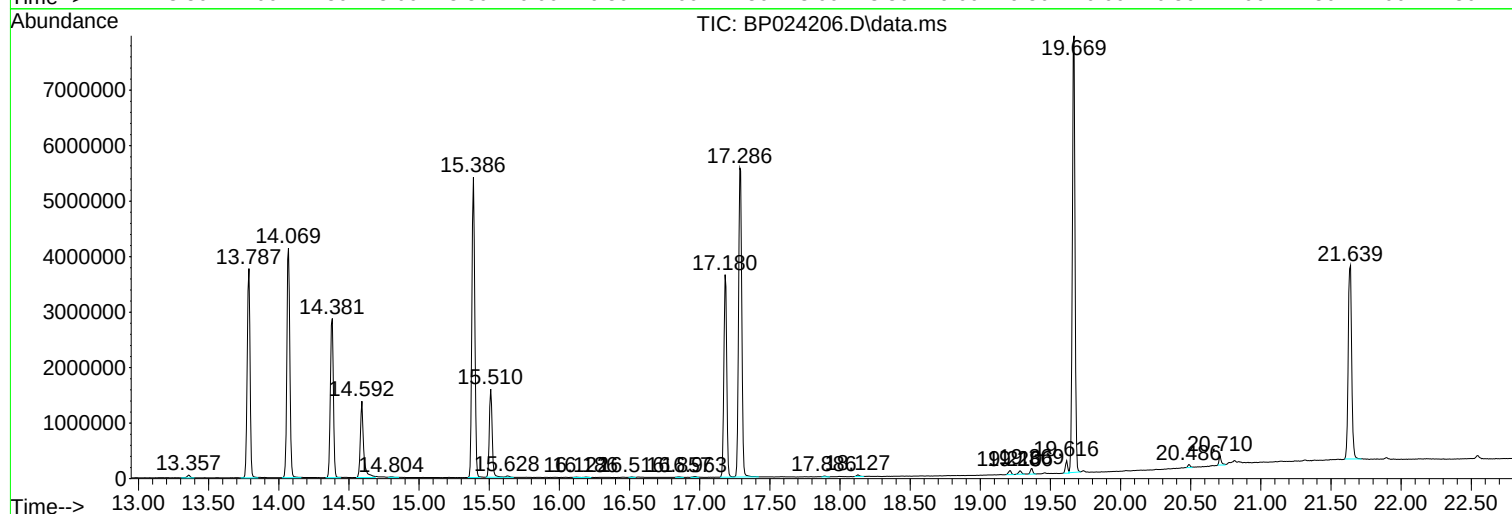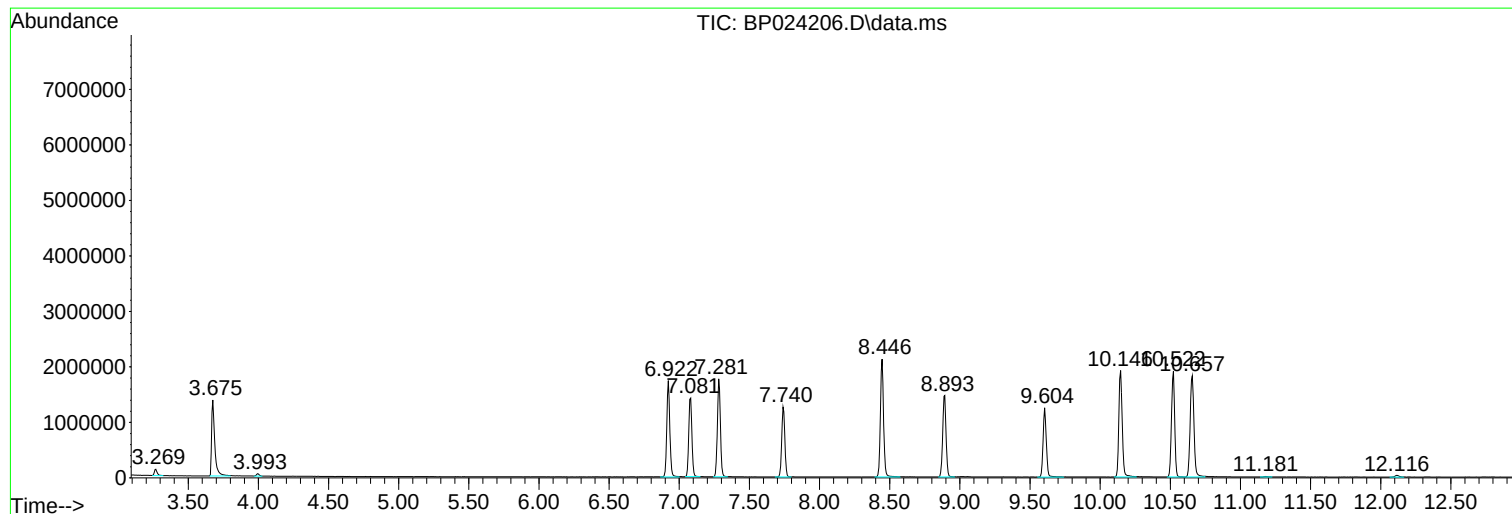

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040125\
Data File : BP024206.D
Acq On : 01 Apr 2025 10:37
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040125\
Data File : BP024206.D
Acq On : 01 Apr 2025 10:37
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------