
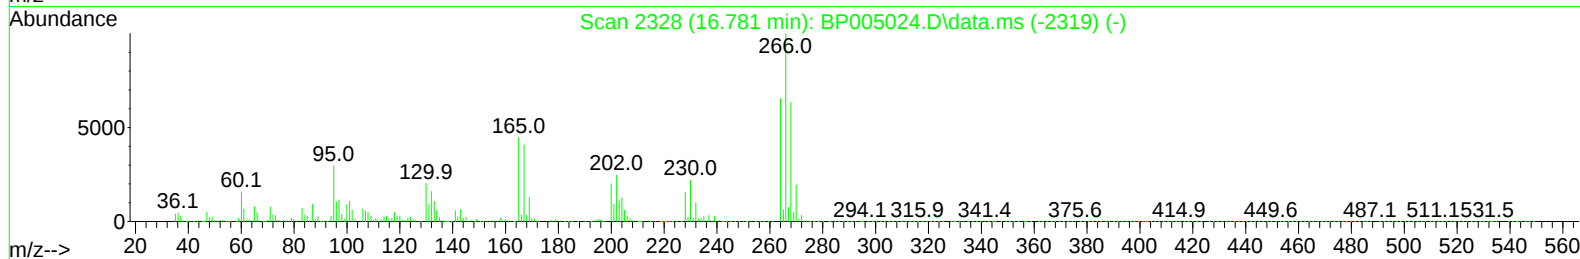
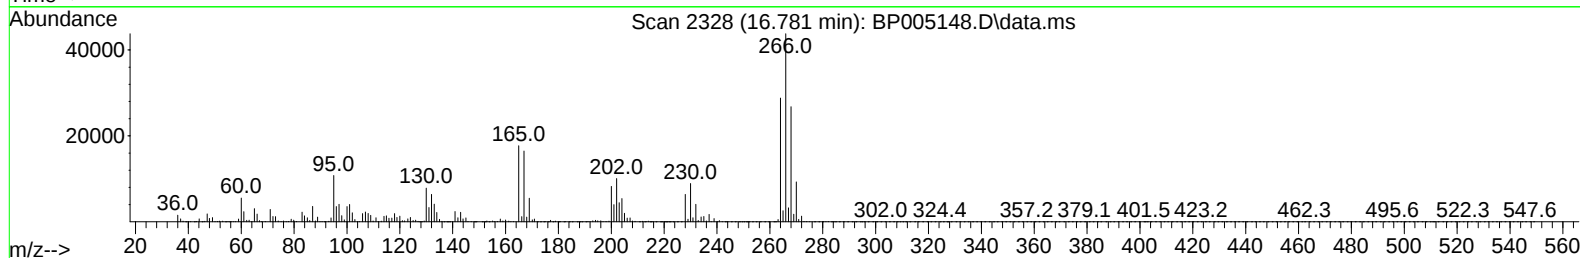


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
Data File : BP005148.D
Acq On : 02 Apr 2021 08:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 11:17:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration

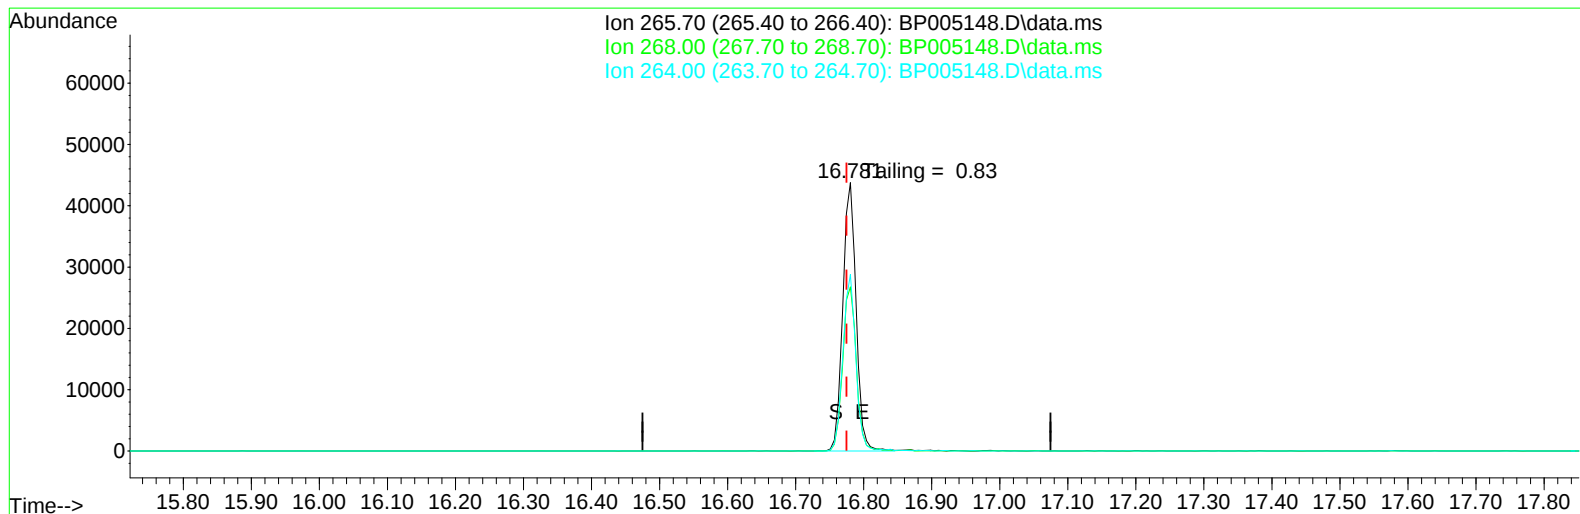

TIC: BP005148.D\data.ms

(70) Pentachlorophenol (C)




16.781min (+ 0.006) 55808.38 ng

response 59534

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.17
264.00	63.30	65.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
Data File : BP005148.D
Acq On : 02 Apr 2021 08:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 11:17:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration

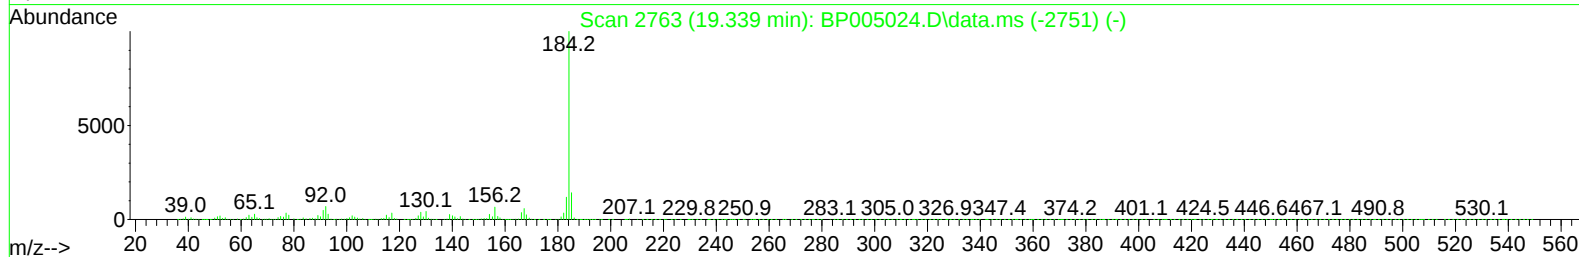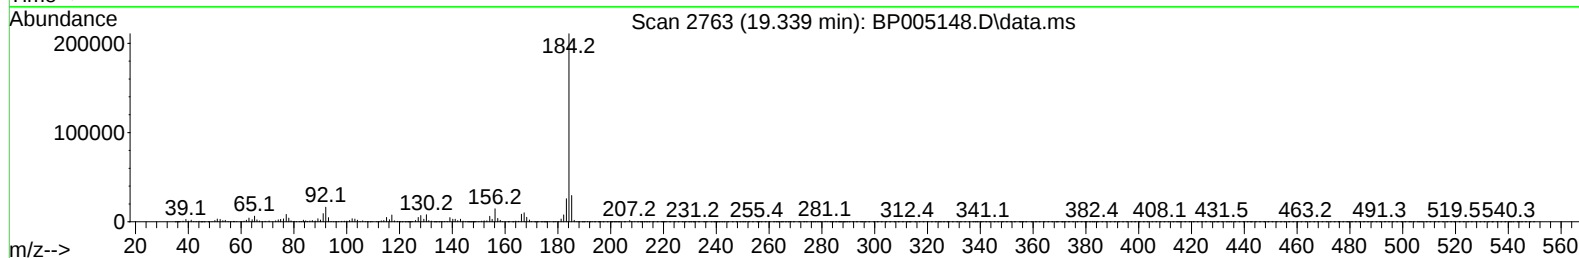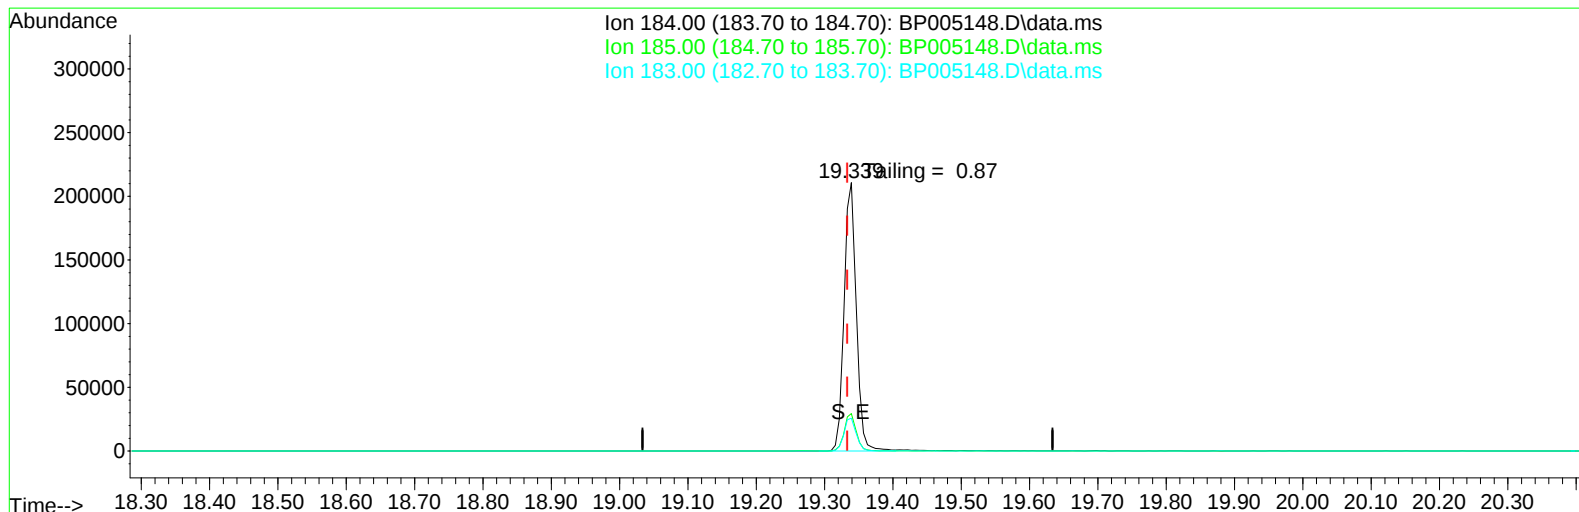

TIC: BP005148.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 1794.22 ng

response 261348

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	12.00	12.25
0.00	0.00	0.00