

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
 Data File : BP005152.D
 Acq On : 02 Apr 2021 11:02
 Operator : CG/JU
 Sample : M1872-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SP-GIS

Quant Time: Apr 02 11:44:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	26924	20.00	ng	# 0.00
21) Naphthalene-d8	10.493	136	106160	20.00	ng	# 0.00
39) Acenaphthene-d10	14.357	164	69164	20.00	ng	0.00
64) Phenanthrene-d10	17.122	188	143592	20.00	ng	# 0.00
76) Chrysene-d12	21.216	240	154053	20.00	ng	-0.01
86) Perylene-d12	23.504	264	155453	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.299	112	178222	101.87	ng	0.00
7) Phenol-d6	6.881	99	234696	93.65	ng	0.00
23) Nitrobenzene-d5	8.863	82	150511	60.83	ng	0.00
42) 2,4,6-Tribromophenol	15.857	330	80158	88.95	ng	0.00
45) 2-Fluorobiphenyl	12.975	172	267505	52.32	ng	0.00
79) Terphenyl-d14	19.698	244	405909	47.97	ng	0.00
Target Compounds						
						Qvalue
10) Phenol	6.905	94	5688	2.21	ng	74
50) Dimethylphthalate	13.816	163	12122	2.28	ng	99
60) Diethylphthalate	15.187	149	17213	3.30	ng	96
74) Di-n-butylphthalate	18.092	149	22995	2.73	ng	# 97
84) Bis(2-ethylhexyl)phtha...	21.133	149	12946	2.25	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
Data File : BP005152.D
Acq On : 02 Apr 2021 11:02
Operator : CG/JU
Sample : M1872-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP-GIS

Quant Time: Apr 02 11:44:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration




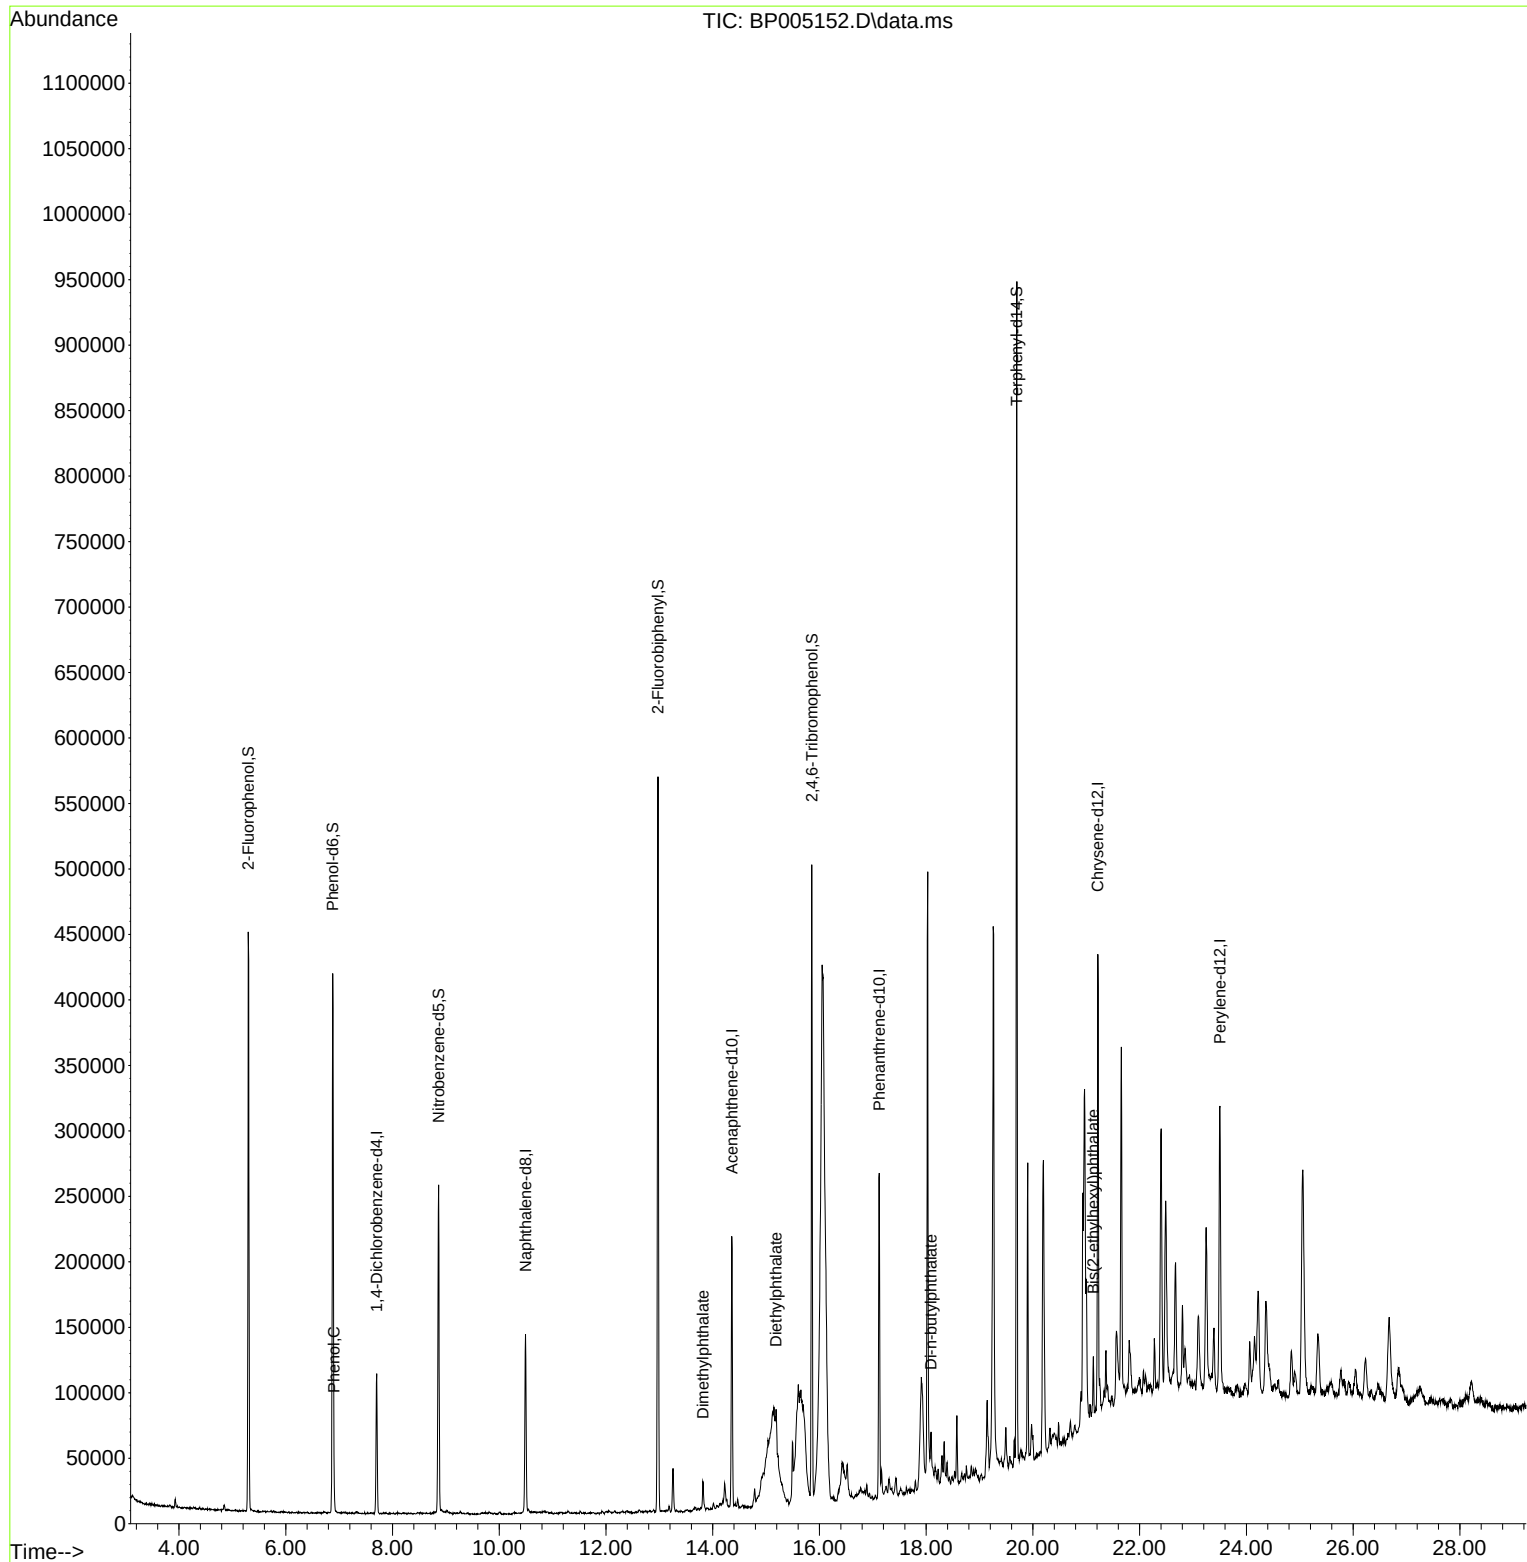




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.705 min Scan# 785
Delta R.T. -0.000 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampleId :
SP-GIS


Tgt Ion:152 Resp: 26924
Ion Ratio Lower Upper
152 100
150 149.6 123.8 185.6
115 66.0 43.8 65.6#

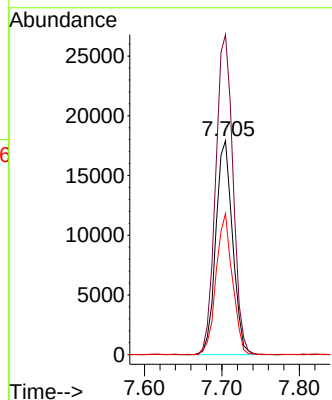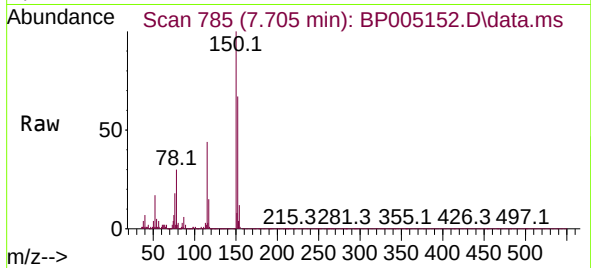

#5
2-Fluorophenol
Concen: 101.87 ng
RT: 5.299 min Scan# 376
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion:112 Resp: 178222
Ion Ratio Lower Upper
112 100
64 59.2 32.8 49.2#
63 30.9 17.0 25.4#


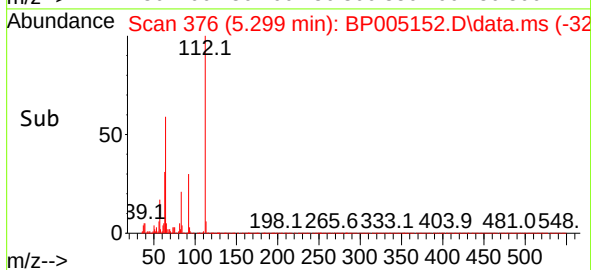
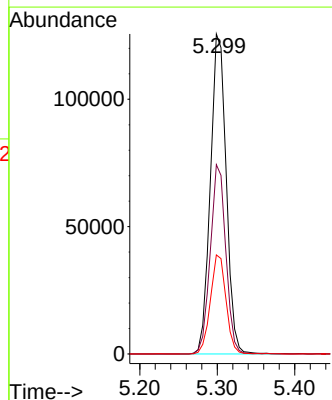





#7
Phenol-d6
Concen: 93.65 ng
RT: 6.881 min Scan# 645
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampleId :
SP-GIS


Tgt Ion: 99 Resp: 234696
Ion Ratio Lower Upper
99 100
42 13.6 8.6 13.0#
71 37.4 23.4 35.2#

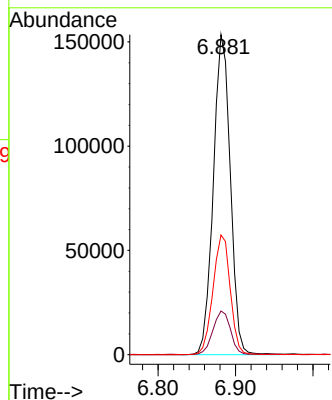

#10
Phenol
Concen: 2.21 ng
RT: 6.905 min Scan# 649
Delta R.T. -0.012 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion: 94 Resp: 5688
Ion Ratio Lower Upper
94 100
65 29.8 2.3 42.3
66 49.7 10.9 50.9


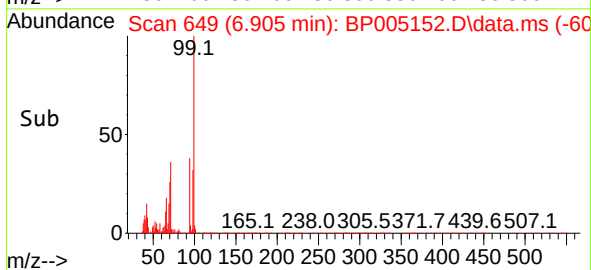
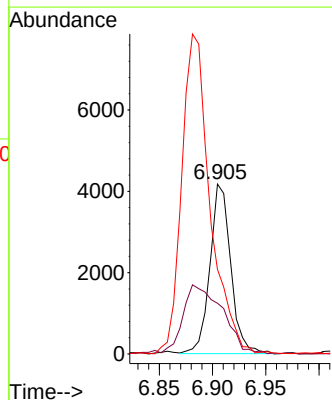



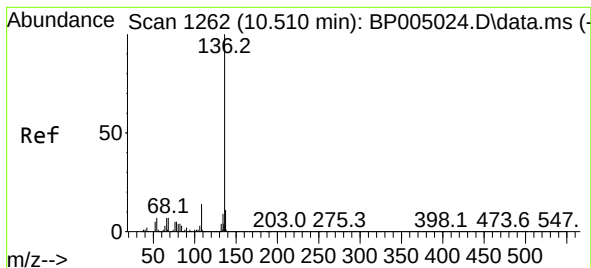

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.493 min Scan# 1259
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampleId :
SP-GIS


Tgt Ion:	136	Resp:	106160
Ion Ratio	Lower	Upper	
136	100		
137	10.1	8.6	13.0
54	7.4	3.6	5.4#
68	6.6	3.3	4.9#

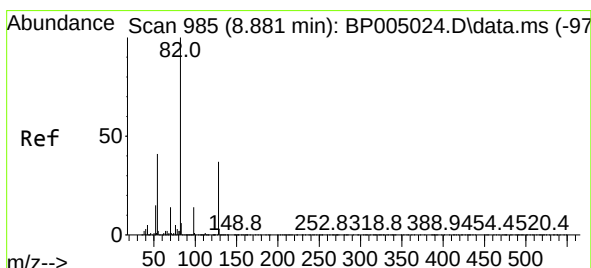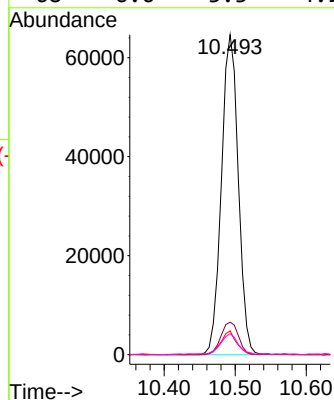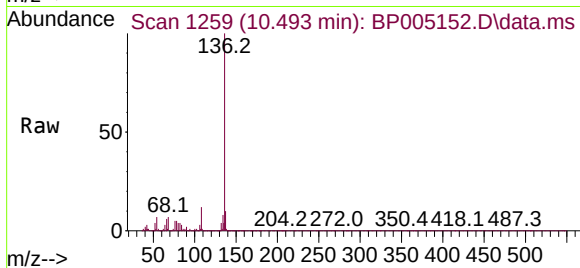

#23
Nitrobenzene-d5
Concen: 60.83 ng
RT: 8.863 min Scan# 982
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion:	82	Resp:	150511
Ion Ratio	Lower	Upper	
82	100		
128	38.7	45.6	68.4#
54	38.3	30.1	45.1


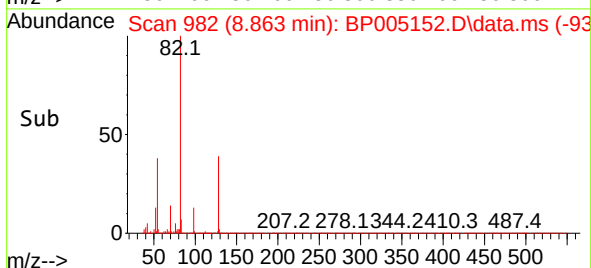
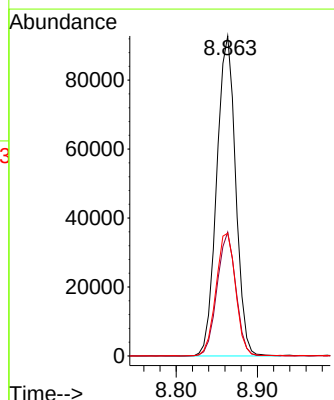
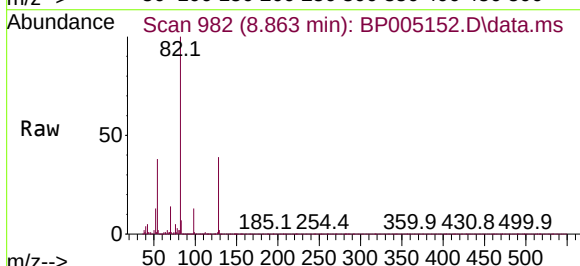




#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.357 min Scan# 1916
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampleId :
SP-GIS


Tgt Ion:164 Resp: 69164
Ion Ratio Lower Upper
164 100
162 95.8 79.4 119.2
160 43.5 36.1 54.1

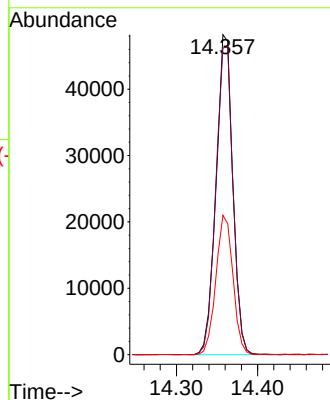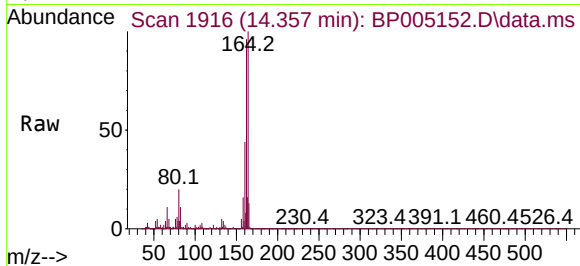

#42
2,4,6-Tribromophenol
Concen: 88.95 ng
RT: 15.857 min Scan# 2171
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion:330 Resp: 80158
Ion Ratio Lower Upper
330 100
332 97.0 77.1 115.7
141 35.9 23.4 35.2#


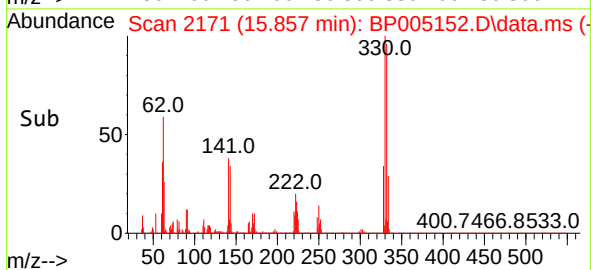
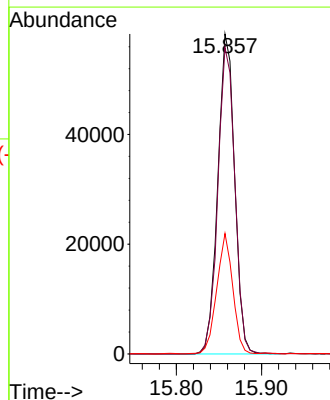
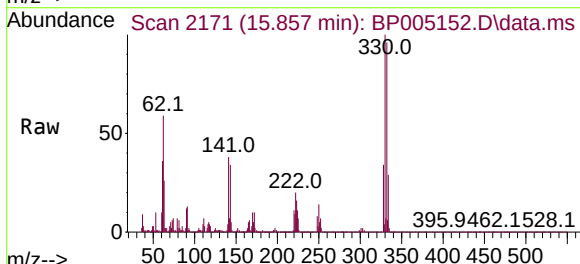




#45
2-Fluorobiphenyl
Concen: 52.32 ng
RT: 12.975 min Scan# 1681
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampleId :
SP-GIS


Tgt Ion:172	Resp:	267505
Ion Ratio	Lower	Upper
172	100	
171	34.5	28.5 42.7
170	22.5	19.2 28.8

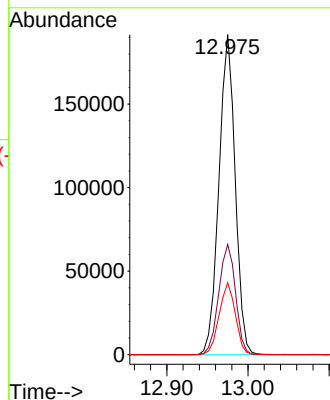

#50
Dimethylphthalate
Concen: 2.28 ng
RT: 13.816 min Scan# 1824
Delta R.T. -0.012 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion:163	Resp:	12122
Ion Ratio	Lower	Upper
163	100	
194	4.7	3.3 4.9
164	9.9	8.2 12.2


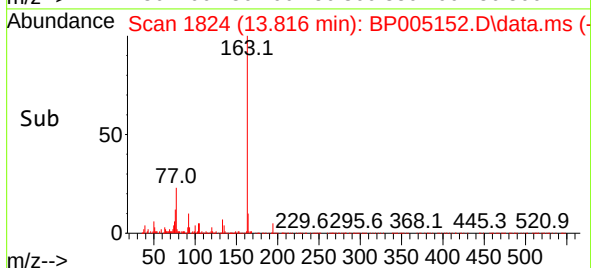
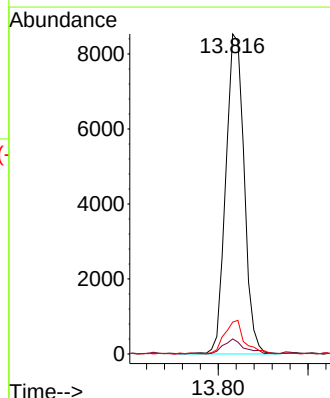





#60
Diethylphthalate
Concen: 3.30 ng
RT: 15.187 min Scan# 2057
Delta R.T. -0.012 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampled :
SP-GIS


Tgt Ion:	149	Resp:	17213
Ion Ratio	Lower	Upper	
149	100		
177	20.4	18.0	27.0
150	11.2	10.0	15.0

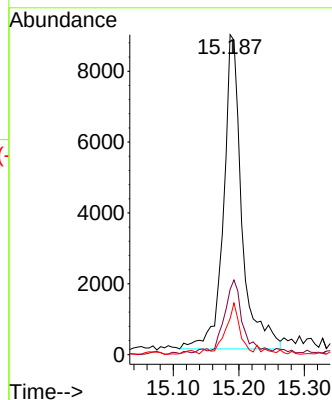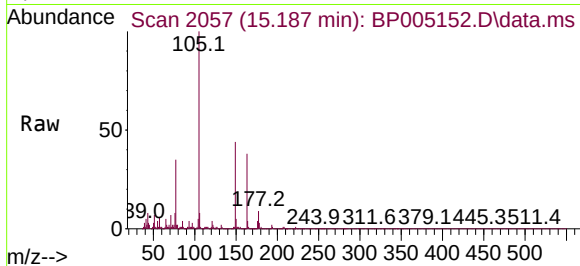

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.122 min Scan# 2386
Delta R.T. -0.006 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion:	188	Resp:	143592
Ion Ratio	Lower	Upper	
188	100		
94	9.6	6.2	9.2#
80	10.2	6.2	9.2#


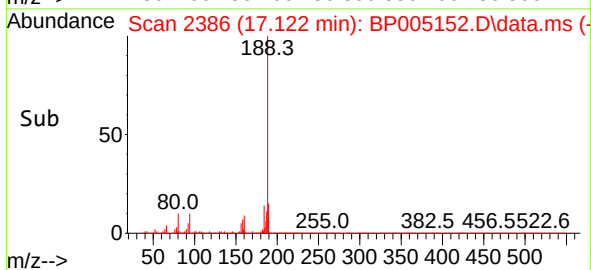
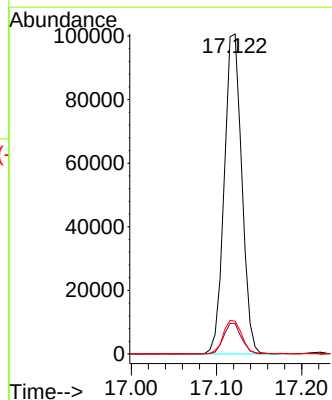
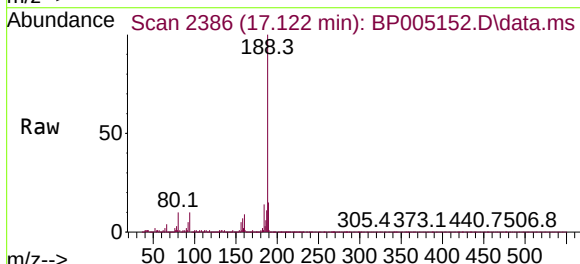




#74
Di-n-butylphthalate
Concen: 2.73 ng
RT: 18.092 min Scan# 2551
Delta R.T. -0.000 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02




Instrument :
BNA_P
ClientSampleId :
SP-GIS


Tgt Ion:	149	Resp:	22995
Ion Ratio	Lower	Upper	
149	100		
150	10.0	7.3	10.9
104	5.9	3.4	5.0#

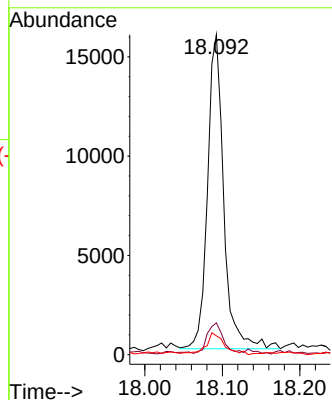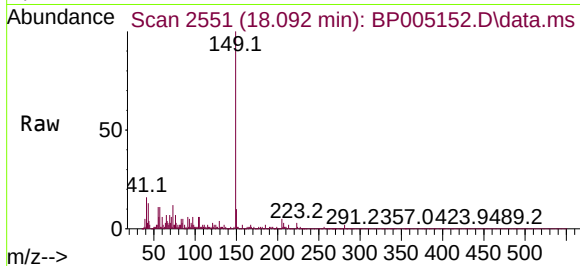

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.216 min Scan# 3082
Delta R.T. -0.012 min
Lab File: BP005152.D
Acq: 02 Apr 2021 11:02

Tgt Ion:	240	Resp:	154053
Ion Ratio	Lower	Upper	
240	100		
120	10.1	7.8	11.6
236	24.0	20.8	31.2

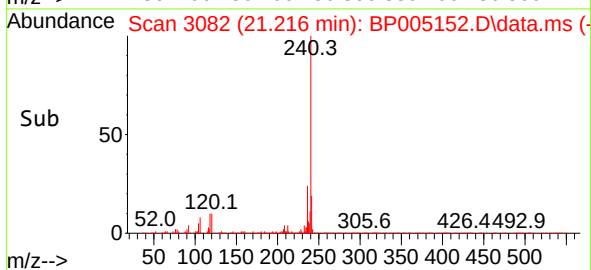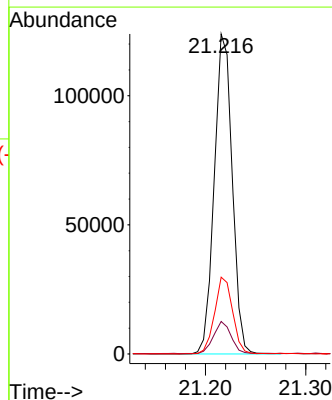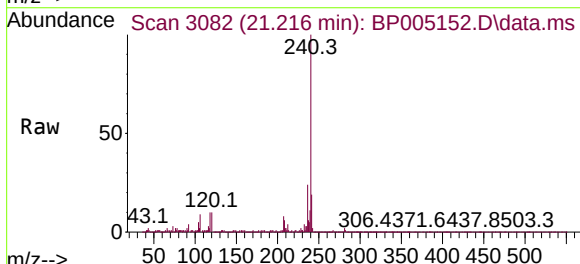







#79
 Terphenyl-d14
 Concen: 47.97 ng
 RT: 19.698 min Scan# 2824
 Delta R.T. -0.000 min
 Lab File: BP005152.D
 Acq: 02 Apr 2021 11:02

Instrument :
 BNA_P
 ClientSampleId :
 SP-GIS

Tgt Ion:244 Resp: 405909




Ion	Ratio	Lower	Upper
244	100		
212	6.5	5.8	8.6
122	9.5	7.8	11.8

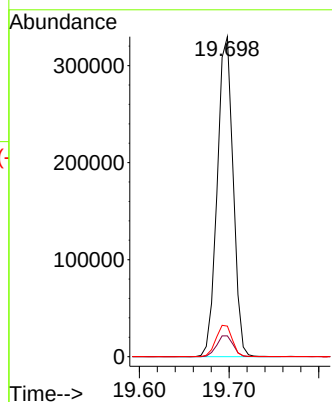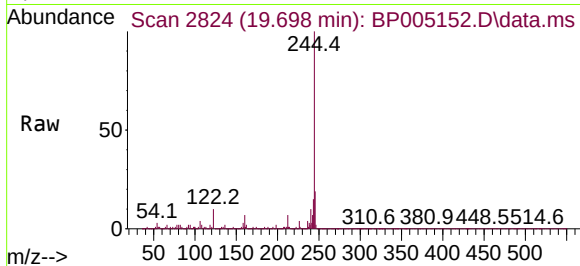


#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.25 ng
 RT: 21.133 min Scan# 3068
 Delta R.T. -0.006 min
 Lab File: BP005152.D
 Acq: 02 Apr 2021 11:02

Tgt Ion:149 Resp: 12946

Ion	Ratio	Lower	Upper
149	100		
167	31.2	22.6	34.0
279	5.2	4.2	6.2

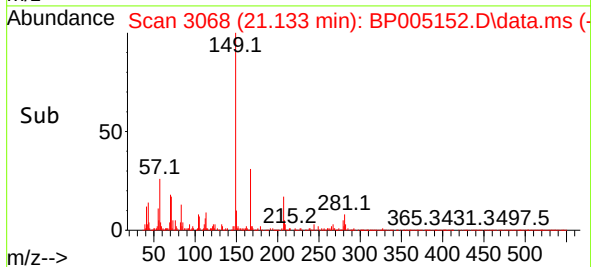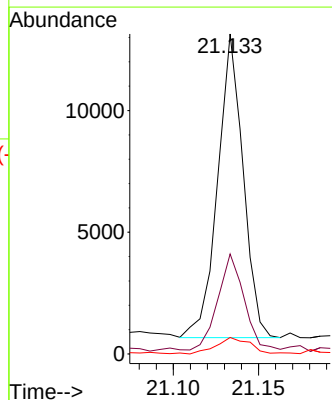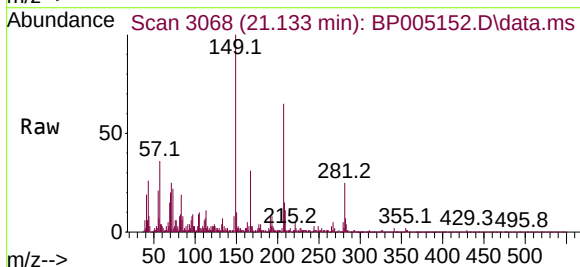

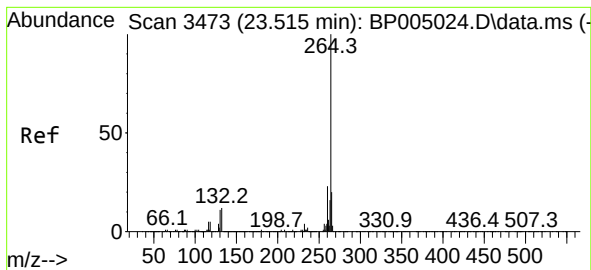

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.504 min Scan# 3471
 Delta R.T. -0.006 min
 Lab File: BP005152.D
 Acq: 02 Apr 2021 11:02

Instrument :
 BNA_P
 ClientSampleId :
 SP-GIS

Tgt Ion:264 Resp: 155453
 Ion Ratio Lower Upper
 264 100
 260 25.7 18.8 28.2
 265 21.4 17.4 26.2

