
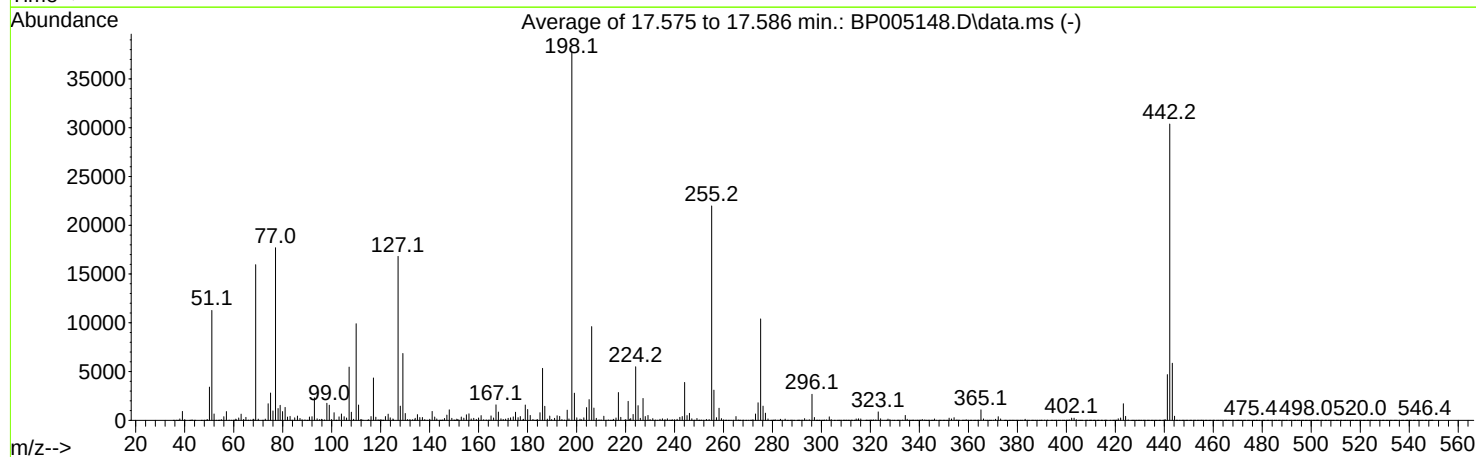


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
 Data File : BP005148.D
 Acq On : 02 Apr 2021 08:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 01 12:23:57 2021

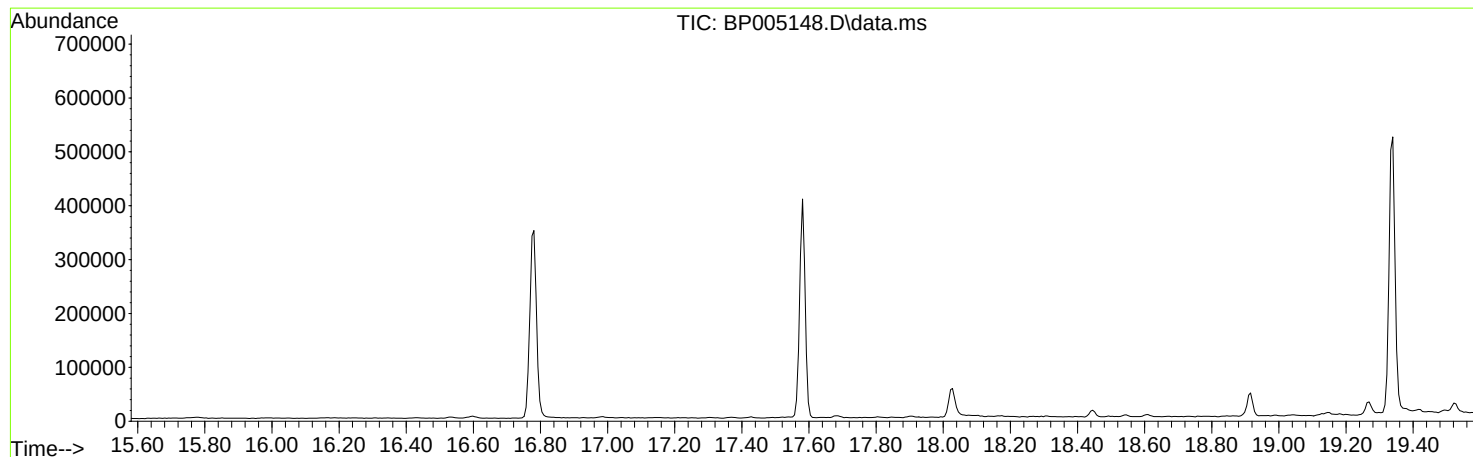

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	11270	PASS
68	69	0.00	2	0.8	120	PASS
69	198	0.00	100	42.3	15963	PASS
70	69	0.00	2	0.8	131	PASS
127	198	10	80	44.6	16806	PASS
197	198	0.00	2	0.4	145	PASS
198	198	100	100	100.0	37709	PASS
199	198	5	9	7.4	2793	PASS
275	198	10	60	27.6	10402	PASS
365	198	1	100	2.9	1079	PASS
441	198	0.01	100	12.4	4689	PASS
442	442	100	100	100.0	30379	PASS
443	442	15	24	19.3	5851	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/2/2021	BNA_P	<u>BP005148.D</u>
Compound Name	Response	Retention Time
DDT	154782	20.53
DDD	3115	20.11
DDE	406	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3521	158303	2.22

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
Data File : BP005148.D
Acq On : 02 Apr 2021 08:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 02 11:17:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration

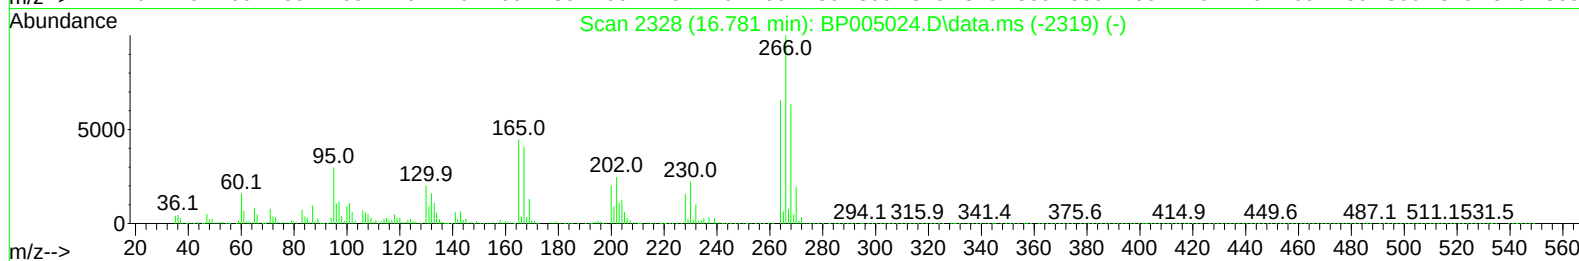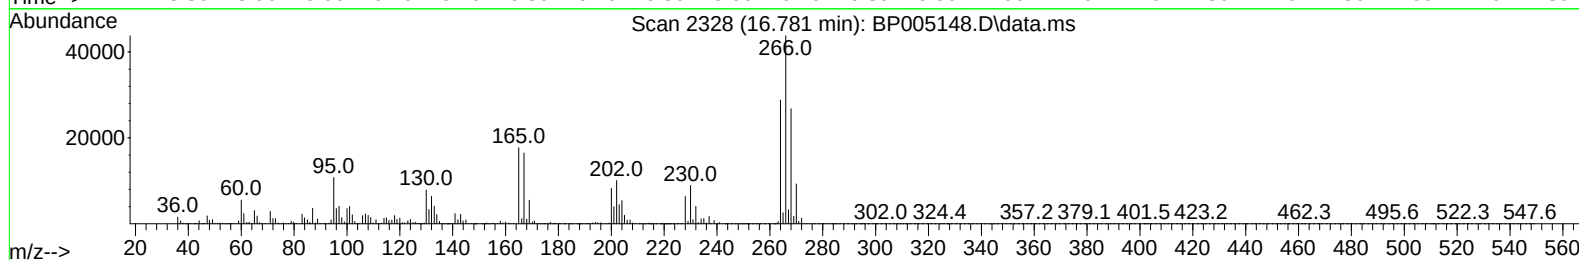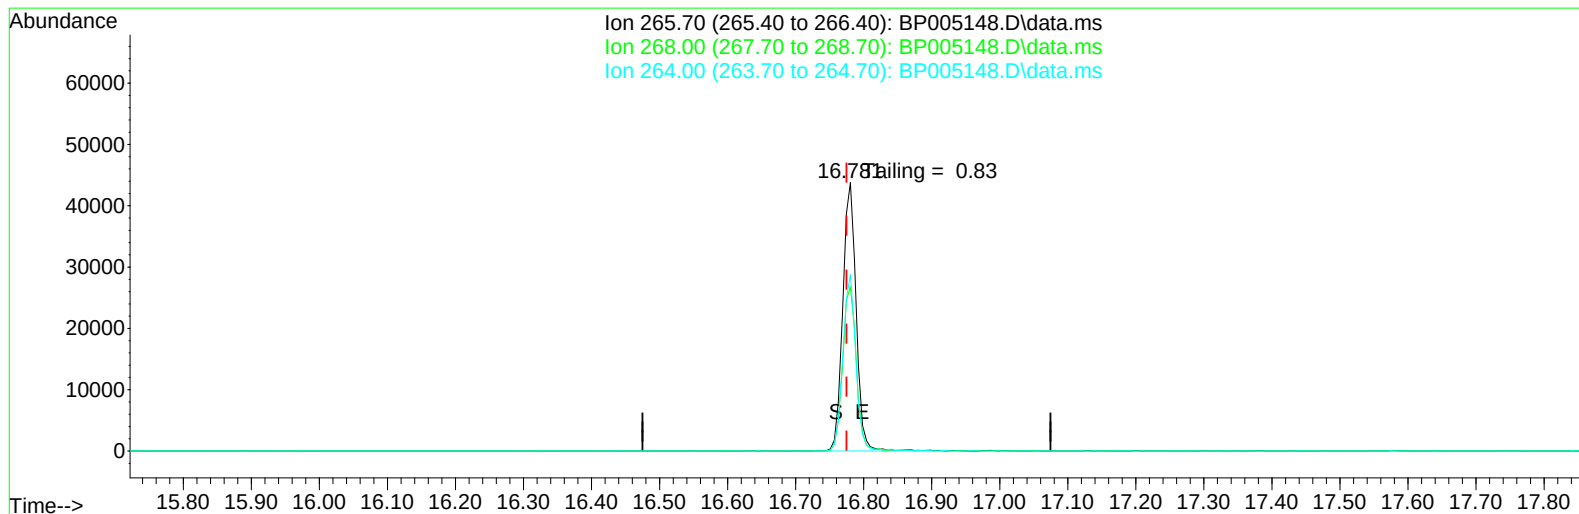

TIC: BP005148.D\data.ms

(70) Pentachlorophenol (C)

16.781min (+ 0.006) 55808.38 ng




response 59534

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.17
264.00	63.30	65.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040221\
Data File : BP005148.D
Acq On : 02 Apr 2021 08:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 02 11:17:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration

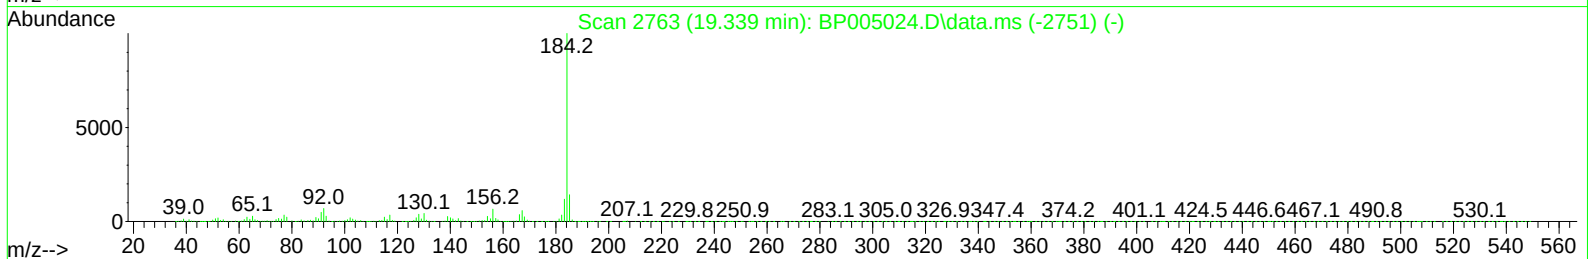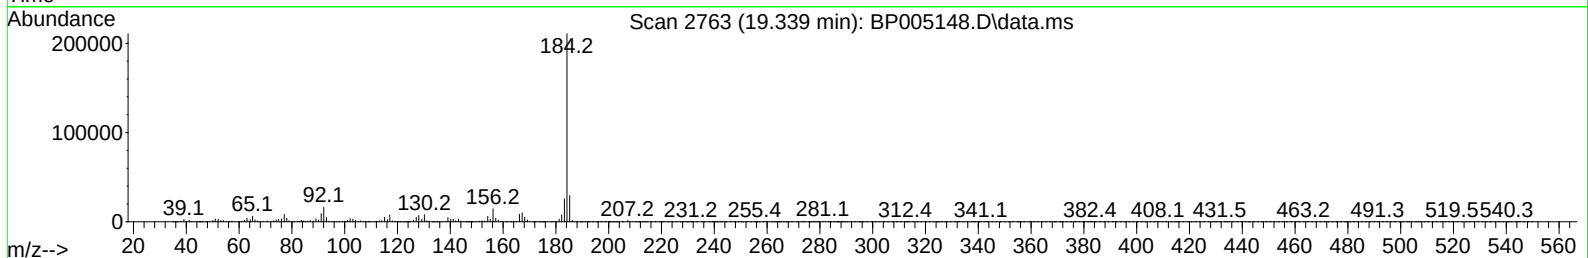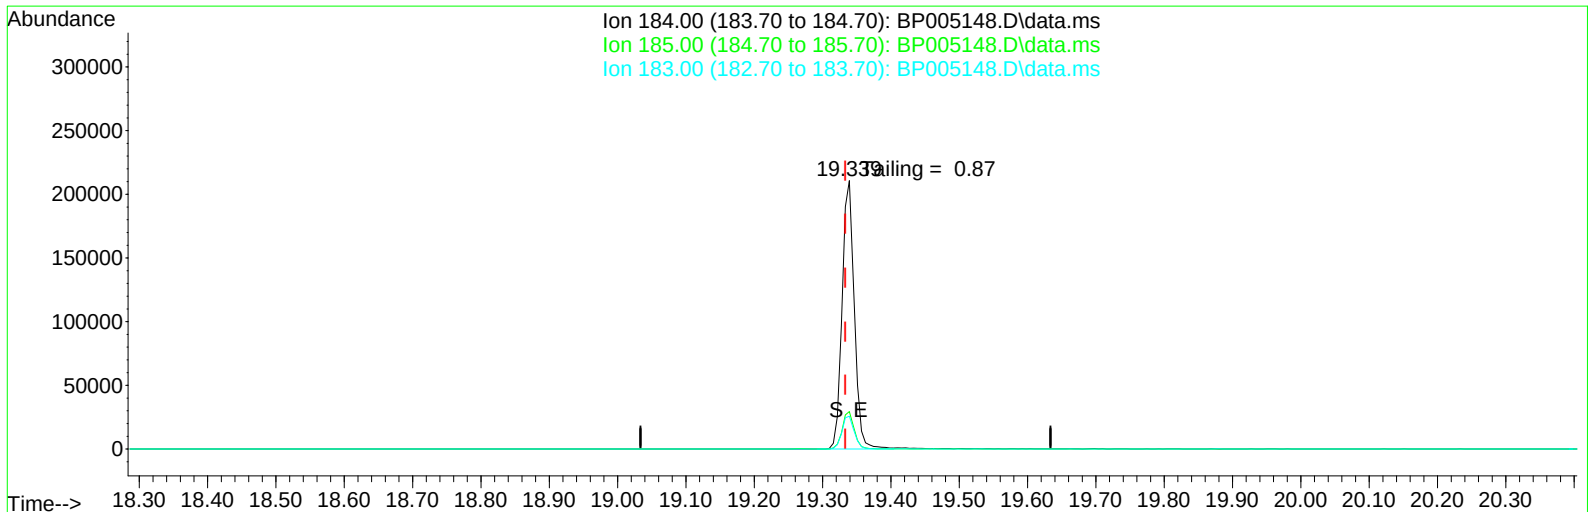

TIC: BP005148.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 1794.22 ng

response 261348

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	12.00	12.25
0.00	0.00	0.00