




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:51:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

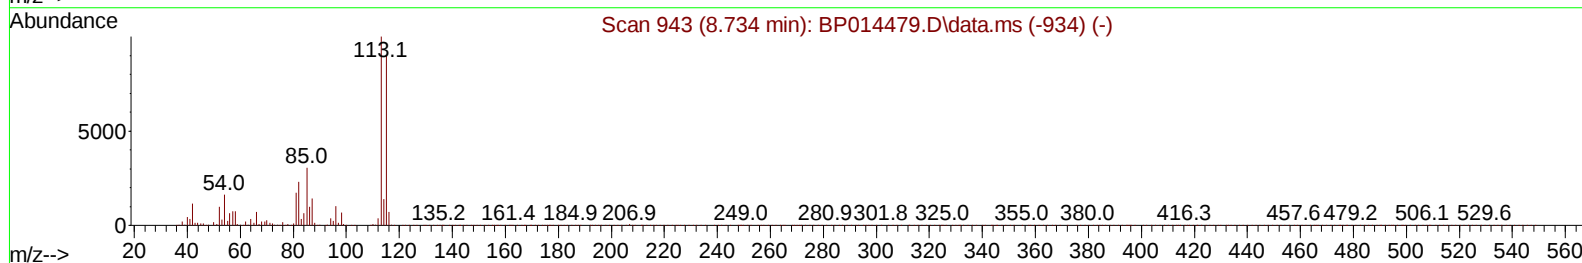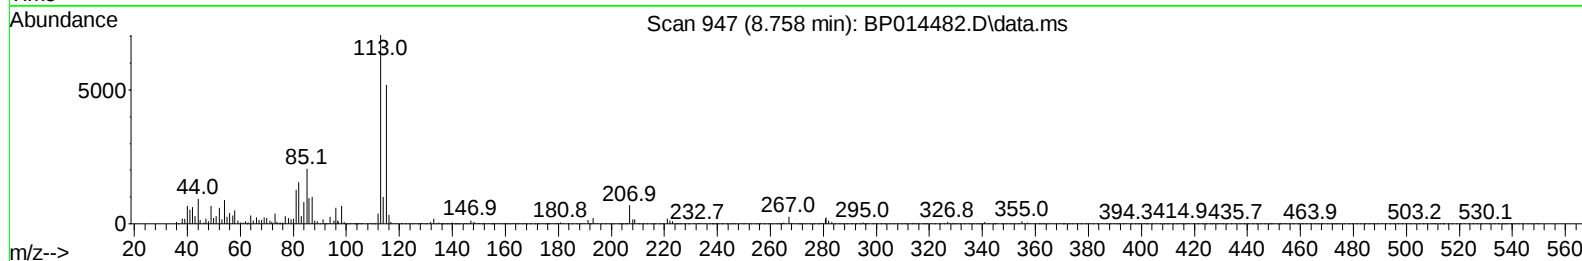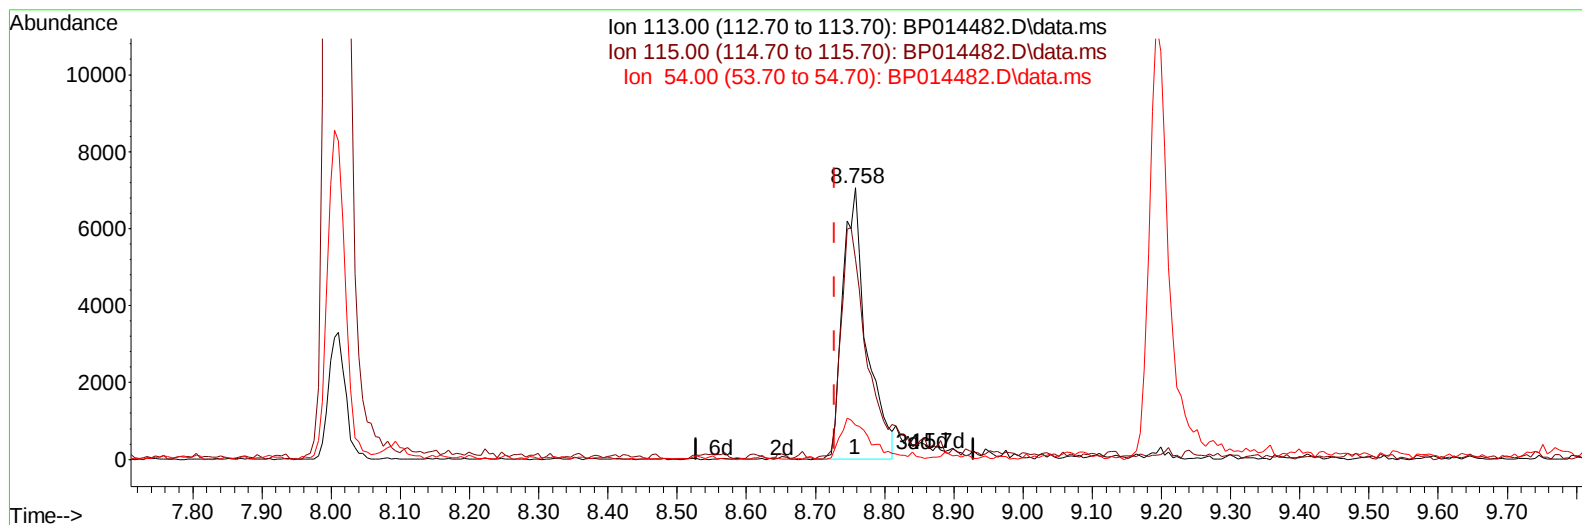

TIC: BP014482.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.758min (+ 0.029) 1.39 ng/u1

response 16739

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	73.60
54.00	15.10	12.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:51:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

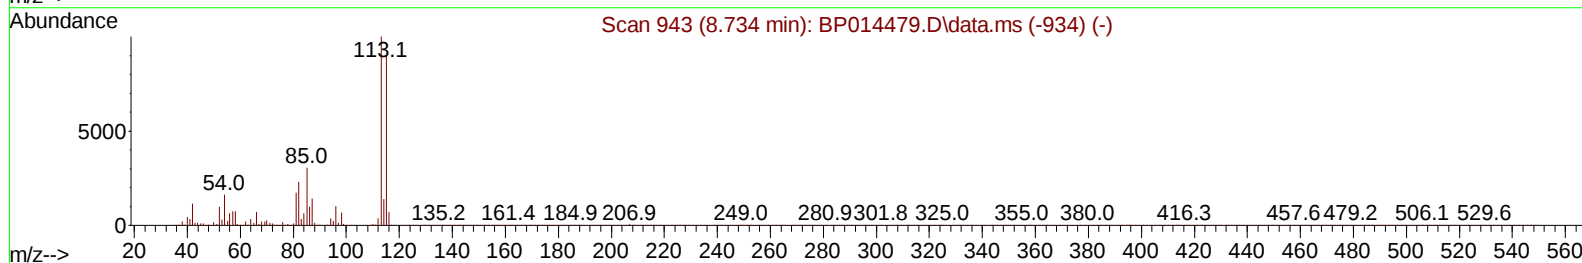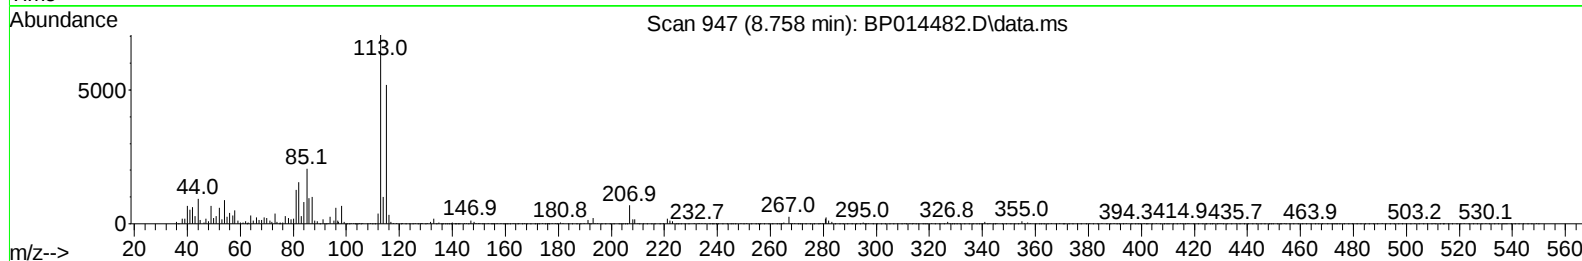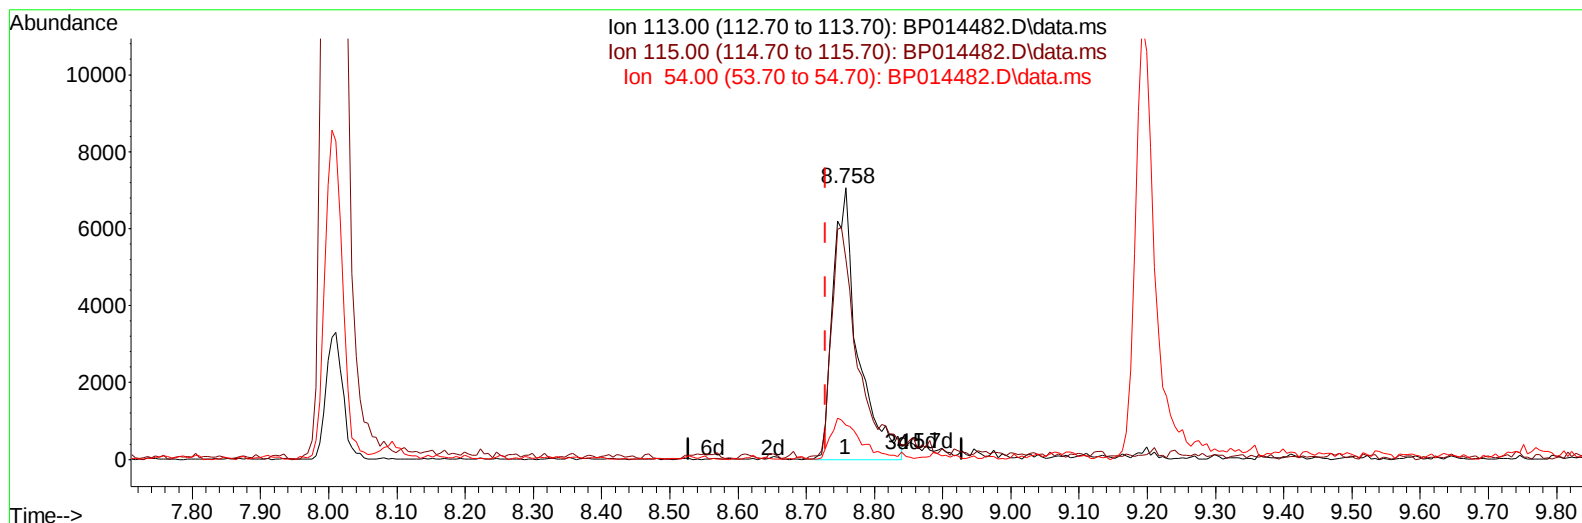

TIC: BP014482.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.758min (+ 0.029) 1.48 ng/ul m

response 17805

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	73.60
54.00	15.10	12.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:51:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

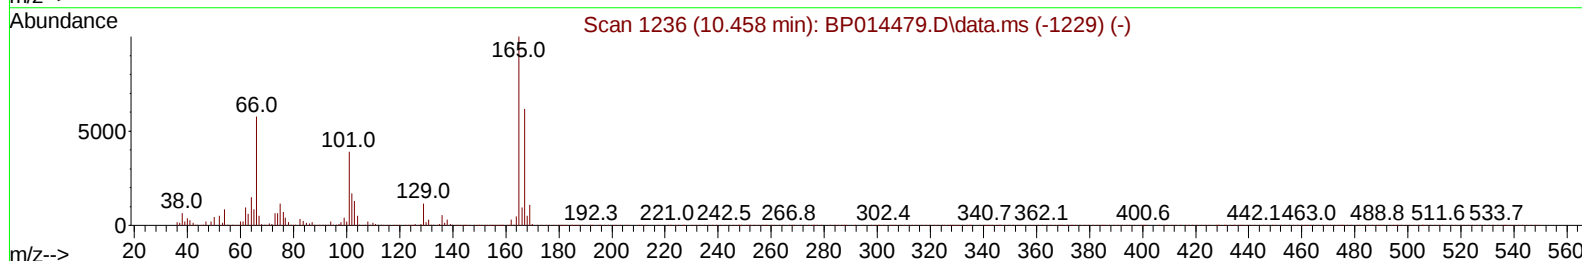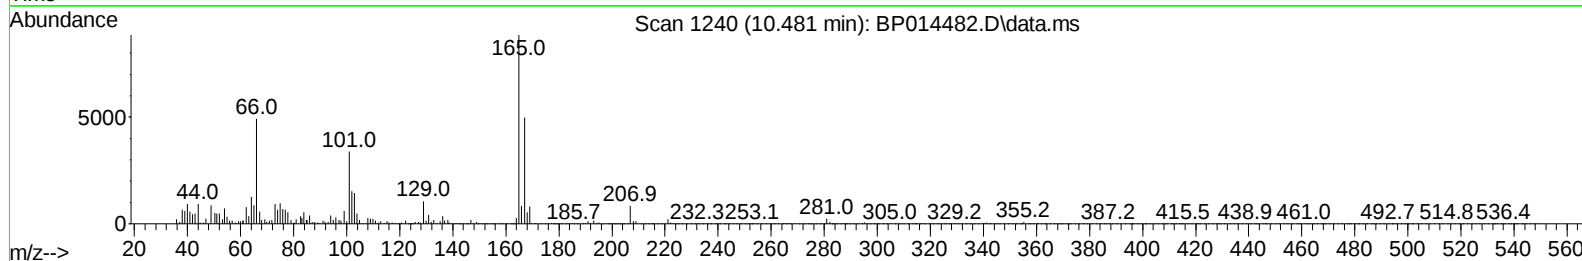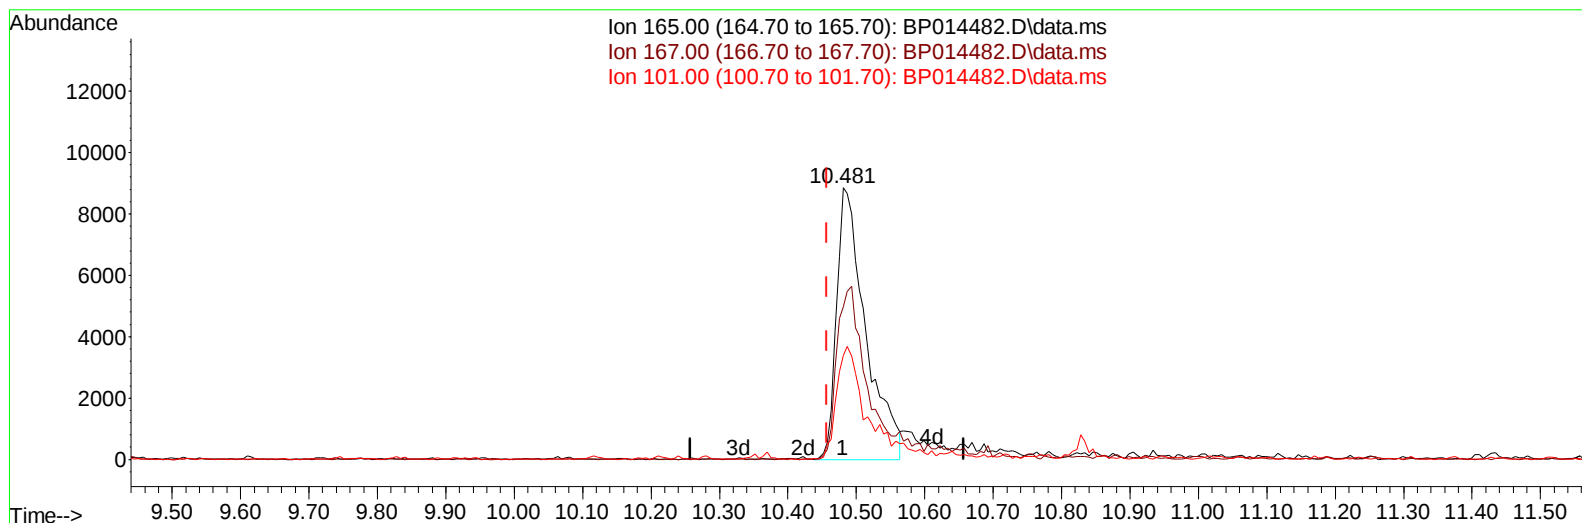

TIC: BP014482.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.481min (+ 0.024) 2.14 ng/ul

response 26028

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	56.28
101.00	39.20	38.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:51:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

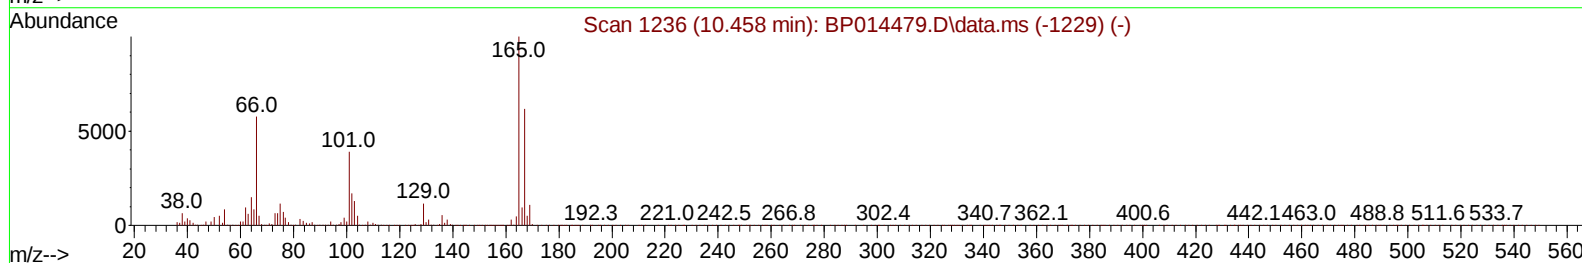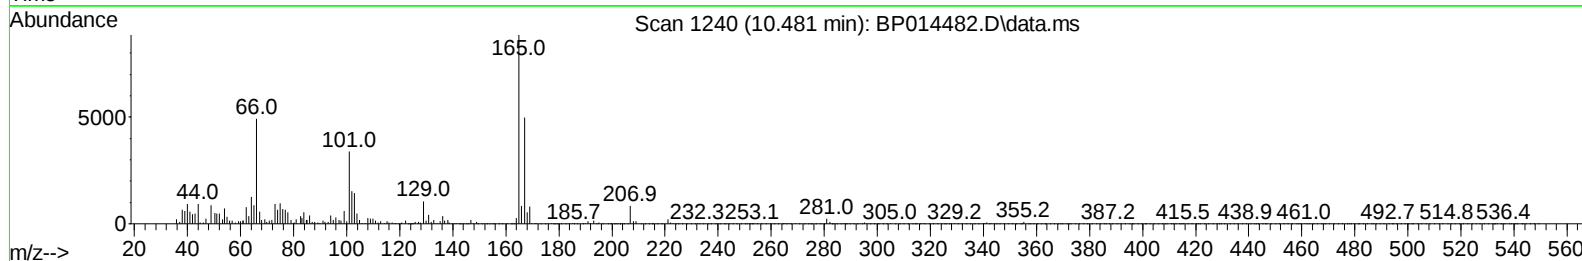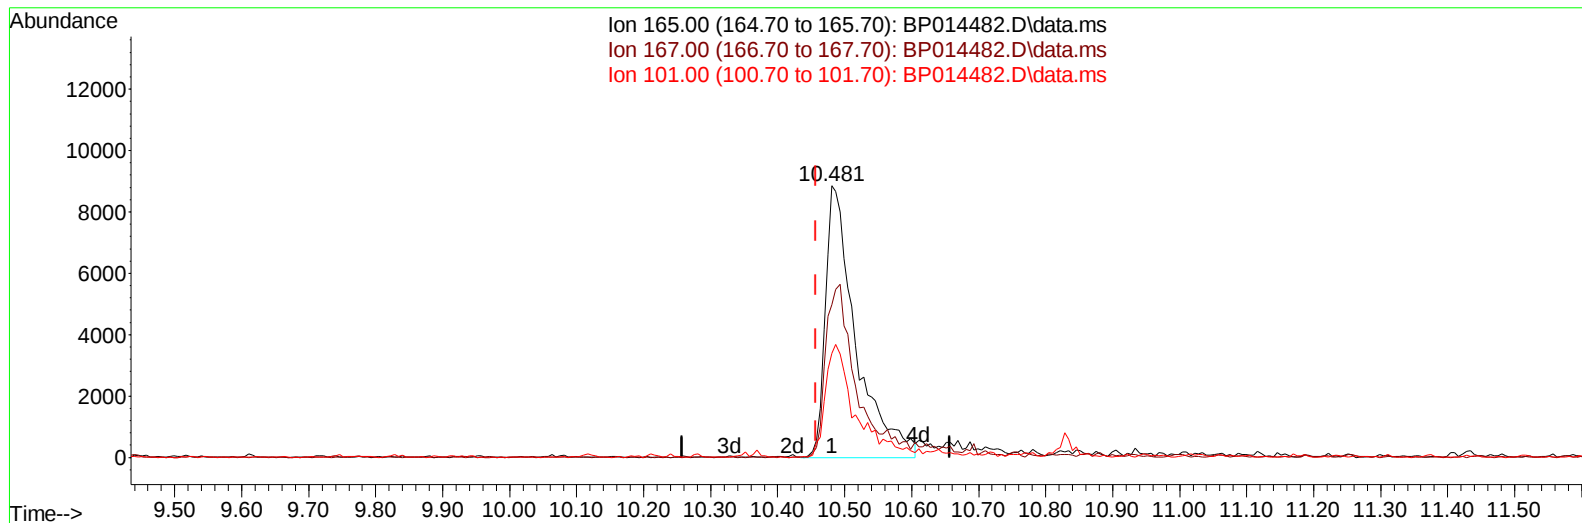

TIC: BP014482.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.481min (+ 0.024) 2.29 ng/ul m

response 2777

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	56.28
101.00	39.20	38.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:51:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

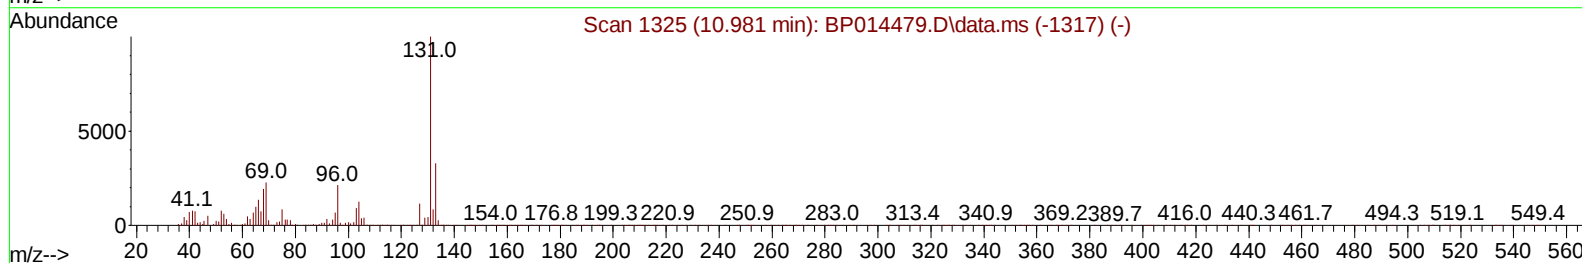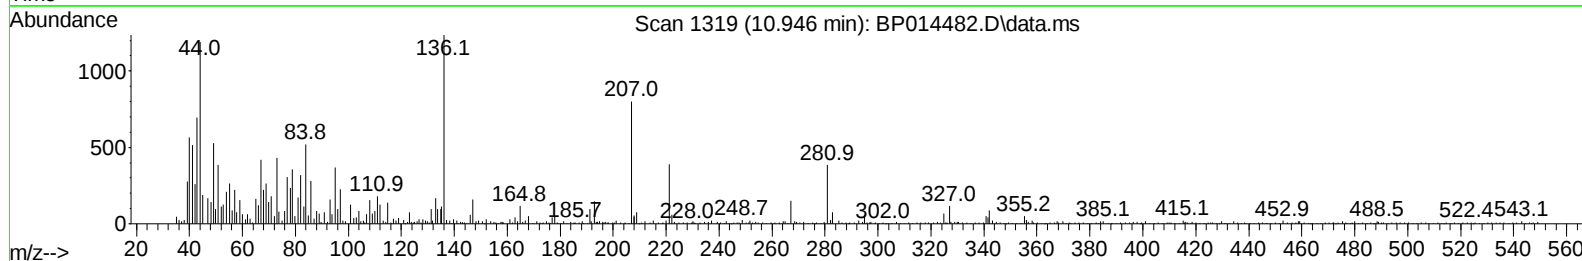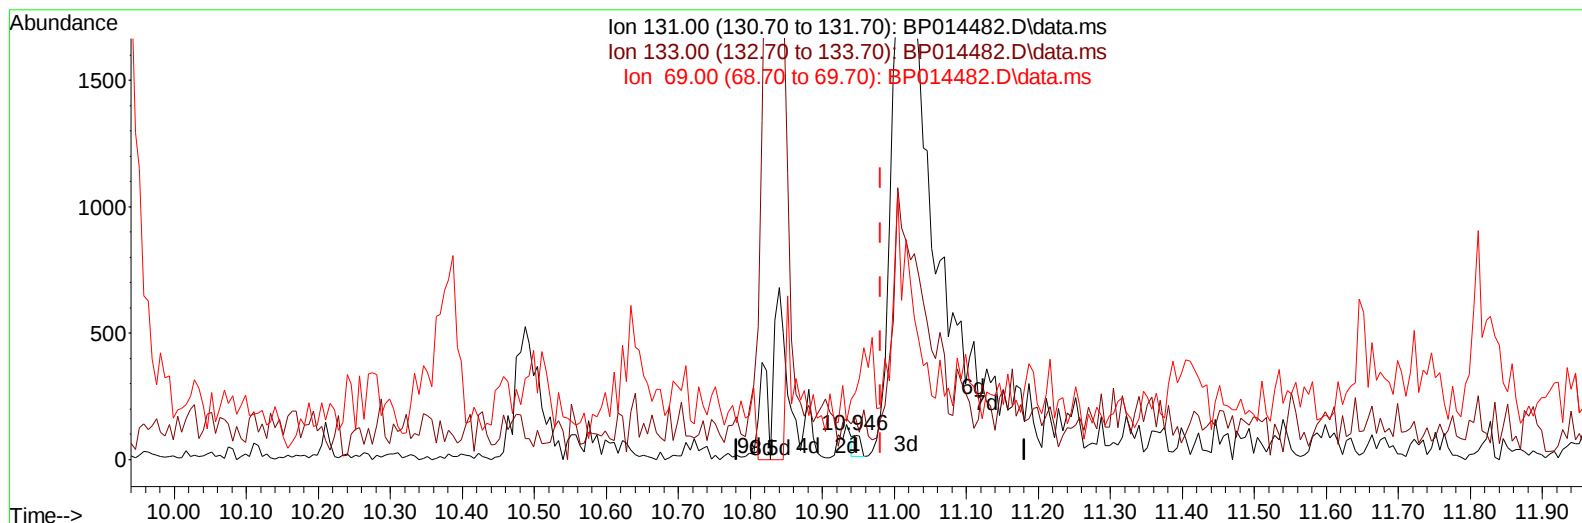

TIC: BP014482.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.946min (-0.035) 0.00 ng/u1

response 58

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	172.92#
69.00	21.30	276.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:51:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

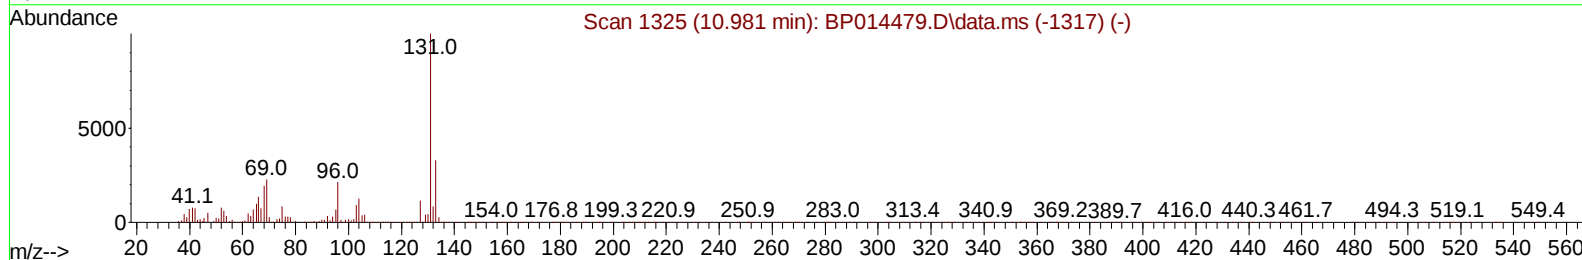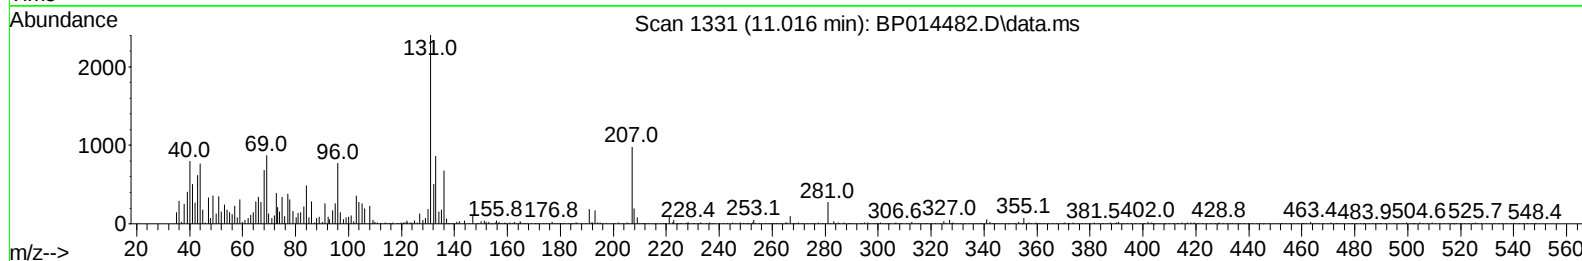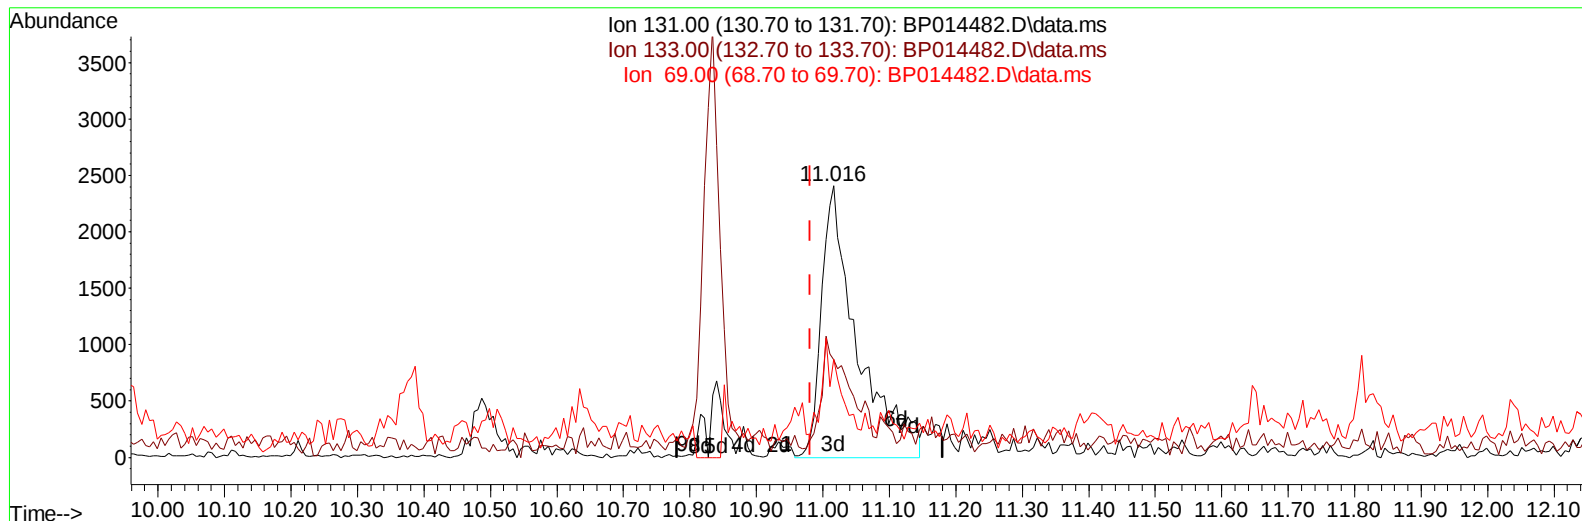

TIC: BP014482.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.016min (+ 0.035) 0.56 ng/ul m

response 9036

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	35.94
69.00	21.30	36.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:51:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	161647	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	721215	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	500150	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1132849	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	964131	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	903736	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	1170	0.281	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.211	99	9090	0.610	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.334	67	28561	2.986	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	23950	2.223	ng/ul	0.00
15) 4-Methylphenol-d8	8.758	113	17805m	1.481	ng/ul	0.03
21) Nitrobenzene-d5	9.193	128	14157	2.432	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	16201	2.430	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	27777m	2.288	ng/ul	0.02
31) 4-Chloroaniline-d4	11.016	131	9036m	0.565	ng/ul	0.04
46) Dimethylphthalate-d6	14.069	166	130064	3.207	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	133939	2.977	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.657	176	115408	3.413	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.528	188	178789	3.261	ng/ul	0.00
81) Pyrene-d10	19.757	212	212120	3.275	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.863	264	151472	3.155	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	59817	13.058	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:51:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

