




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014485.D
 Acq On : 03 Apr 2023 14:07
 Operator : CG/JU
 Sample : 02093-10DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:52:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

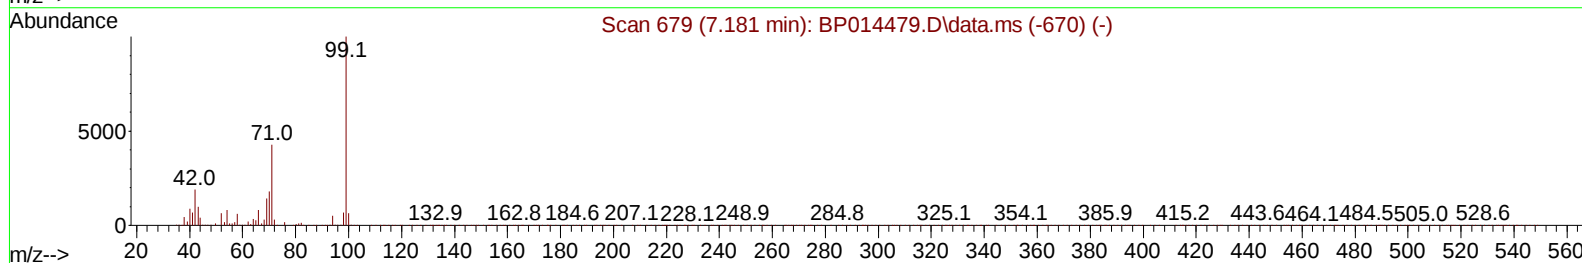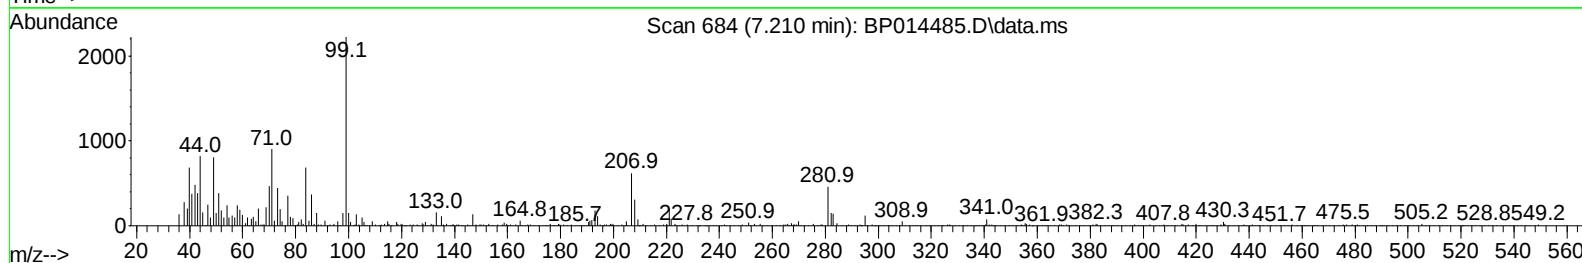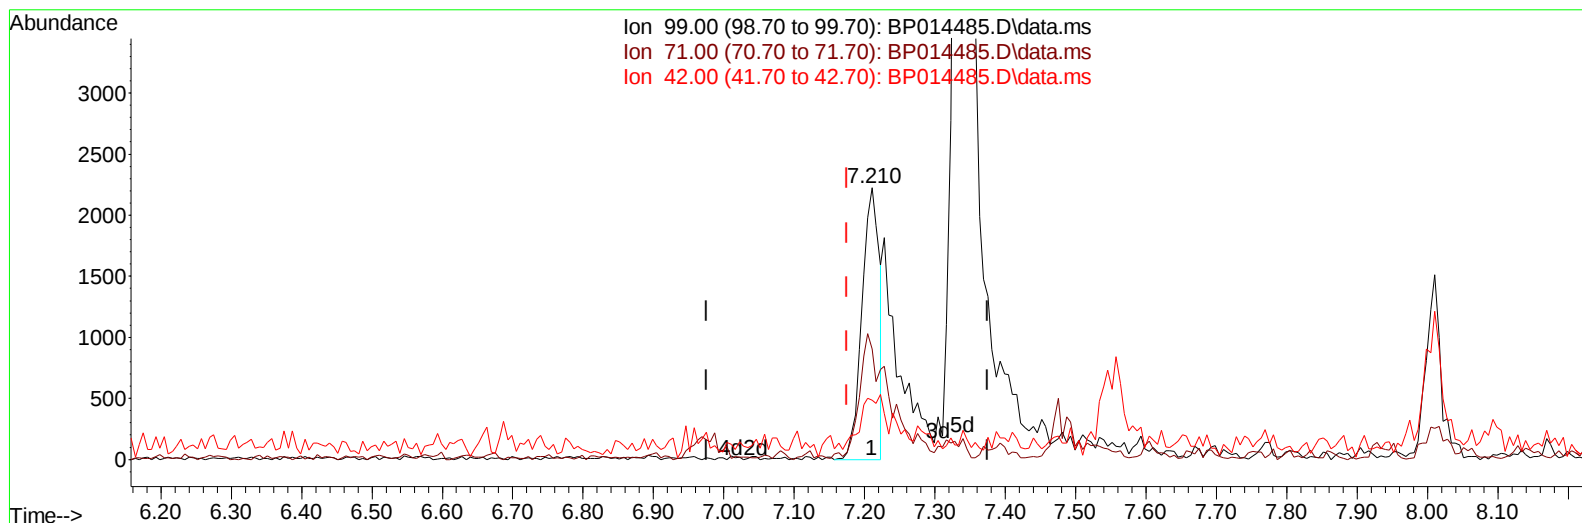

TIC: BP014485.D\data.ms

(7) Phenol-d5 (S)

7.210min (+ 0.035) 0.34 ng/u1

response 3799

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	40.30	40.62
42.00	18.90	21.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014485.D
 Acq On : 03 Apr 2023 14:07
 Operator : CG/JU
 Sample : 02093-10DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:52:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

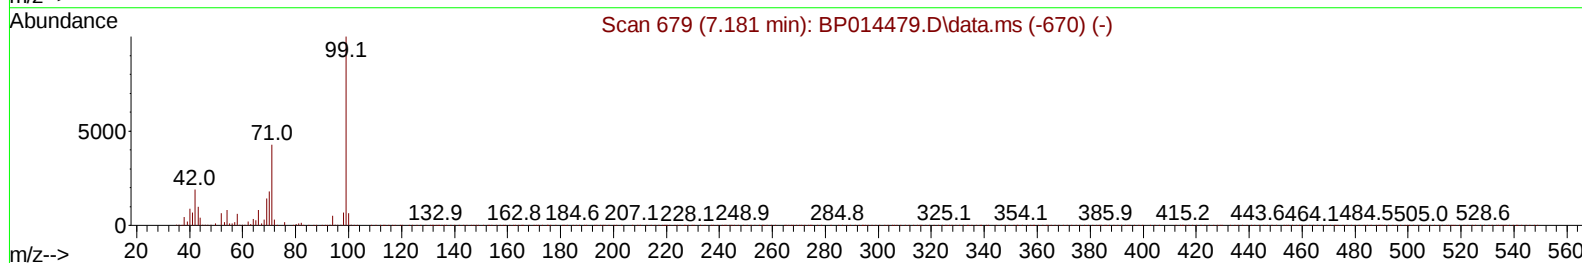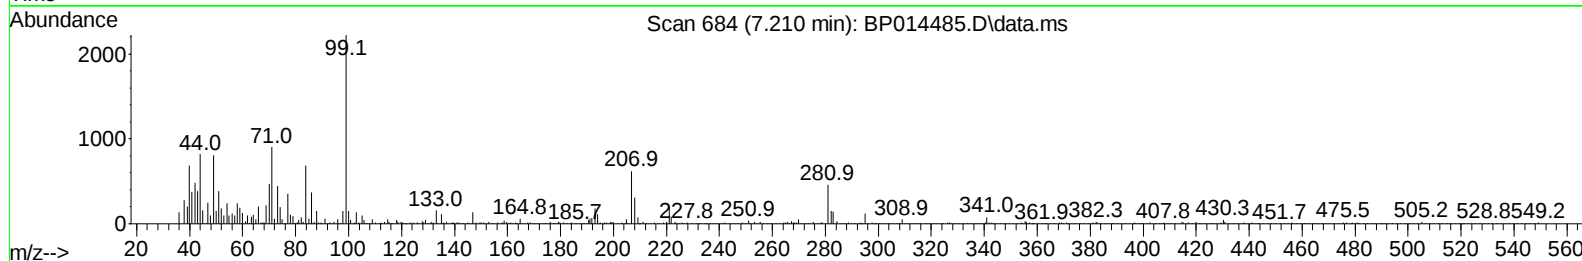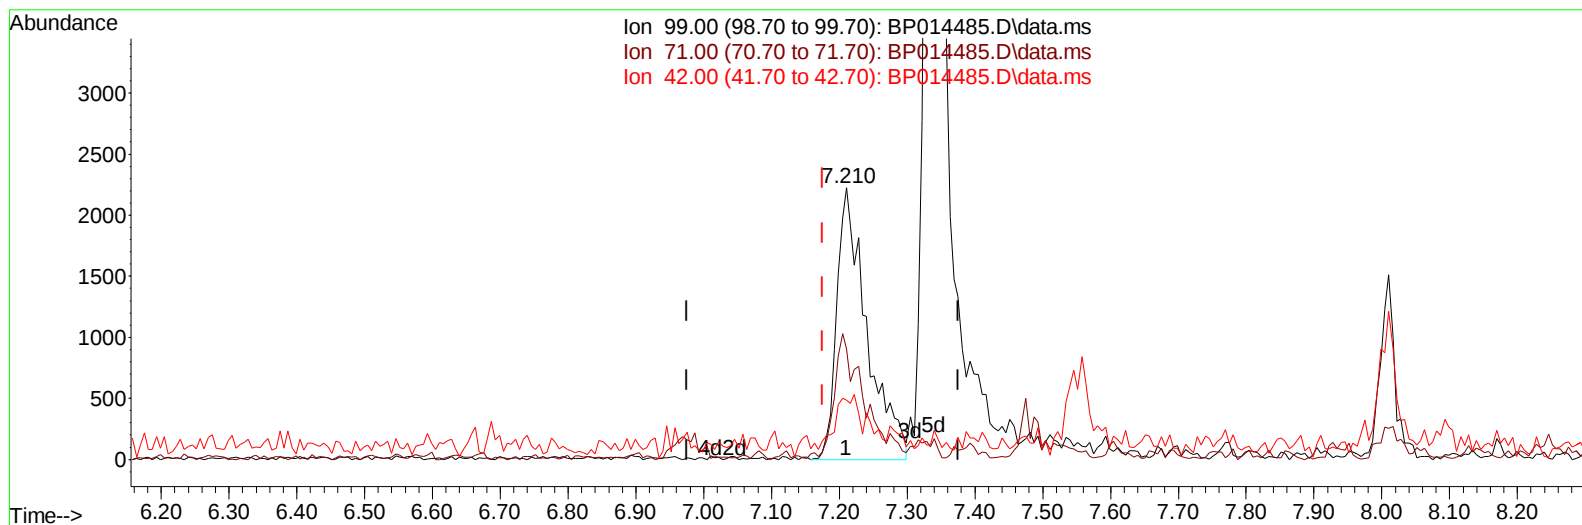

TIC: BP014485.D\data.ms

(7) Phenol-d5 (S)

7.210min (+ 0.035) 0.60 ng/ul m

response 6818

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	40.30	40.62
42.00	18.90	21.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014485.D
 Acq On : 03 Apr 2023 14:07
 Operator : CG/JU
 Sample : 02093-10DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:52:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

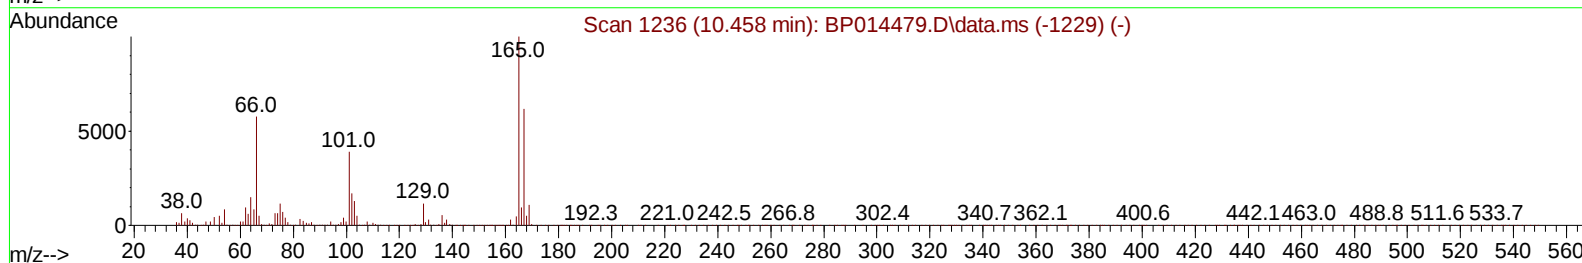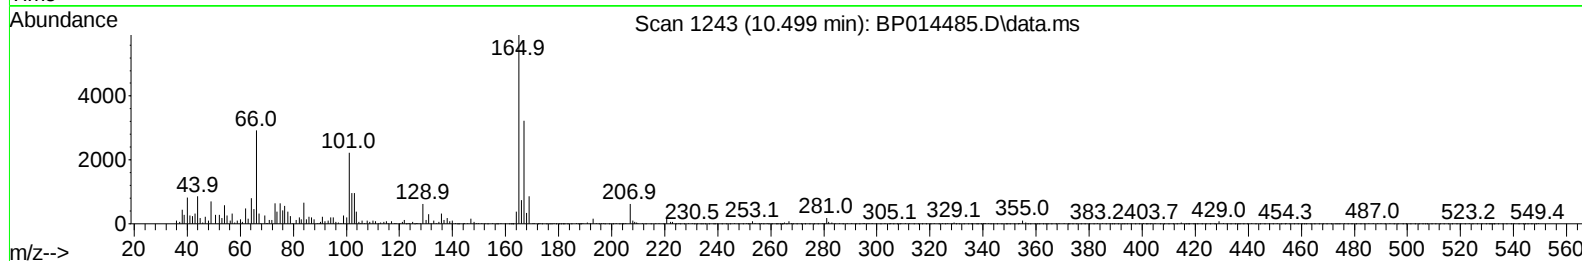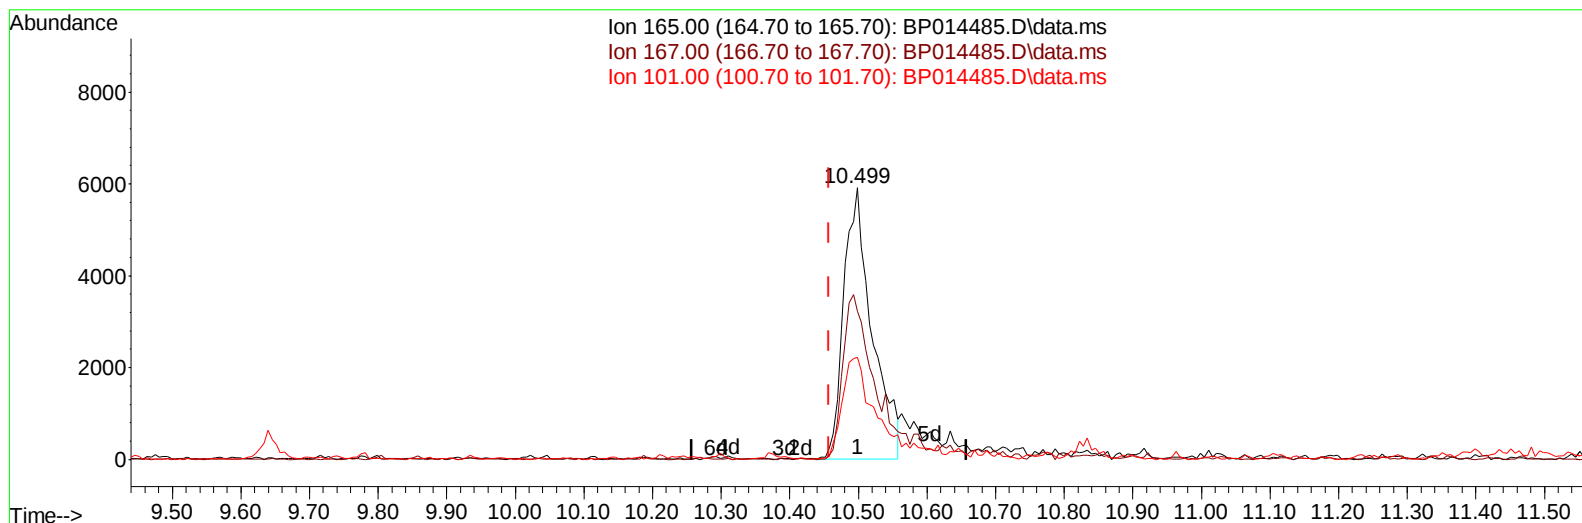

TIC: BP014485.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.499min (+ 0.041) 1.85 ng/ul

response 16937

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	54.57
101.00	39.20	37.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014485.D
Acq On : 03 Apr 2023 14:07
Operator : CG/JU
Sample : 02093-10DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:52:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

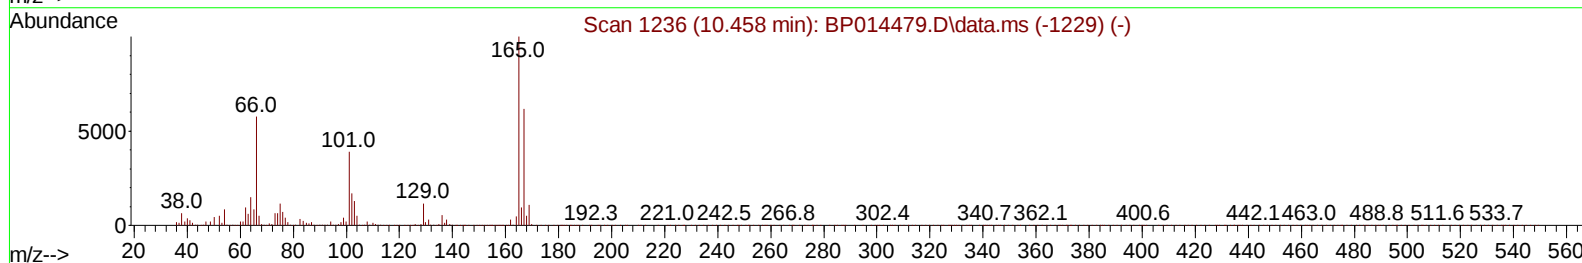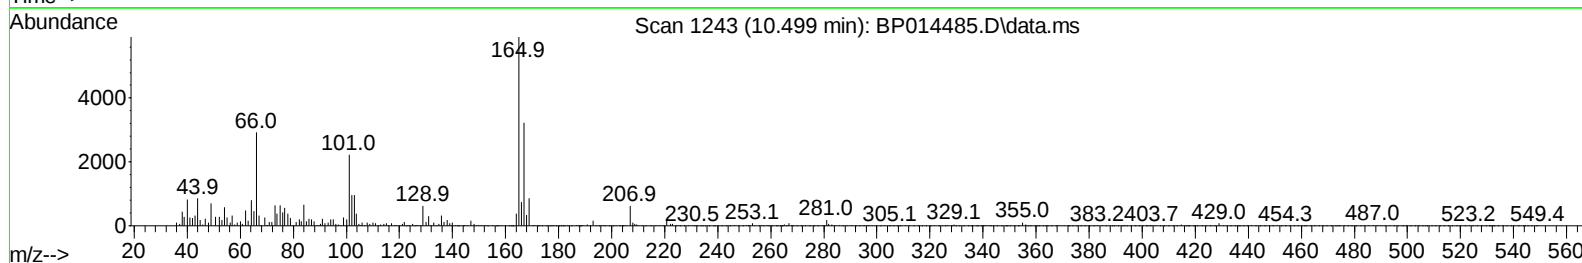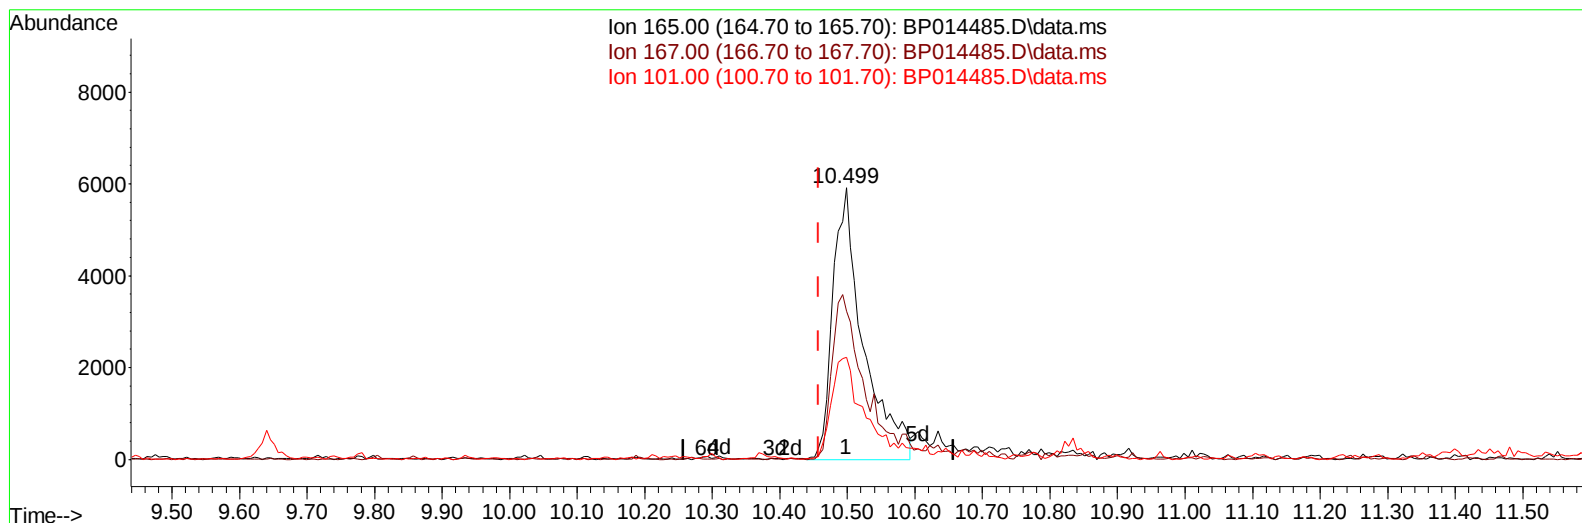

TIC: BP014485.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.499min (+ 0.041) 2.04 ng/ul m

response 18596

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	54.57
101.00	39.20	37.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014485.D
Acq On : 03 Apr 2023 14:07
Operator : CG/JU
Sample : 02093-10DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:52:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

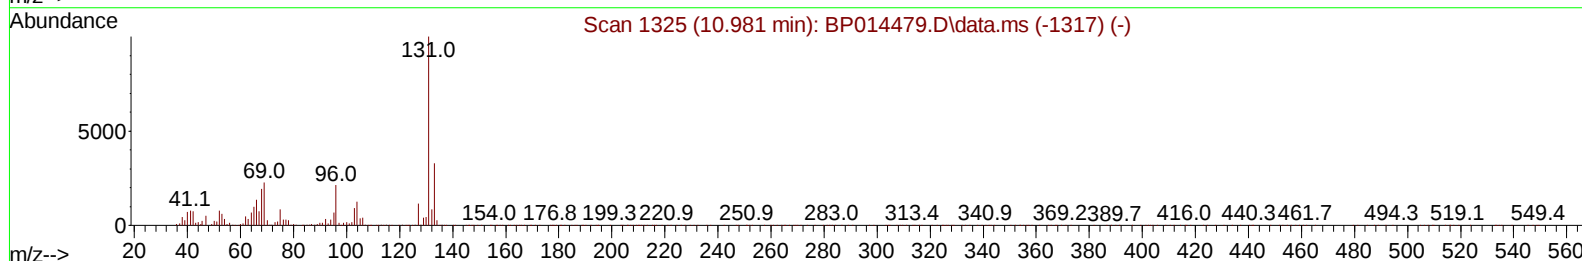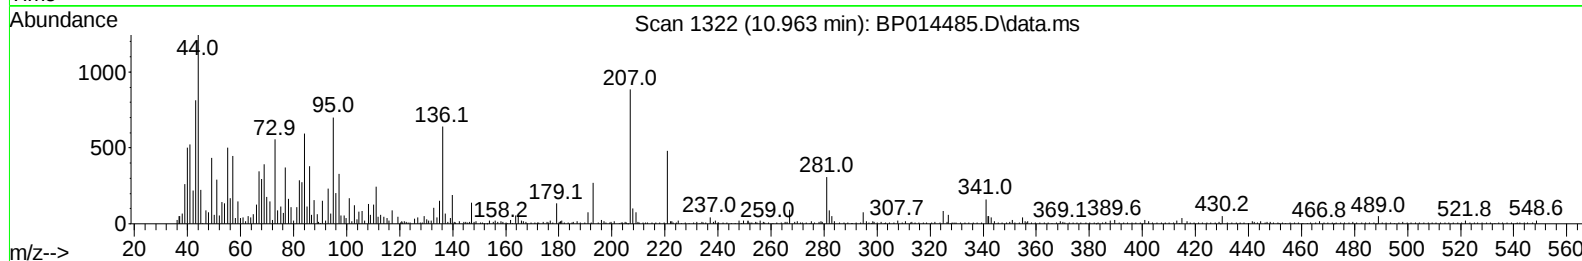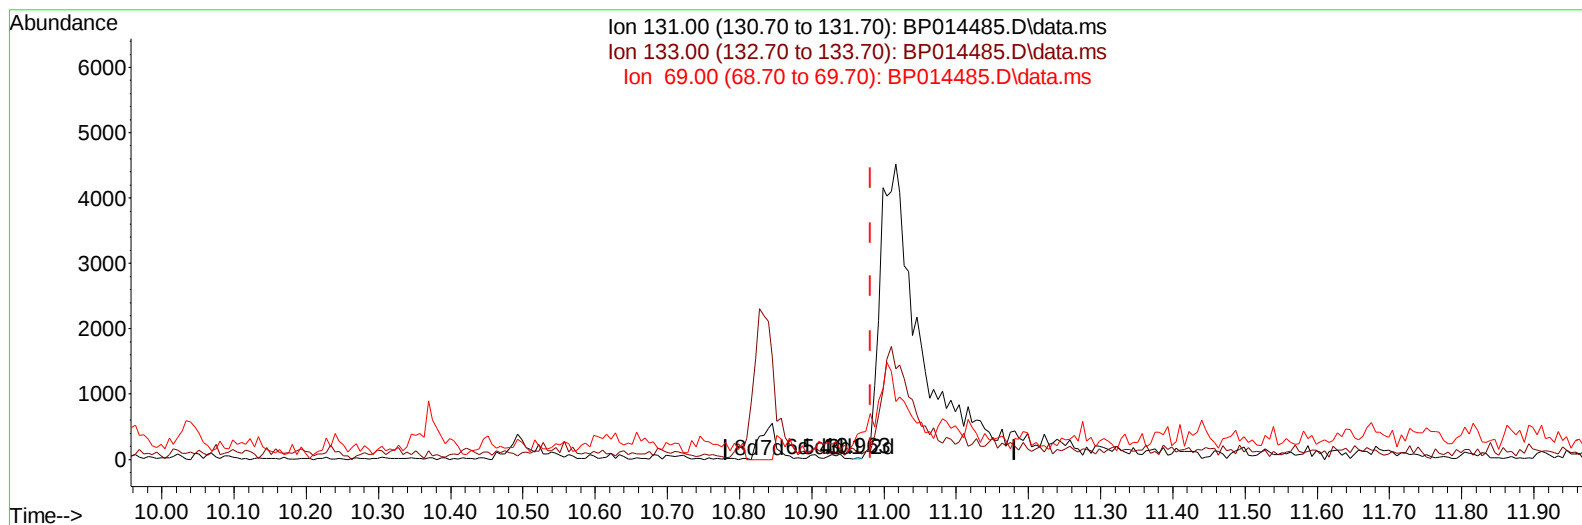

TIC: BP014485.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.963min (-0.018) 0.00 ng/u1

response 5

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	495.24#
69.00	21.30	1861.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014485.D
 Acq On : 03 Apr 2023 14:07
 Operator : CG/JU
 Sample : 02093-10DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:52:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

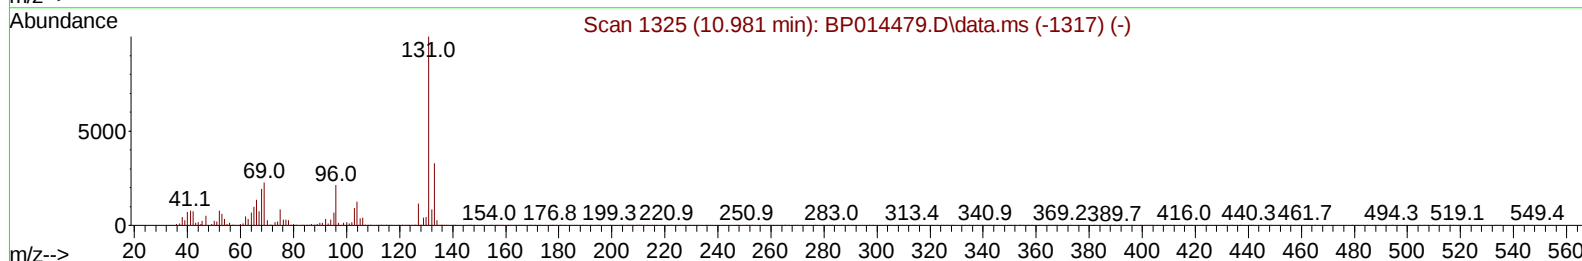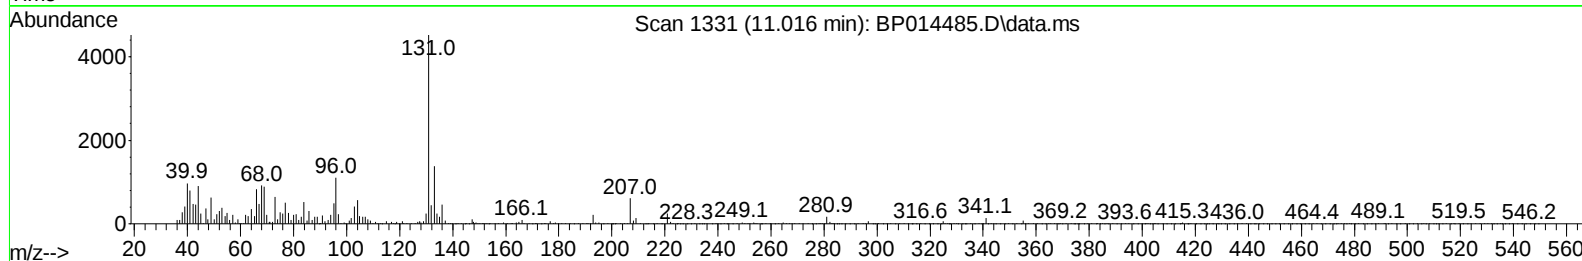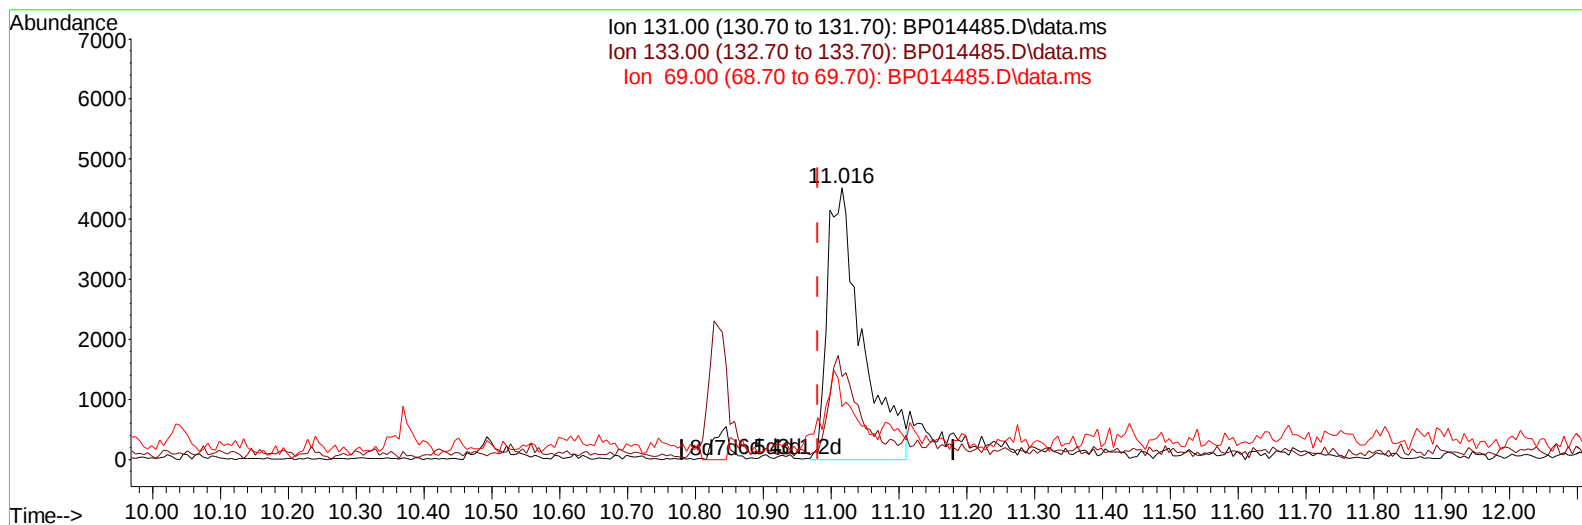

TIC: BP014485.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.016min (+ 0.035) 1.33 ng/ul m

response 15947

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.58
69.00	21.30	19.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014485.D
 Acq On : 03 Apr 2023 14:07
 Operator : CG/JU
 Sample : 02093-10DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:52:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	122394	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	542704	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.663	164	377876	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	902360	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	931202	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	950243	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	1070	0.339	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.210	99	6818m	0.604	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.340	67	19199	2.651	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	15997	1.961	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113	11866	1.303	ng/ul	0.02
21) Nitrobenzene-d5	9.193	128	8595	1.962	ng/ul	0.00
24) 2-Nitrophenol-d4	9.928	143	10757	2.144	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.499	165	18596m	2.035	ng/ul	0.04
31) 4-Chloroaniline-d4	11.016	131	15947m	1.325	ng/ul	0.04
46) Dimethylphthalate-d6	14.075	166	86537	2.824	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	82732	2.434	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.663	176	74964	2.934	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.528	188	123050	2.818	ng/ul	0.00
81) Pyrene-d10	19.757	212	161686	2.585	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	139198	2.757	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	52078	15.015	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014485.D
Acq On : 03 Apr 2023 14:07
Operator : CG/JU
Sample : 02093-10DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:52:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

