




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014488.D
 Acq On : 03 Apr 2023 15:49
 Operator : CG/JU
 Sample : PB151780BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK780

Manual IntegrationsAPPROVED

Quant Time: Apr 04 00:54:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

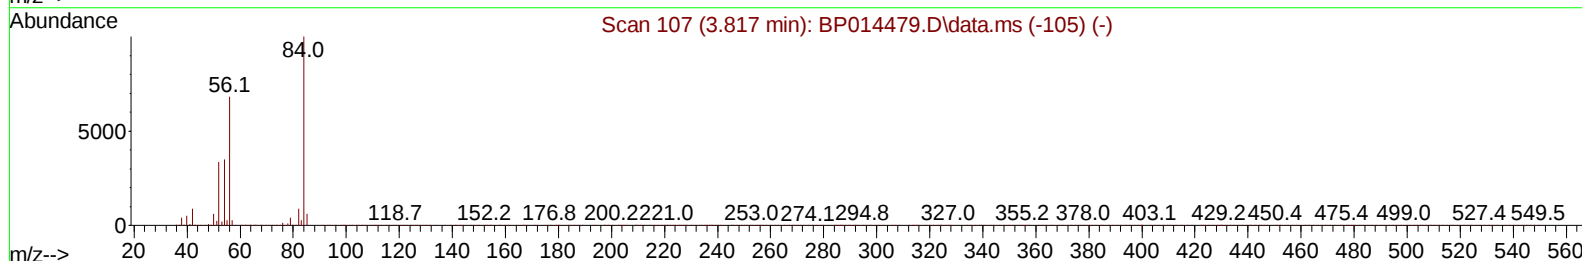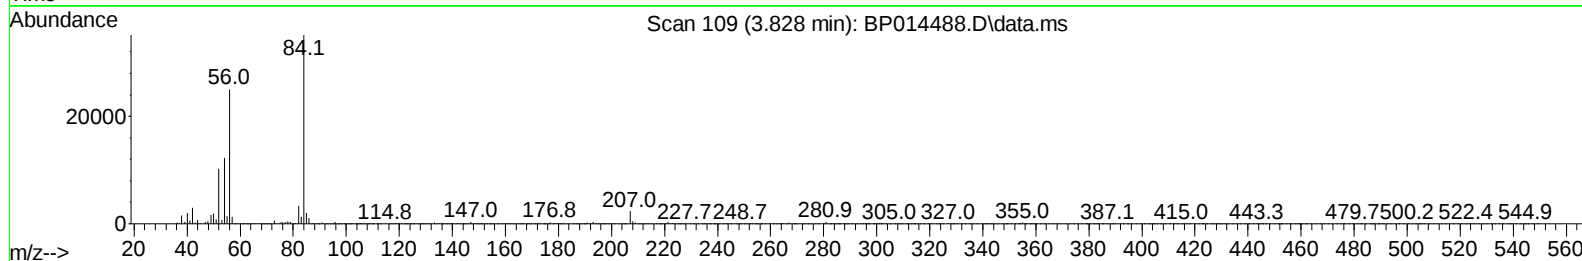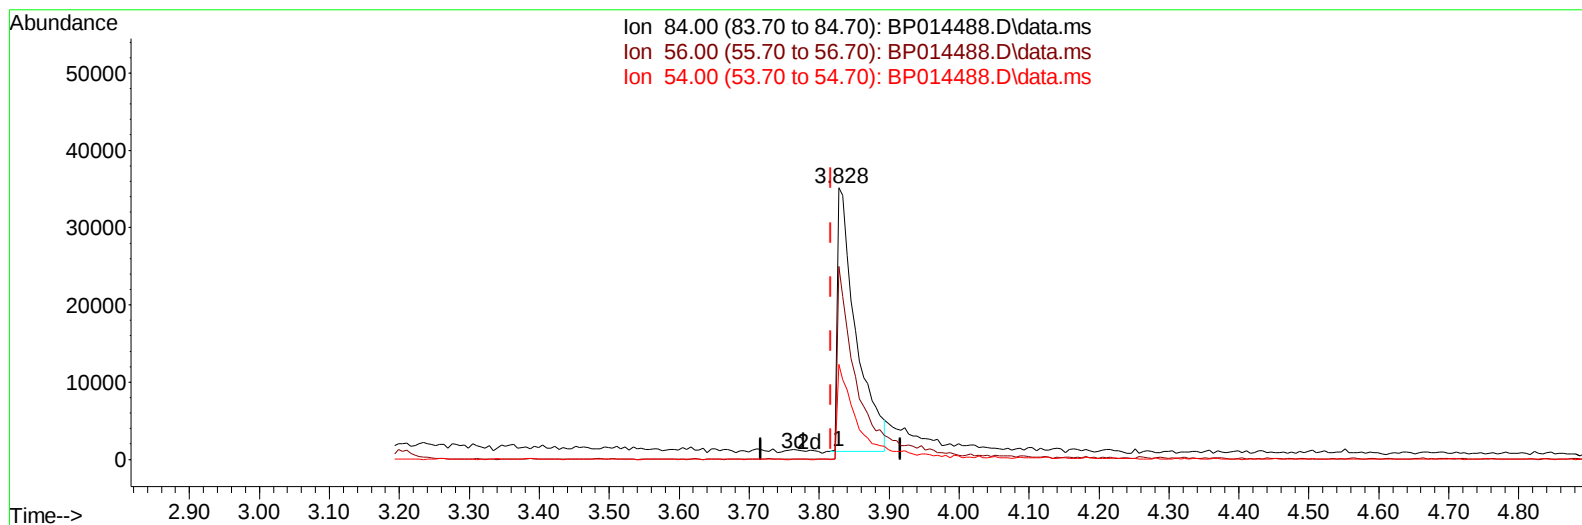

TIC: BP014488.D\data.ms

(4) Pyridine-d5 (S)

3.828min (+ 0.012) 8.14 ng/u1

response 62877

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	71.20
54.00	32.60	35.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

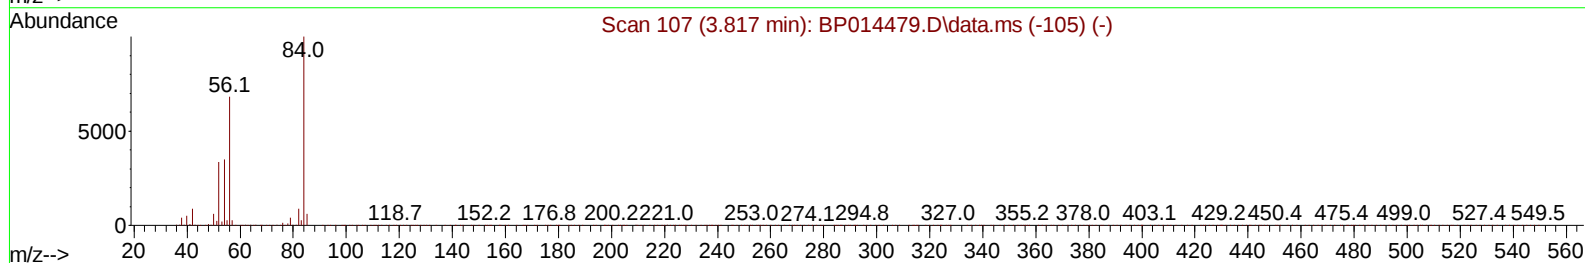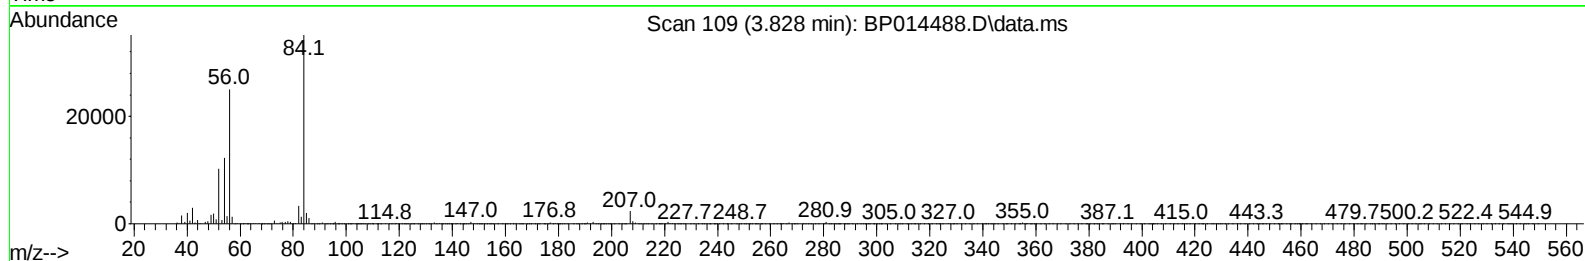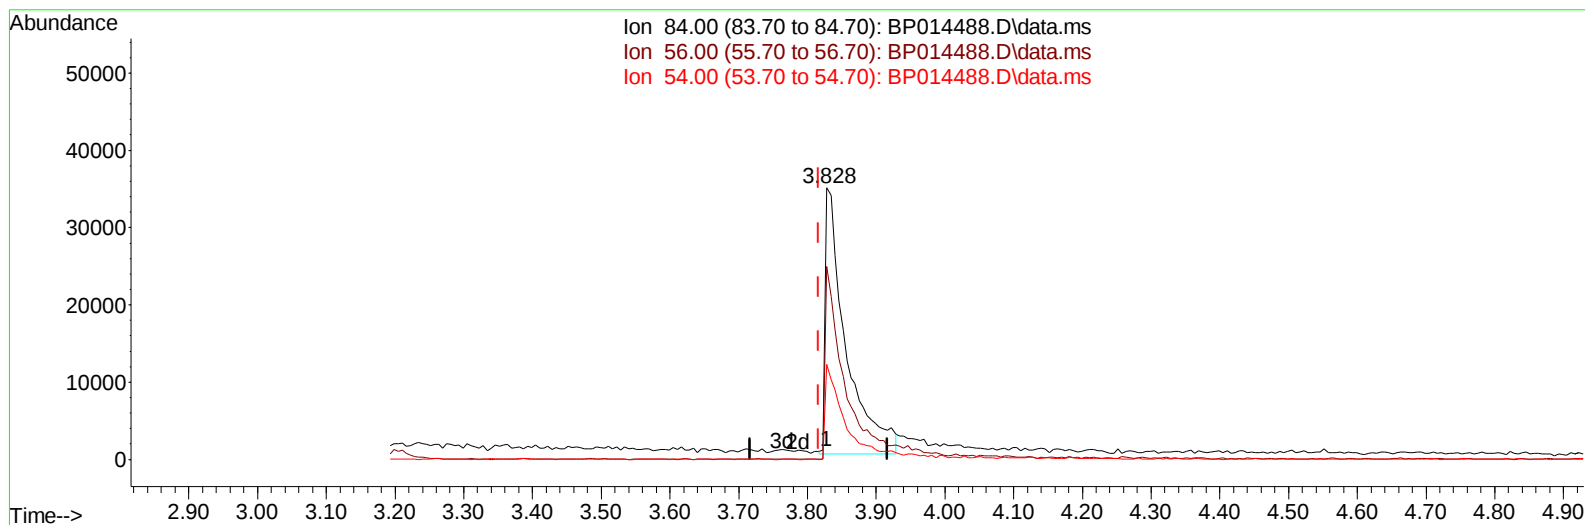

TIC: BP014488.D\data.ms

(4) Pyridine-d5 (S)

3.828min (+ 0.012) 9.24 ng/u1 m

response 71409

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	71.20
54.00	32.60	35.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

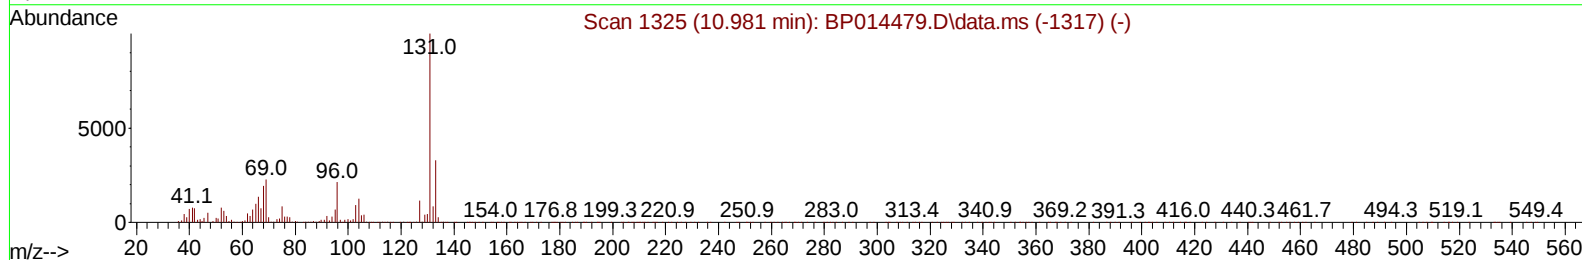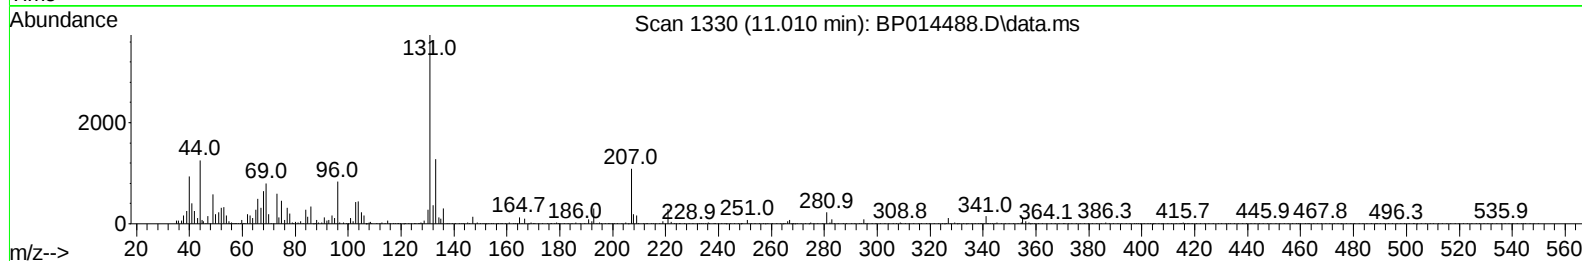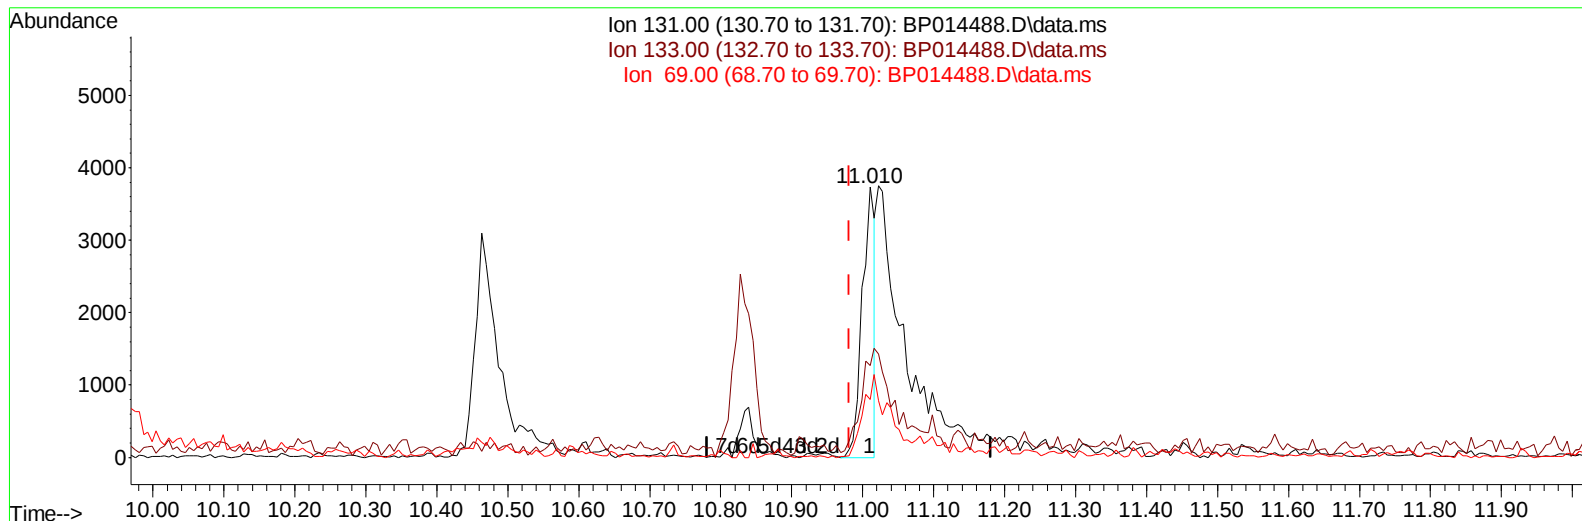

TIC: BP014488.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.010min (+ 0.029) 0.40 ng/u1

response 4663

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	34.10
69.00	21.30	21.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

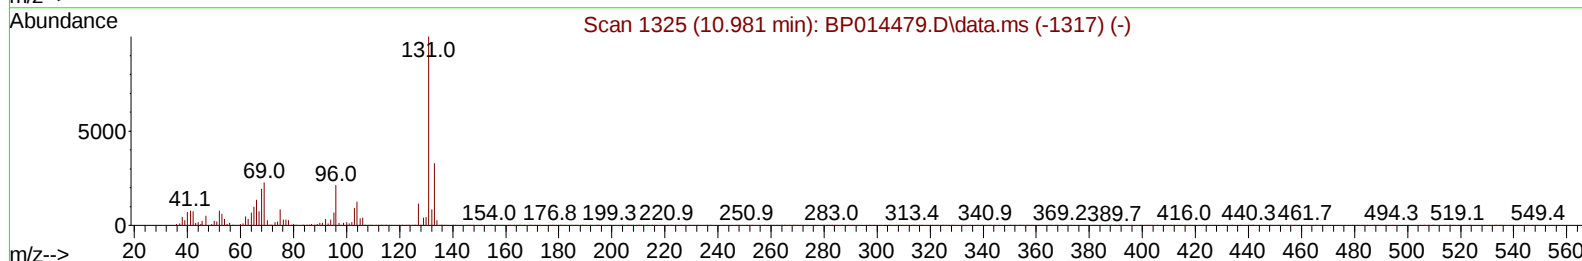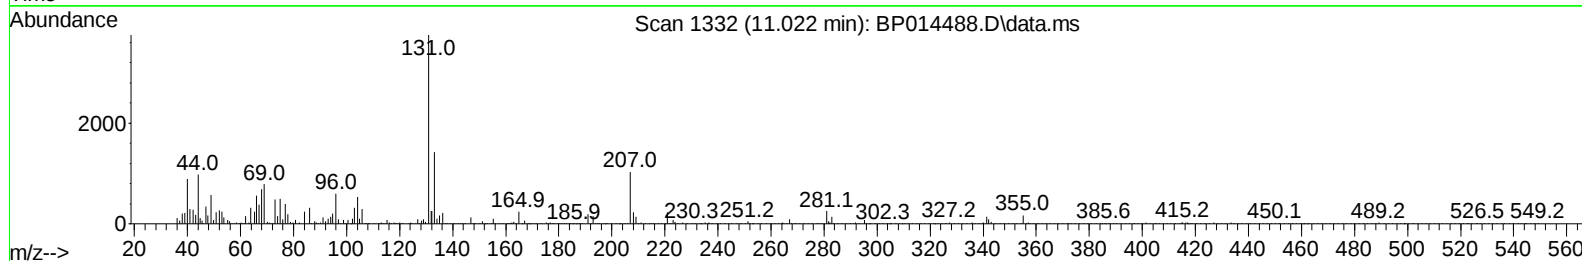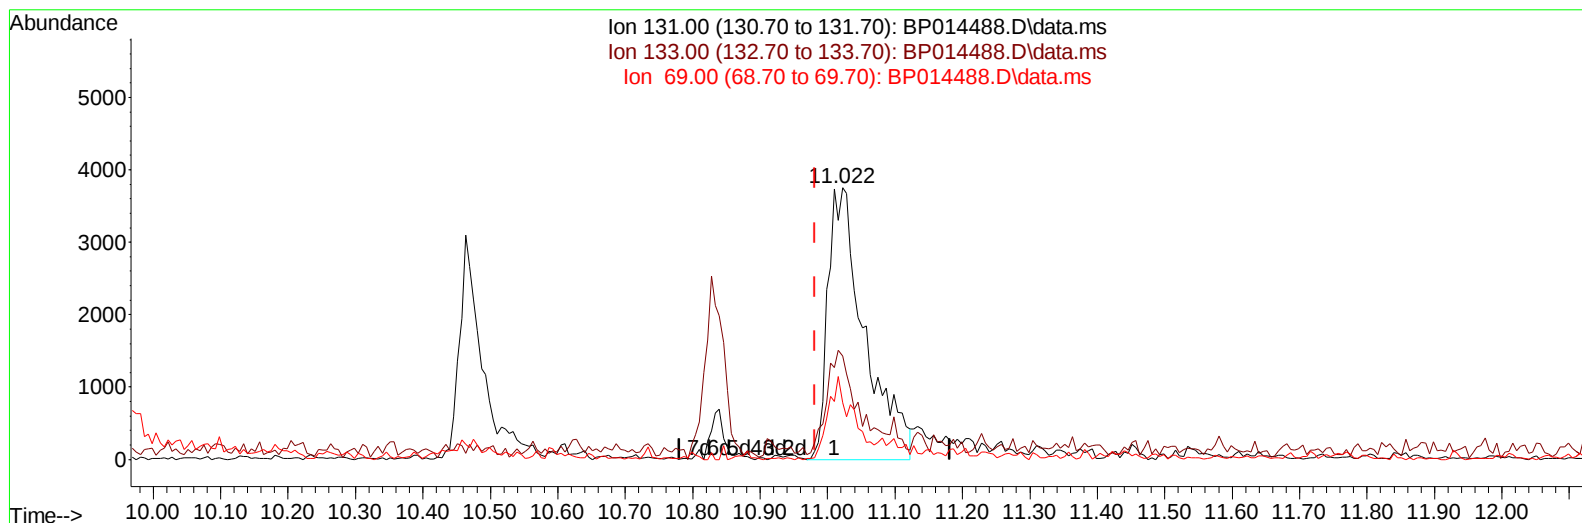

TIC: BP014488.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.022min (+ 0.041) 1.21 ng/ul m

response 14187

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	38.13
69.00	21.30	20.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

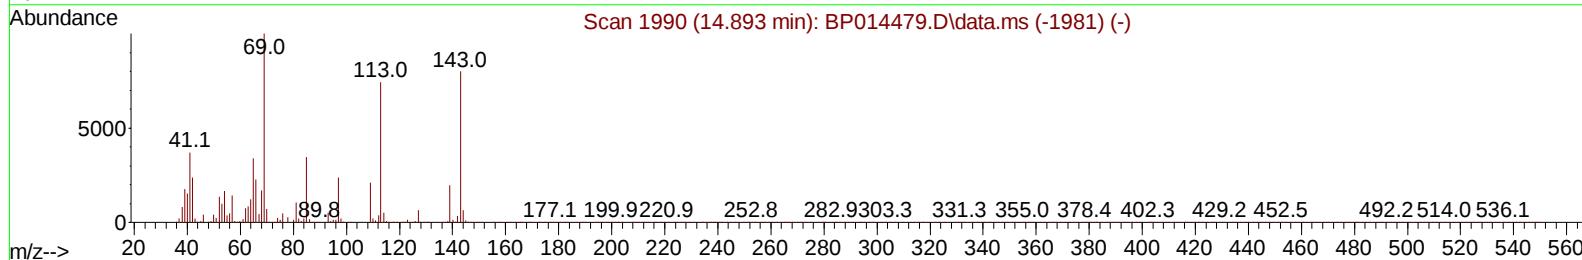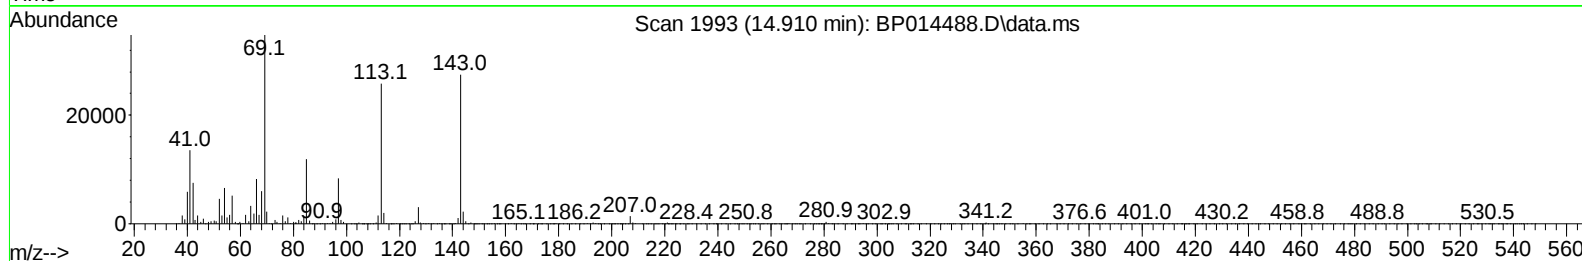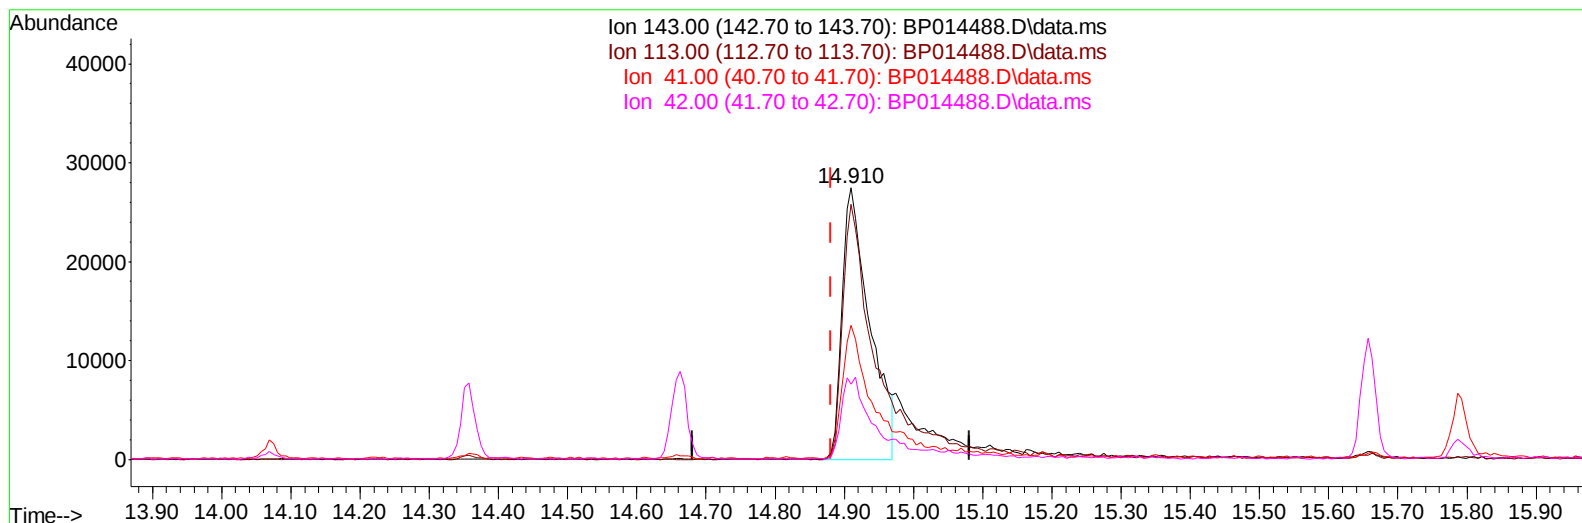

TIC: BP014488.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.029) 16.65 ng/u1

response 76086

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	93.85
41.00	44.20	49.30
42.00	31.50	27.65




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

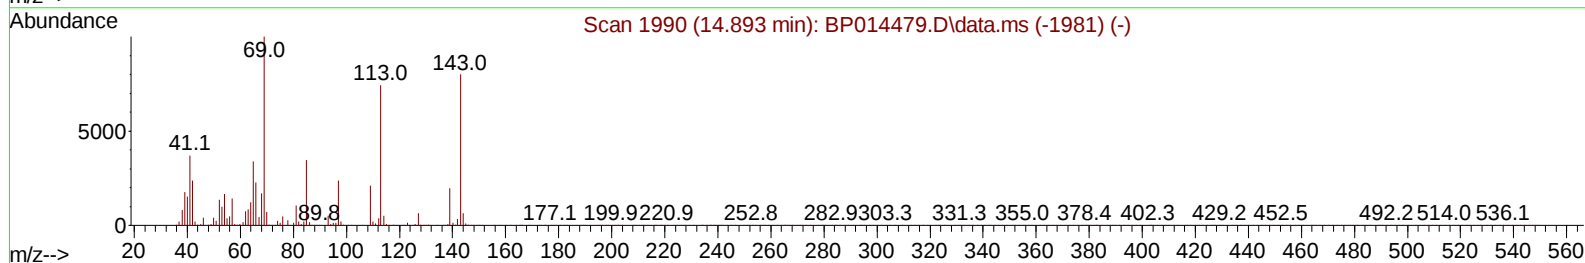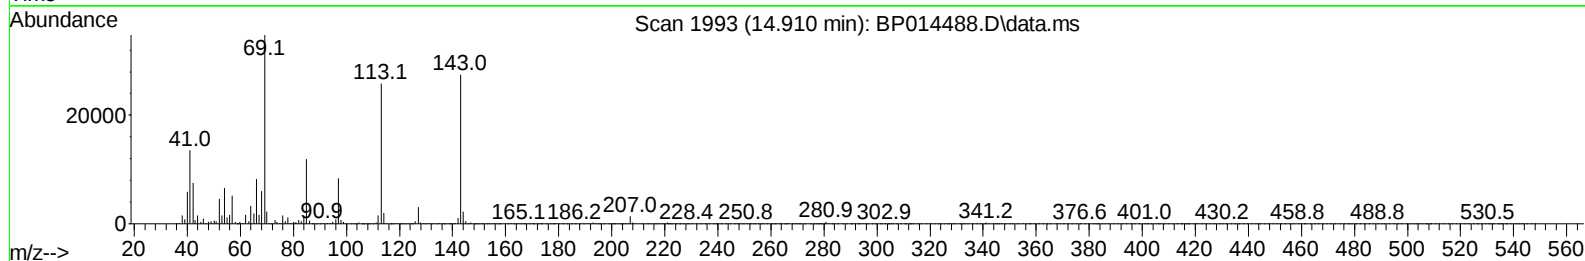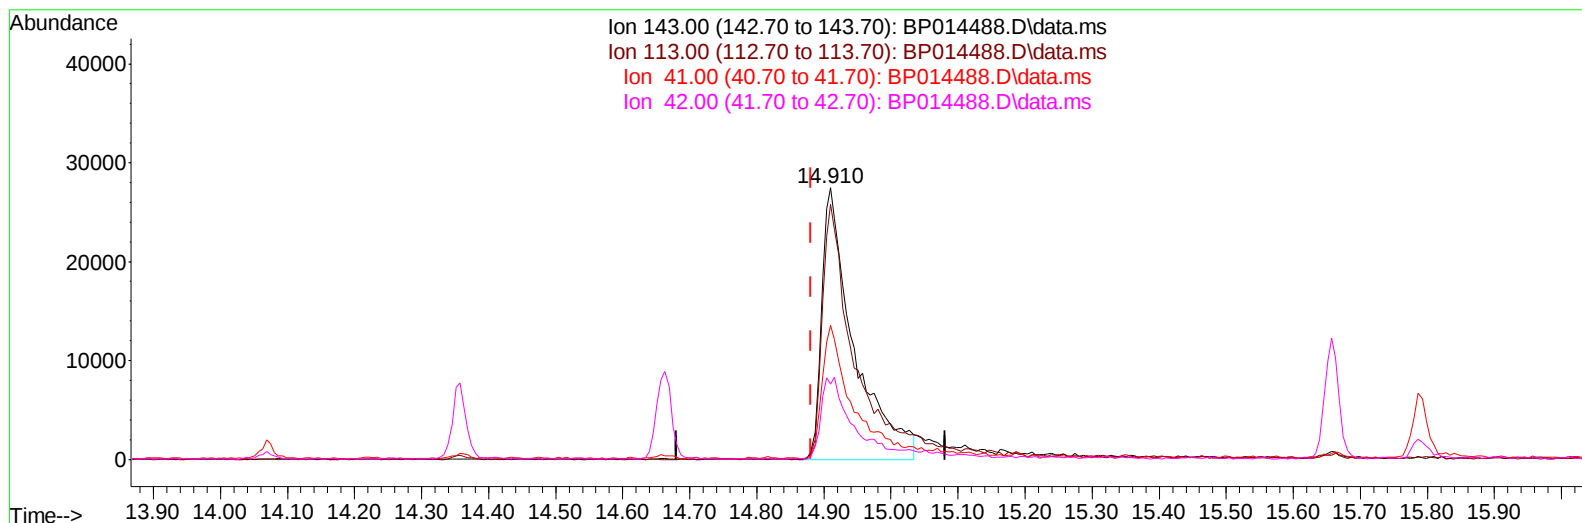

TIC: BP014488.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.029) 19.93 ng/ul m

response 91083

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	93.85
41.00	44.20	49.30
42.00	31.50	27.65

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014488.D
 Acq On : 03 Apr 2023 15:49
 Operator : CG/JU
 Sample : PB151780BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	116936	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	530529	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	373149	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	922169	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	1030025	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	1073297	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	12045	3.994	ng/uL	0.00
4) Pyridine-d5	3.828	84	71409m	9.241	ng/ul	0.01
7) Phenol-d5	7.181	99	241216	22.367	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	156688	22.645	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	180900	23.208	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	195369	22.459	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	89143	20.814	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	106787	21.775	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	185965	20.821	ng/ul	0.01
31) 4-Chloroaniline-d4	11.022	131	14187m	1.206	ng/ul	0.04
46) Dimethylphthalate-d6	14.069	166	681026	22.509	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	737121	21.957	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	91083m	19.927	ng/ul	0.03
60) Fluorene-d10	15.657	176	597586	23.685	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	105478	15.545	ng/ul	0.00
73) Anthracene-d10	17.528	188	1034375	23.177	ng/ul	0.00
81) Pyrene-d10	19.751	212	1358173	19.631	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1316236	23.082	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:54:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

