




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014496.D
Acq On : 03 Apr 2023 20:21
Operator : CG/JU
Sample : 02093-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB991

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:39:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

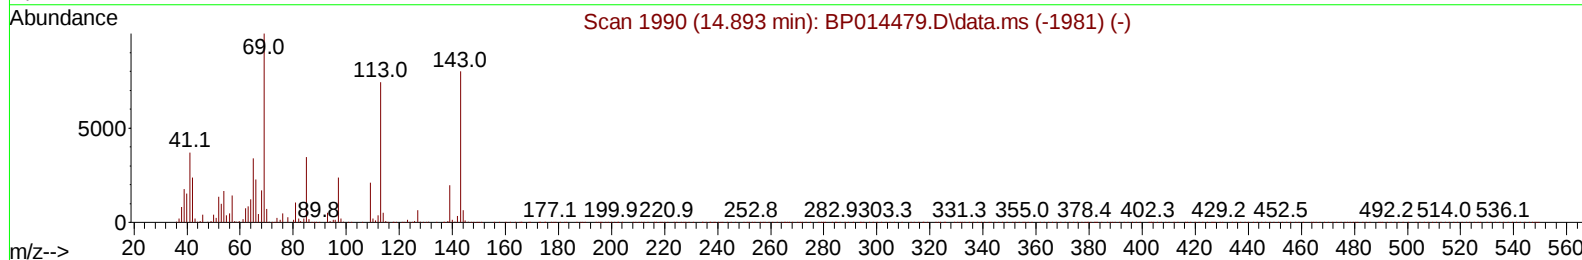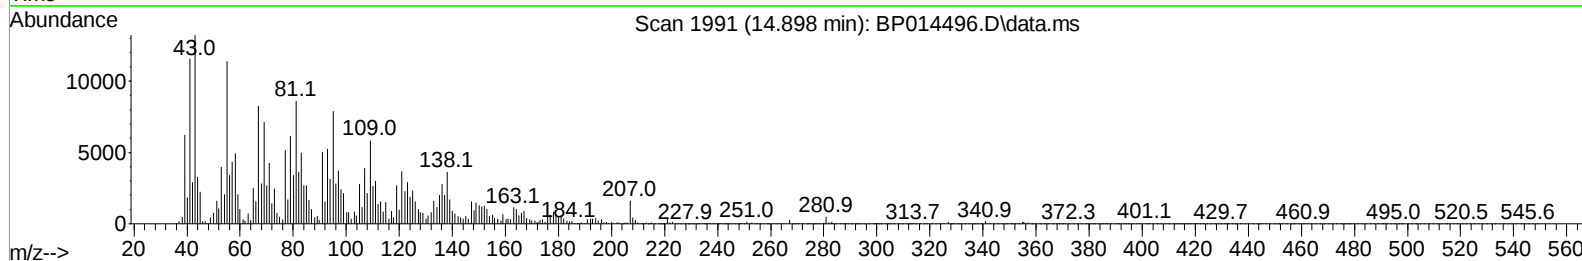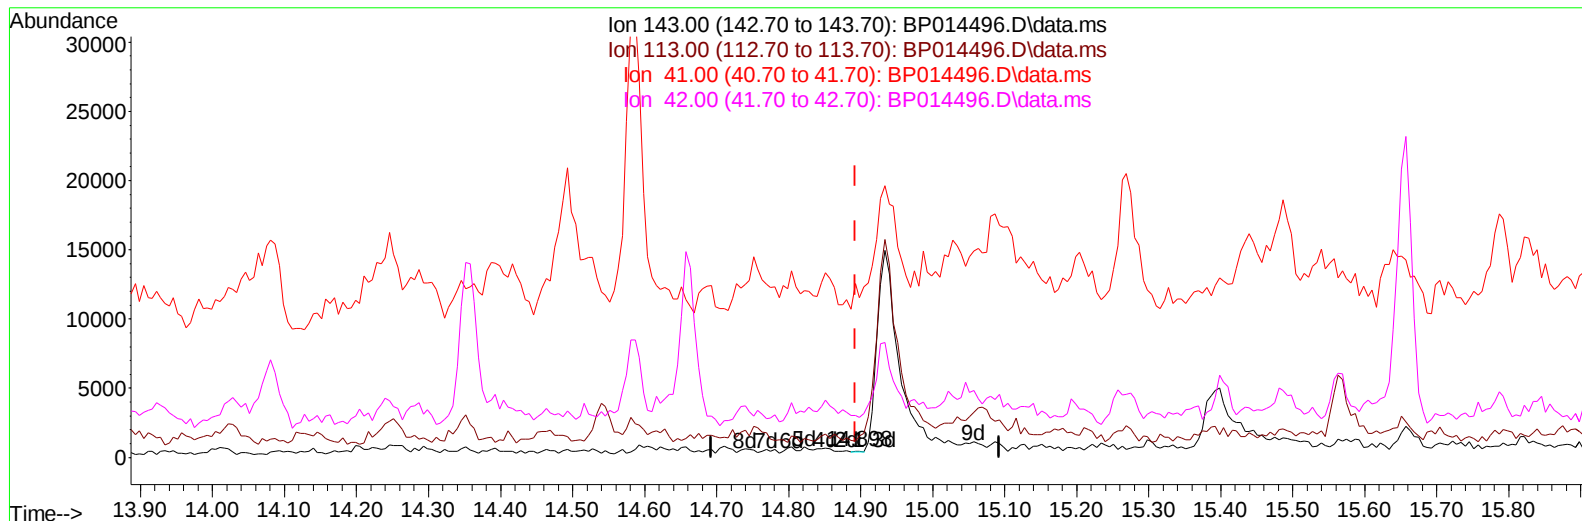

TIC: BP014496.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.898min (+ 0.006) 0.01 ng/ul

response 39

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	343.08#
41.00	44.20	2540.00#
42.00	31.50	641.10#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014496.D
Acq On : 03 Apr 2023 20:21
Operator : CG/JU
Sample : 02093-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB991

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:39:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

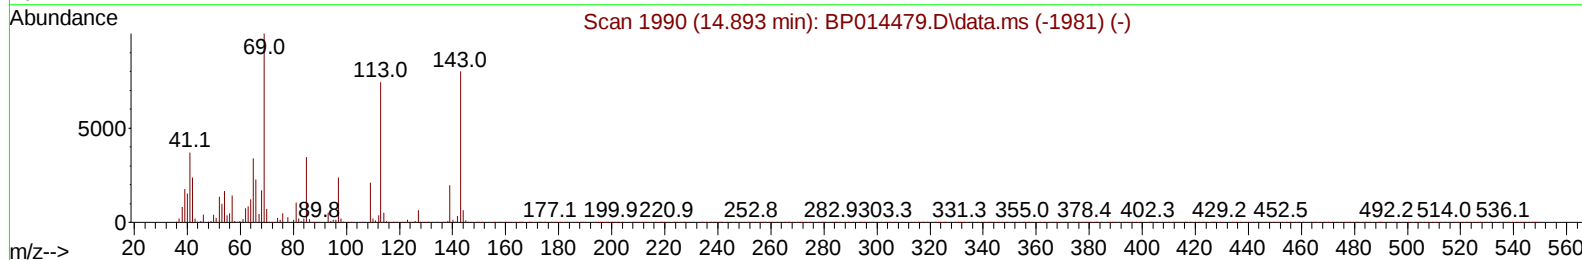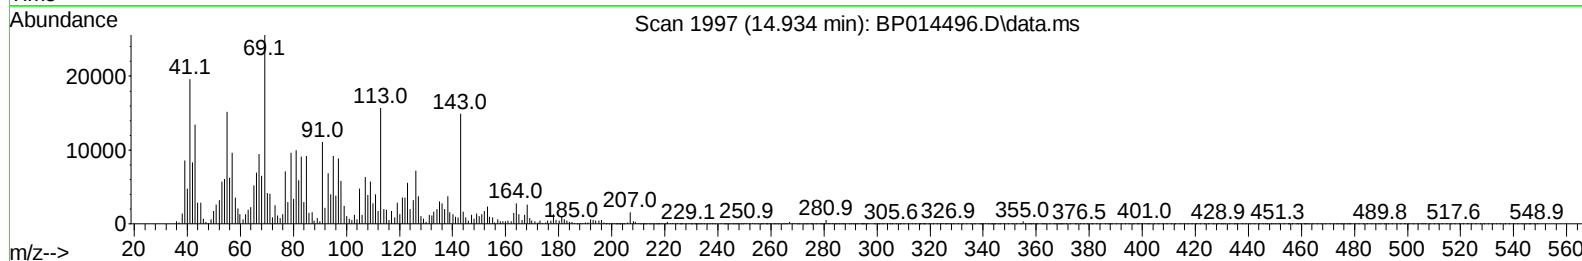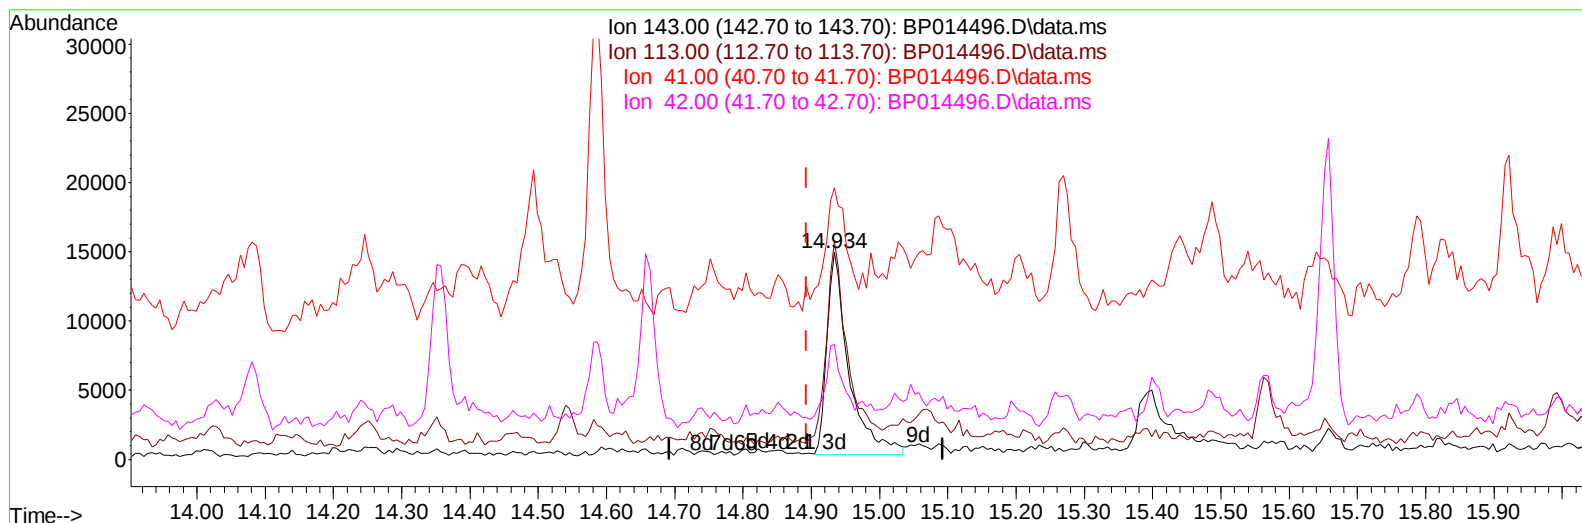

TIC: BP014496.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.041) 5.67 ng/ul m

response 32575

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	105.29
41.00	44.20	131.28#
42.00	31.50	55.55#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014496.D
 Acq On : 03 Apr 2023 20:21
 Operator : CG/JU
 Sample : 02093-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB991

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:39:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	160136	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	706321	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	469077	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	1068724	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	927499	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	881101	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	16395	3.970	ng/uL	0.00
4) Pyridine-d5	3.823	84	184222	17.409	ng/ul	0.00
7) Phenol-d5	7.181	99	145678	9.864	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	272611	28.770	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	264202	24.751	ng/ul	0.00
15) 4-Methylphenol-d8	8.740	113	264654	22.216	ng/ul	0.01
21) Nitrobenzene-d5	9.187	128	163432	28.662	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	175117	26.821	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	327404	27.534	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	427150	27.272	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166	1183838	31.126	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	1251787	29.662	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	32575m	5.669	ng/ul	0.04
60) Fluorene-d10	15.657	176	962812	30.356	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	90792	11.546	ng/ul	0.00
73) Anthracene-d10	17.522	188	1579539	30.539	ng/ul	0.00
81) Pyrene-d10	19.757	212	1841353	29.556	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.869	264	1420975	30.355	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	975226	214.903	ng/uL	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014496.D
Acq On : 03 Apr 2023 20:21
Operator : CG/JU
Sample : 02093-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB991

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 01:39:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

