




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014498.D
Acq On : 03 Apr 2023 21:28
Operator : CG/JU
Sample : 02093-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB994

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

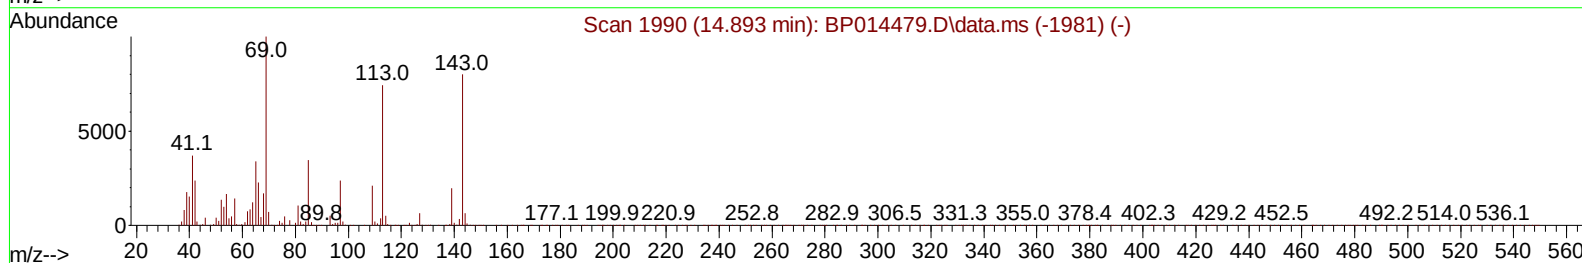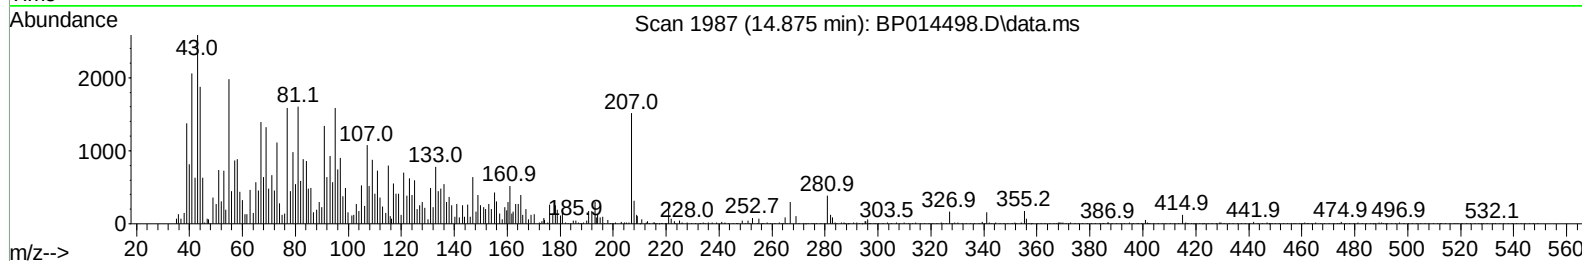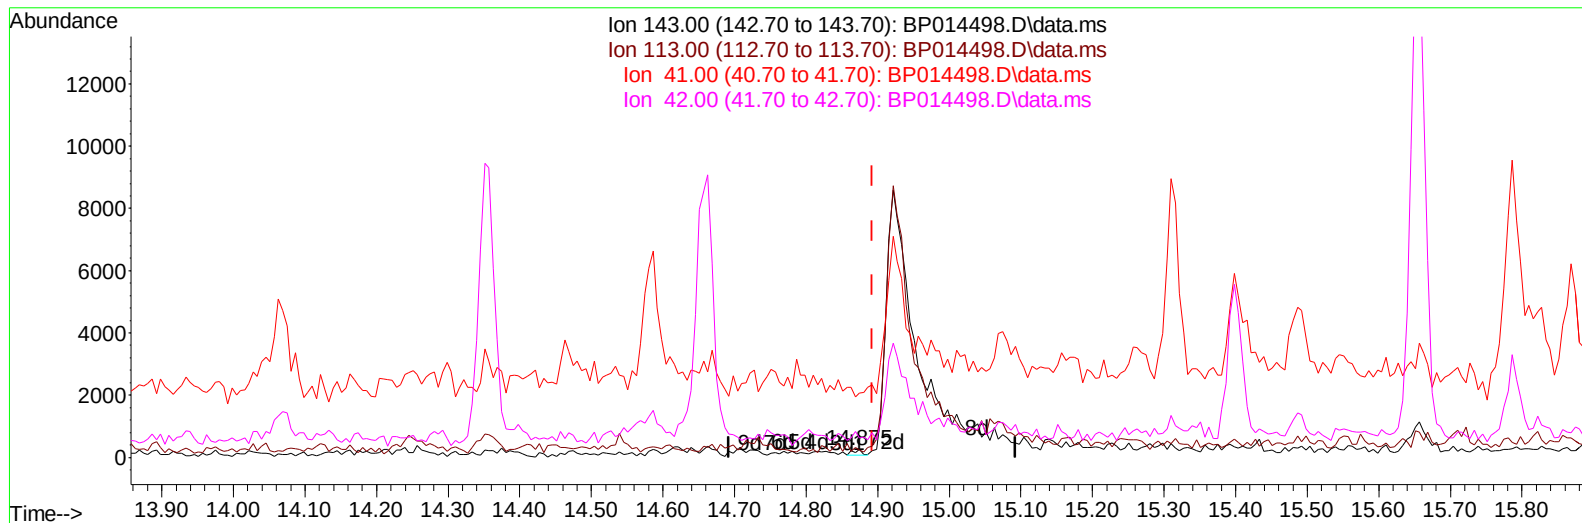

TIC: BP014498.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (-0.018) 0.03 ng/u1

response 152

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	93.00
41.00	44.20	802.33#
42.00	31.50	247.08#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014498.D
Acq On : 03 Apr 2023 21:28
Operator : CG/JU
Sample : 02093-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB994

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

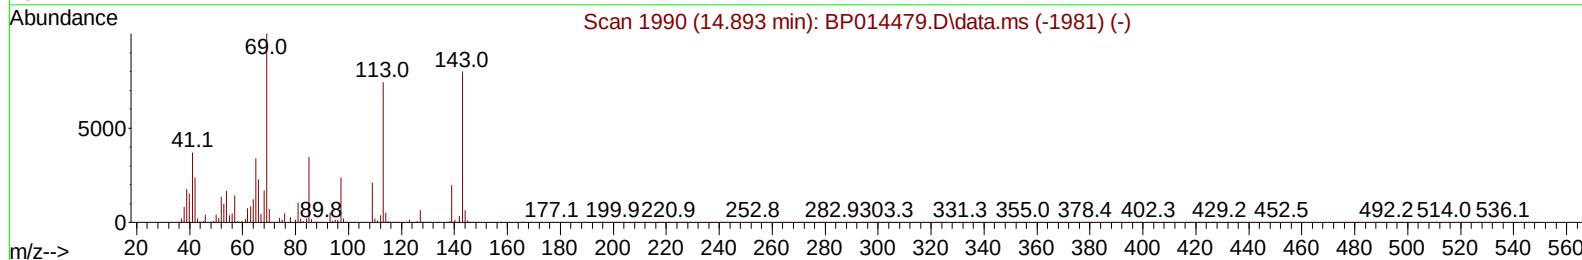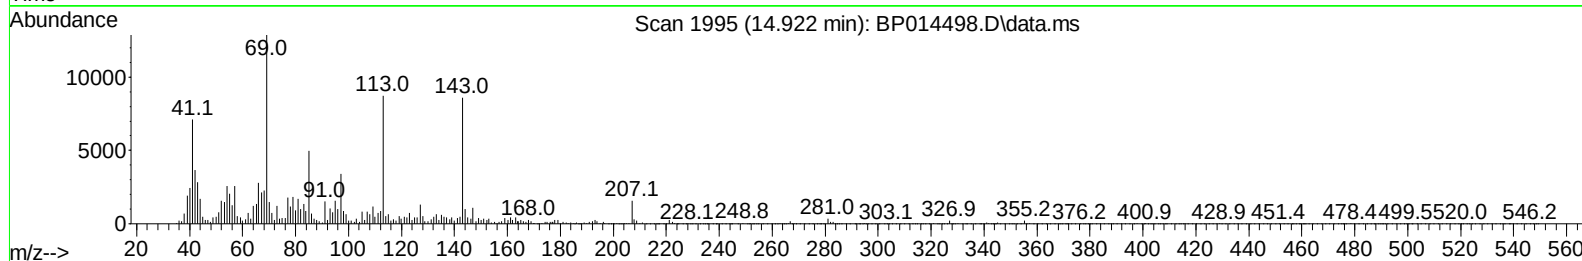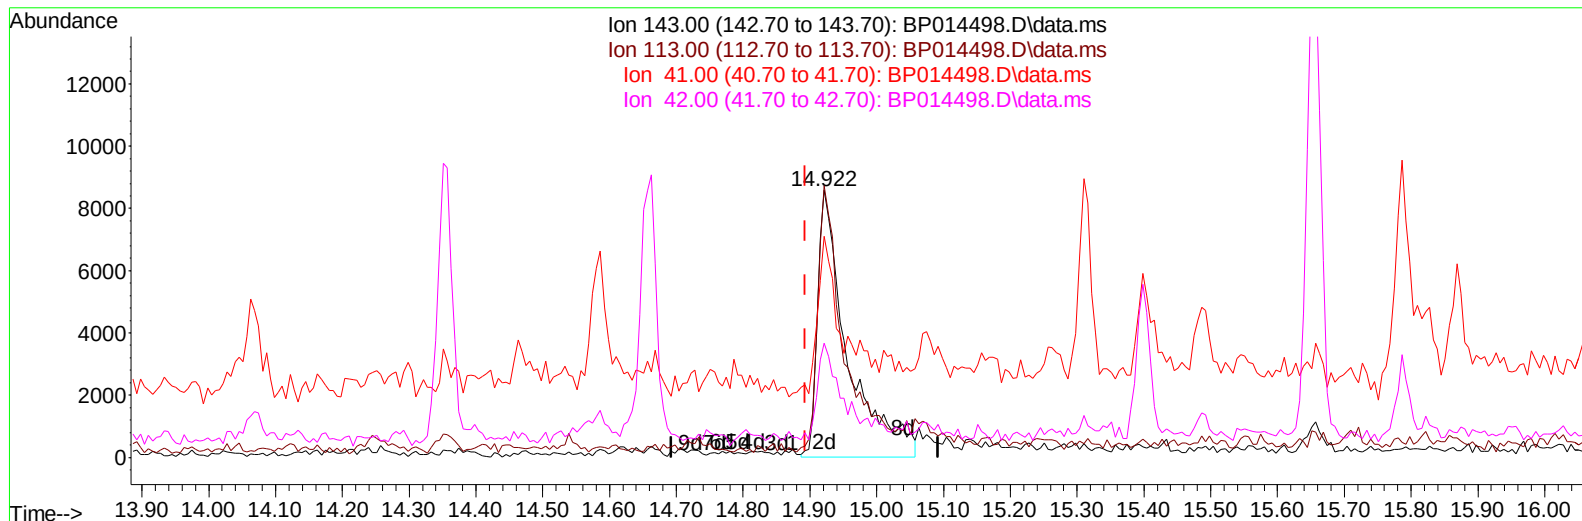

TIC: BP014498.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.029) 5.71 ng/ul m

response 26408

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	101.67
41.00	44.20	82.76#
42.00	31.50	42.70#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014498.D
 Acq On : 03 Apr 2023 21:28
 Operator : CG/JU
 Sample : 02093-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB994

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 01:39:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	122309	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	544529	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	377683	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.421	188	893298	20.000	ng/ul	0.00
79) Chrysene-d12	21.509	240	911142	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	913335	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	13159	4.172	ng/uL	0.00
4) Pyridine-d5	3.822	84	142888	17.679	ng/ul	0.00
7) Phenol-d5	7.181	99	78280	6.940	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	202317	27.955	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	190898	23.415	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	149863	16.471	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	120370	27.382	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	134938	26.807	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	246585	26.899	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	299124	24.772	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166	936870	30.593	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	980622	28.859	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	26408m	5.708	ng/ul	0.03
60) Fluorene-d10	15.657	176	770166	30.158	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	103558	15.755	ng/ul	0.00
73) Anthracene-d10	17.521	188	1299110	30.050	ng/ul	0.00
81) Pyrene-d10	19.751	212	1632644	26.677	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.862	264	1463350	30.157	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	23787	6.863	ng/uL	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014498.D
Acq On : 03 Apr 2023 21:28
Operator : CG/JU
Sample : 02093-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB994

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 01:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

