




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014499.D
Acq On : 03 Apr 2023 22:02
Operator : CG/JU
Sample : 02092-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB996

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

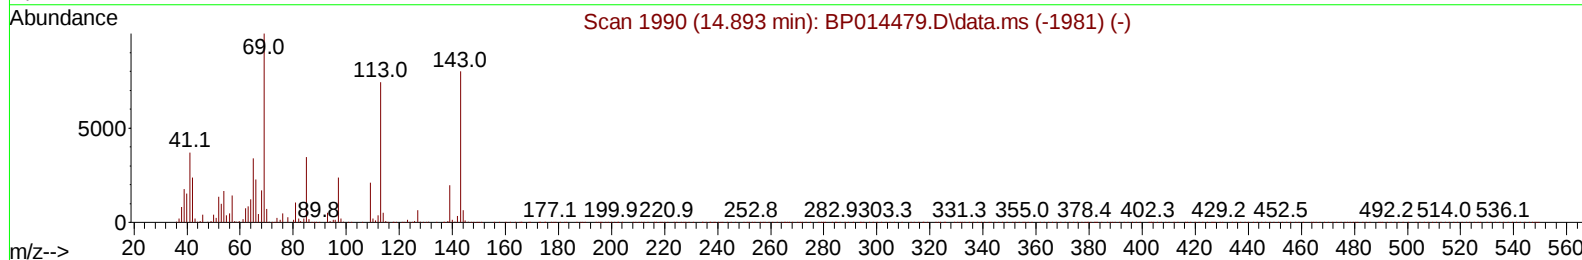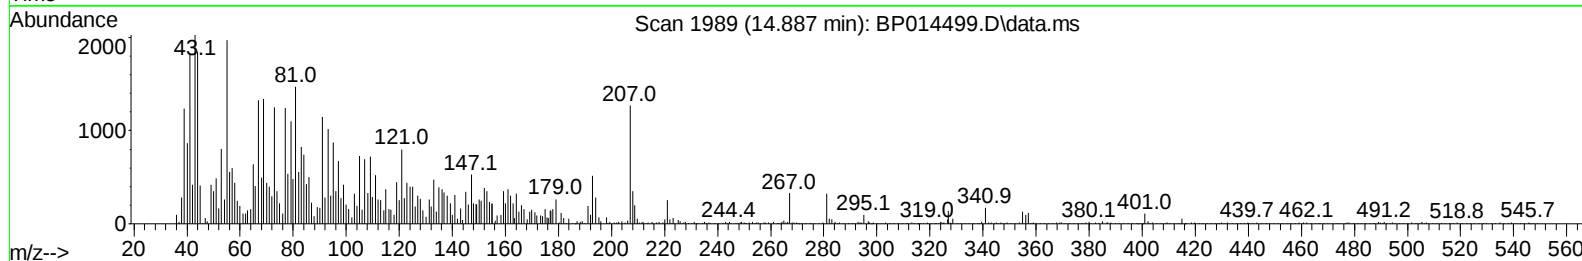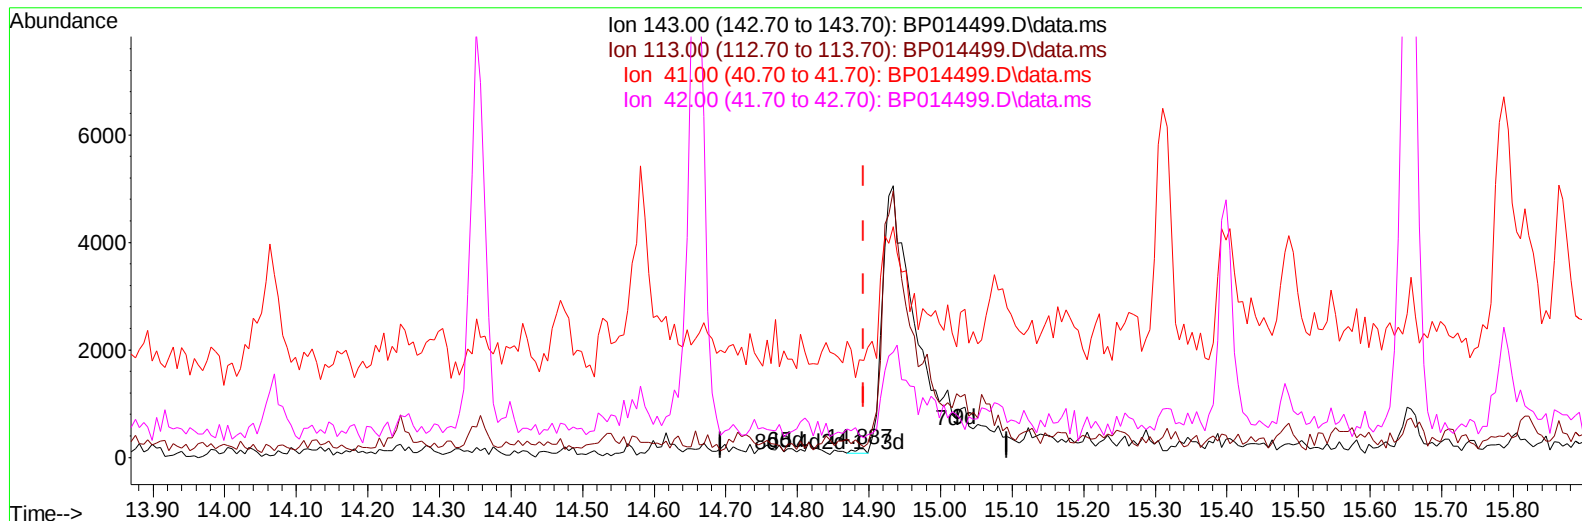

TIC: BP014499.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.887min (-0.006) 0.02 ng/u1

response 98

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	152.98#
41.00	44.20	1084.52#
42.00	31.50	247.62#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014499.D
Acq On : 03 Apr 2023 22:02
Operator : CG/JU
Sample : 02092-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB996

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

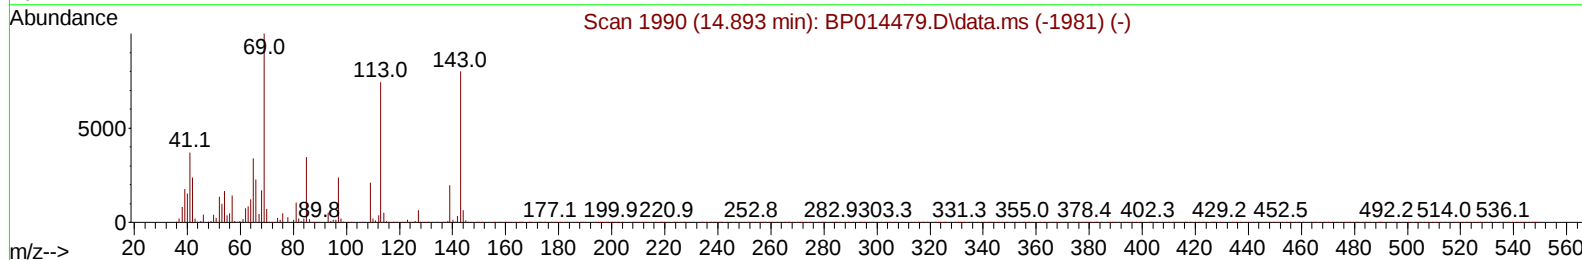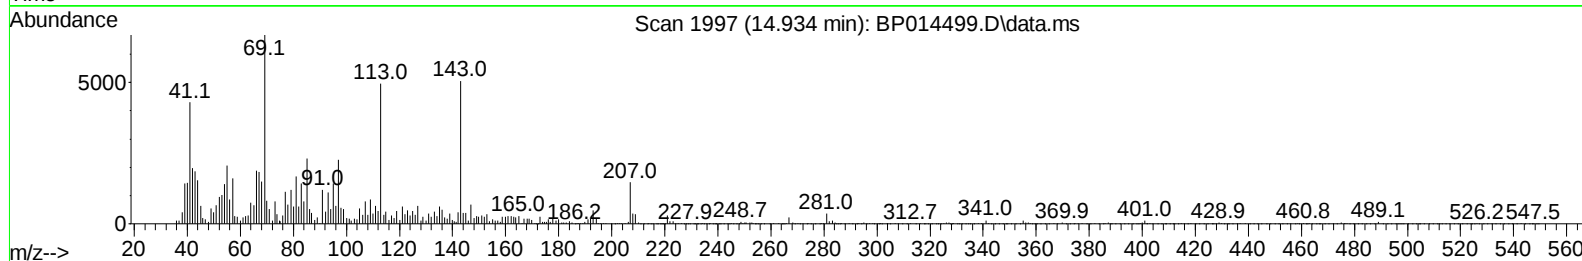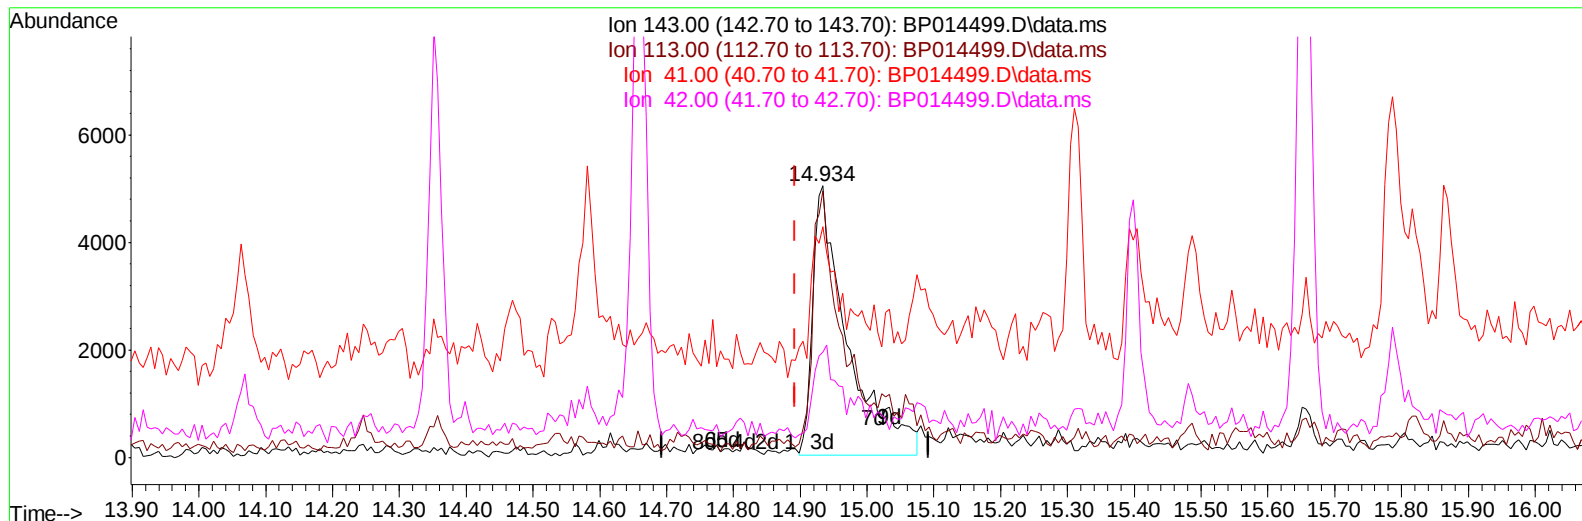

TIC: BP014499.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.041) 3.86 ng/ul m

response 18264

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	98.18
41.00	44.20	85.07#
42.00	31.50	38.88#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014499.D
 Acq On : 03 Apr 2023 22:02
 Operator : CG/JU
 Sample : 02092-22
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB996

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 01:40:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	123581	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	560282	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164	386568	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	915426	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	904220	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	895126	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	12446	3.906	ng/uL	0.00
4) Pyridine-d5	3.823	84	95656	11.713	ng/ul	0.00
7) Phenol-d5	7.187	99	51770	4.542	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	154508	21.129	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	136063	16.517	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	105436	11.469	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	92550	20.462	ng/ul	0.00
24) 2-Nitrophenol-d4	9.911	143	98173	18.955	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.458	165	185526	19.669	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	239278	19.259	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166	765287	24.416	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	766603	22.042	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	18264m	3.857	ng/ul	0.04
60) Fluorene-d10	15.657	176	618148	23.649	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	76531	11.362	ng/ul	0.00
73) Anthracene-d10	17.522	188	1040139	23.478	ng/ul	0.00
81) Pyrene-d10	19.751	212	1284768	21.153	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.863	264	1114323	23.431	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	17125	4.890	ng/uL	95
52) Acenaphthene	14.722	153	29742	1.136	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014499.D
Acq On : 03 Apr 2023 22:02
Operator : CG/JU
Sample : 02092-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB996

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 01:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

