




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014504.D
Acq On : 04 Apr 2023 00:51
Operator : CG/JU
Sample : 02158-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PMW-4(20230329)

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 02:35:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

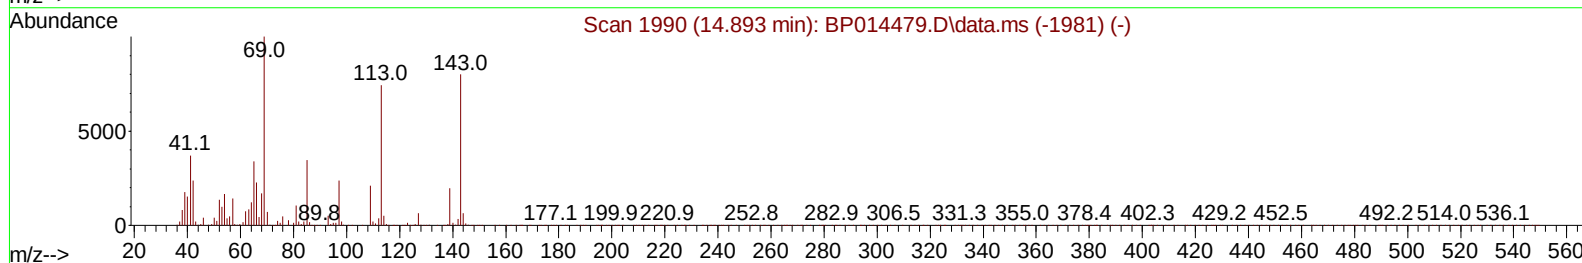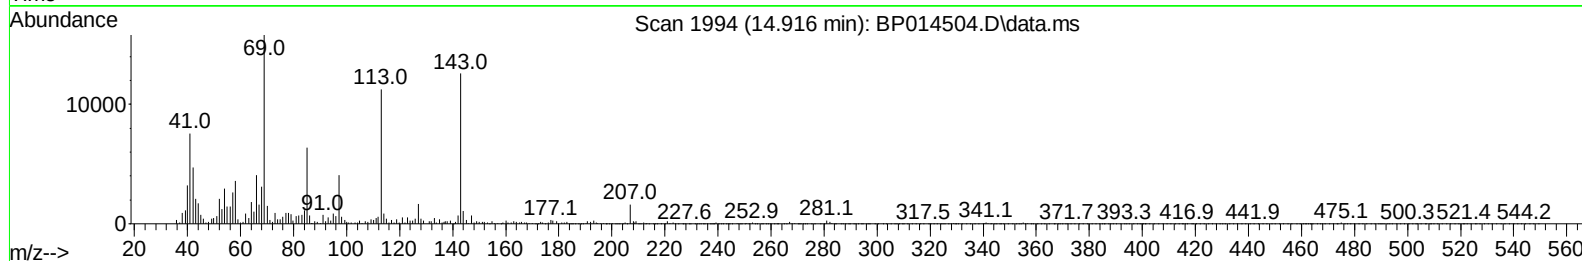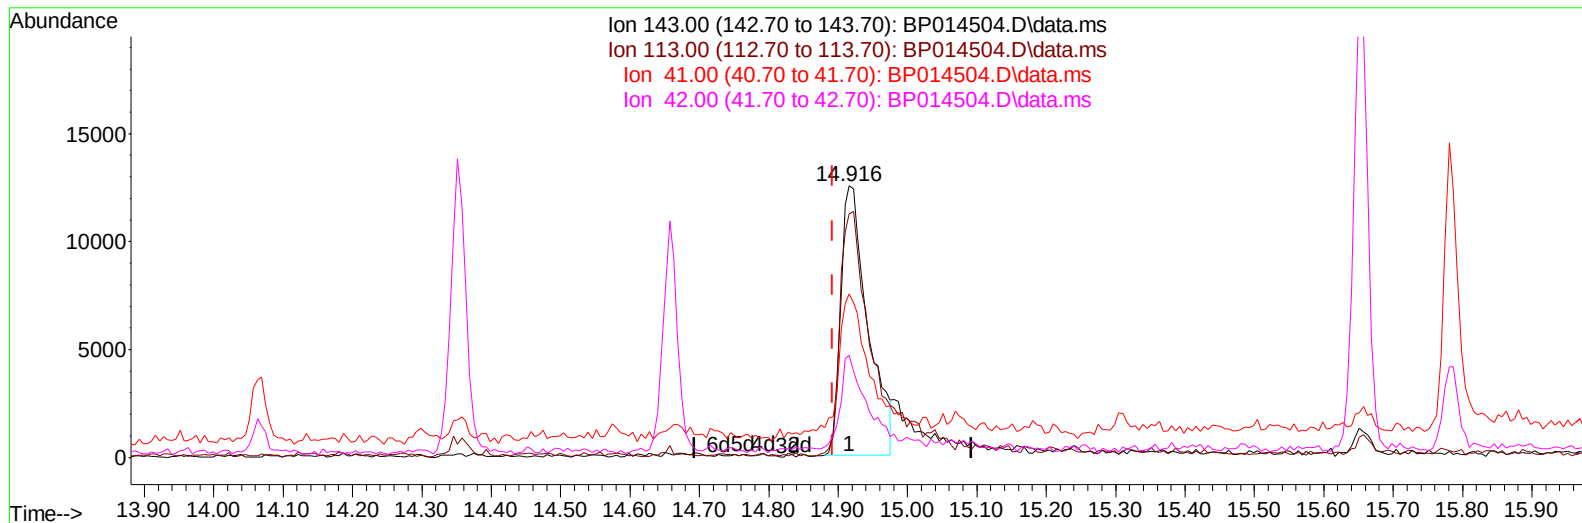

TIC: BP014504.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.023) 6.64 ng/ul

response 33939

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	89.65
41.00	44.20	60.29#
42.00	31.50	37.62

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014504.D
 Acq On : 04 Apr 2023 00:51
 Operator : CG/JU
 Sample : 02158-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-4(20230329)

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 02:35:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	137672	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	621151	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164	417551	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	969898	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	957673	20.000	ng/ul	0.00
88) Perylene-d12	24.027	264	952043	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	17322	4.879	ng/uL	0.00
4) Pyridine-d5	3.822	84	96978	10.660	ng/ul	0.00
7) Phenol-d5	7.181	99	115755	9.117	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	296984	36.456	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	287966	31.380	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	216051	21.095	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	177209	35.340	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	207113	36.070	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	354453	33.896	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	243724	17.694	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166	1284521	37.941	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	1400618	37.284	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	40150m	7.850	ng/ul	0.02
60) Fluorene-d10	15.657	176	1077270	38.156	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	203079	28.456	ng/ul	0.00
73) Anthracene-d10	17.522	188	1752770	37.342	ng/ul	0.00
81) Pyrene-d10	19.751	212	2167703	33.698	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.863	264	1887965	37.325	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014504.D
Acq On : 04 Apr 2023 00:51
Operator : CG/JU
Sample : 02158-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PMW-4(20230329)

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 02:35:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

