




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 06:18:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

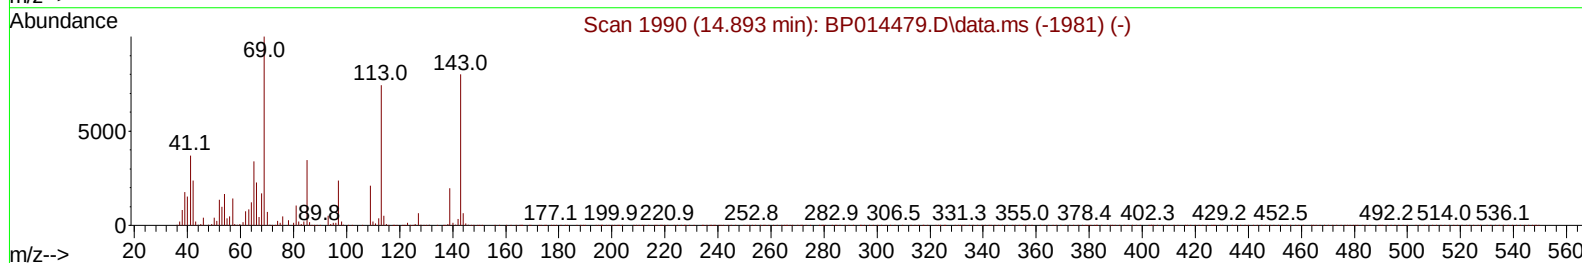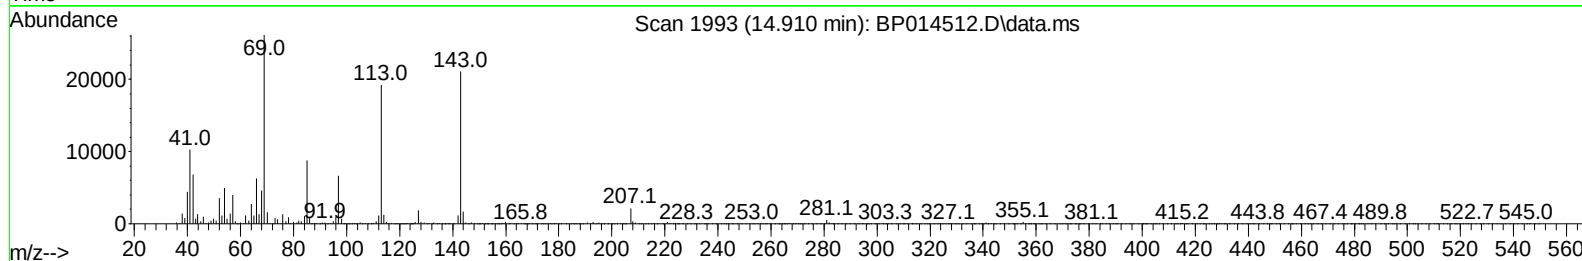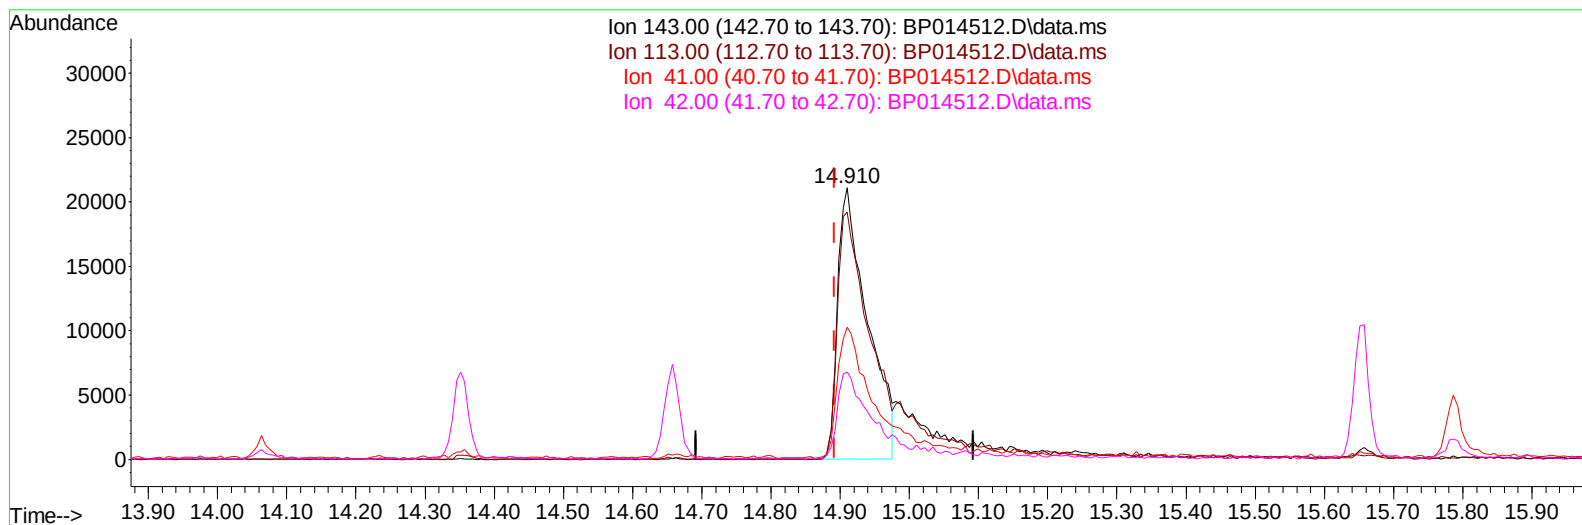

TIC: BP014512.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.018) 17.43 ng/ul

response 63140

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.13
41.00	44.20	48.63
42.00	31.50	32.28




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 06:18:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

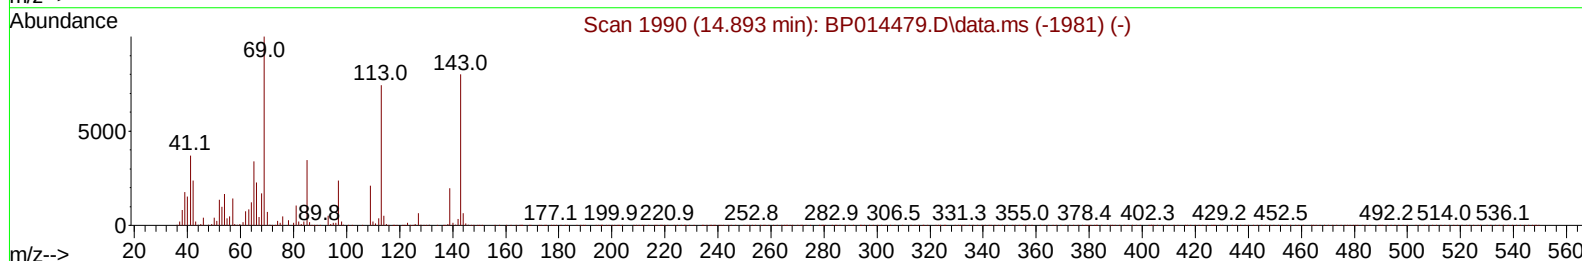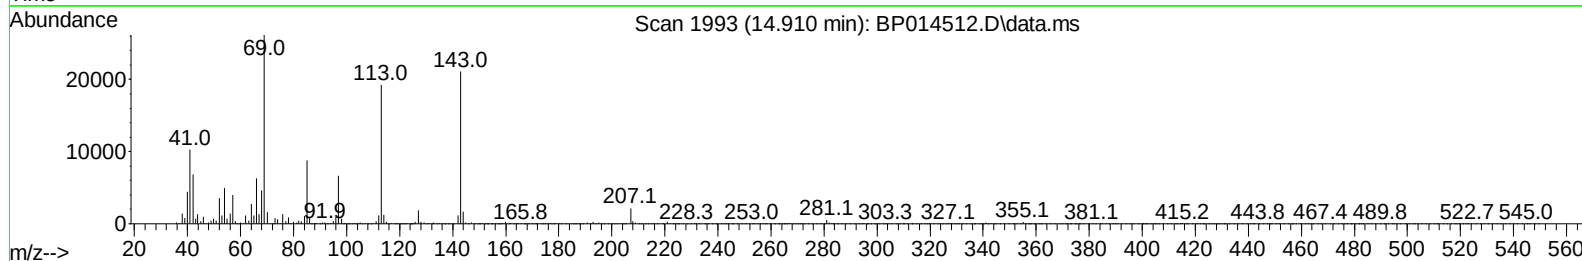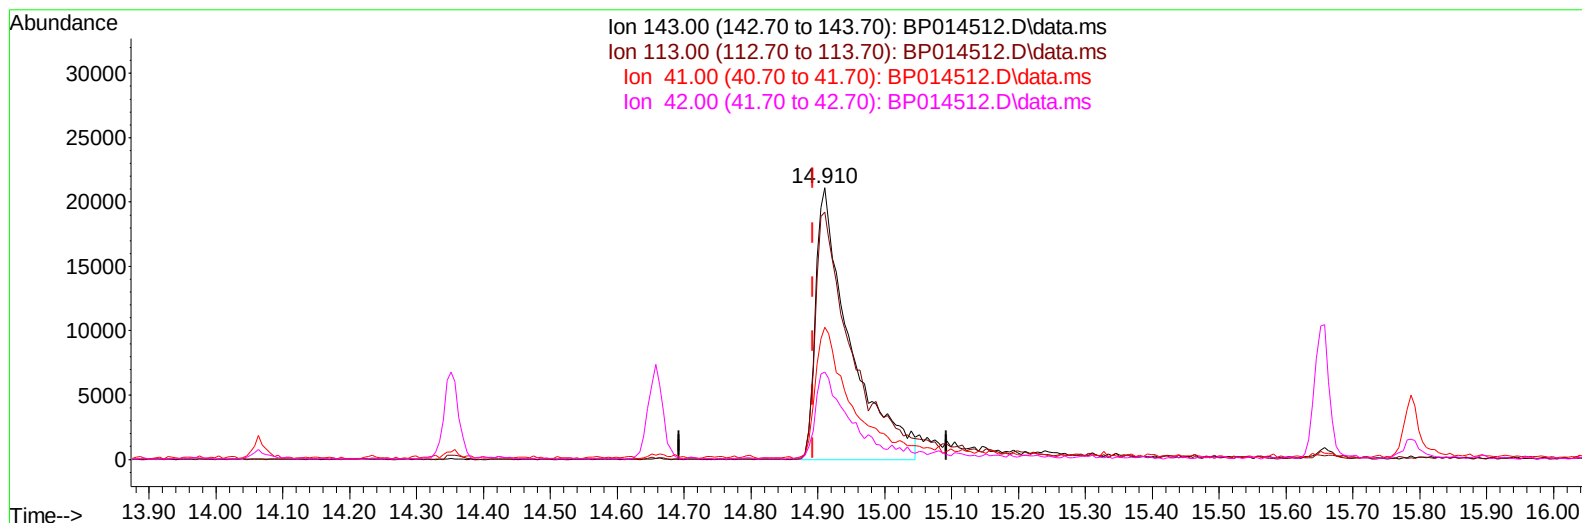

TIC: BP014512.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.018) 20.91 ng/ul m

response 75755

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.13
41.00	44.20	48.63
42.00	31.50	32.28

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014512.D
 Acq On : 04 Apr 2023 05:54
 Operator : CG/JU
 Sample : PB151804BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK804

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 06:18:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	127142	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	499584	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164	295794	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	639649	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	675828	20.000	ng/ul	0.00
88) Perylene-d12	24.021	264	792915	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	18576	5.666	ng/uL	0.00
4) Pyridine-d5	3.817	84	215727	25.676	ng/ul	0.00
7) Phenol-d5	7.175	99	287685	24.535	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	194885	25.904	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	225056	26.556	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	222968	23.574	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	104262	25.852	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	118708	25.705	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	196398	23.352	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	251955	22.743	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	623534	25.998	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	694227	26.087	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	75755m	20.908	ng/ul	0.02
60) Fluorene-d10	15.657	176	528382	26.418	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	85709	18.210	ng/ul	0.00
73) Anthracene-d10	17.522	188	846774	27.354	ng/ul	0.00
81) Pyrene-d10	19.751	212	1046824	23.060	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.857	264	1158461	27.499	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/04/2023
Supervised By :Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 06:18:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

