




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014525.D
 Acq On : 04 Apr 2023 13:28
 Operator : CG/JU
 Sample : 02093-15DL 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

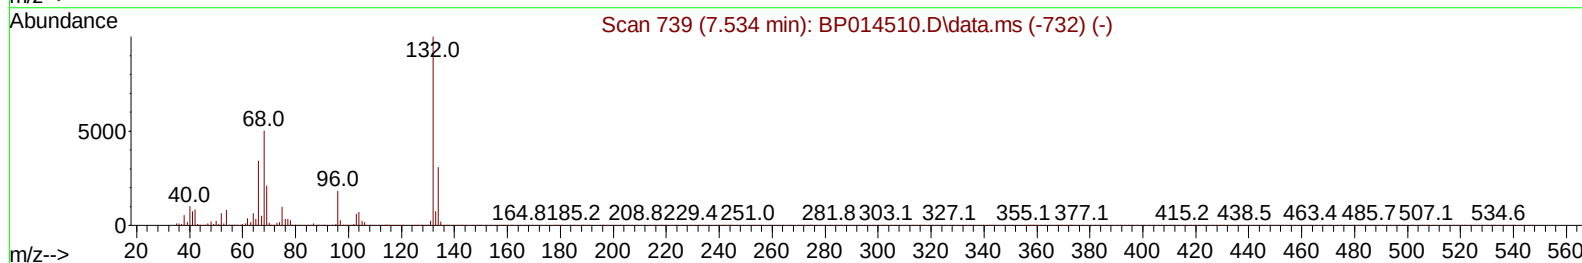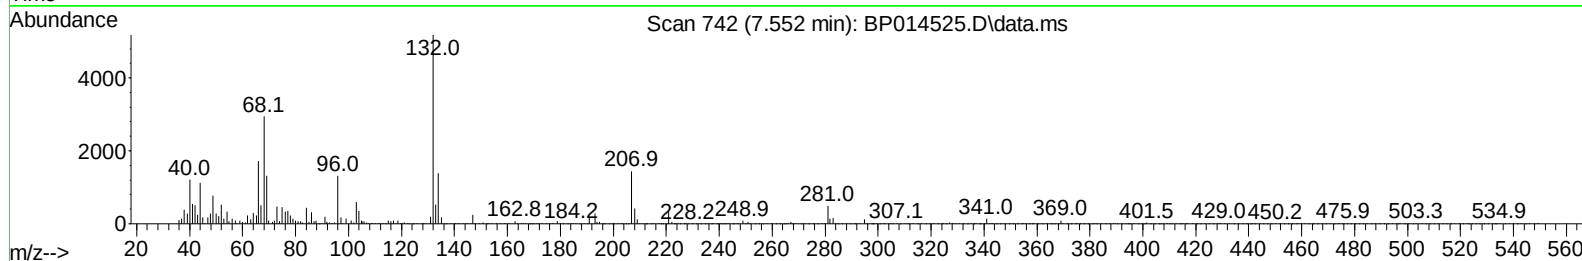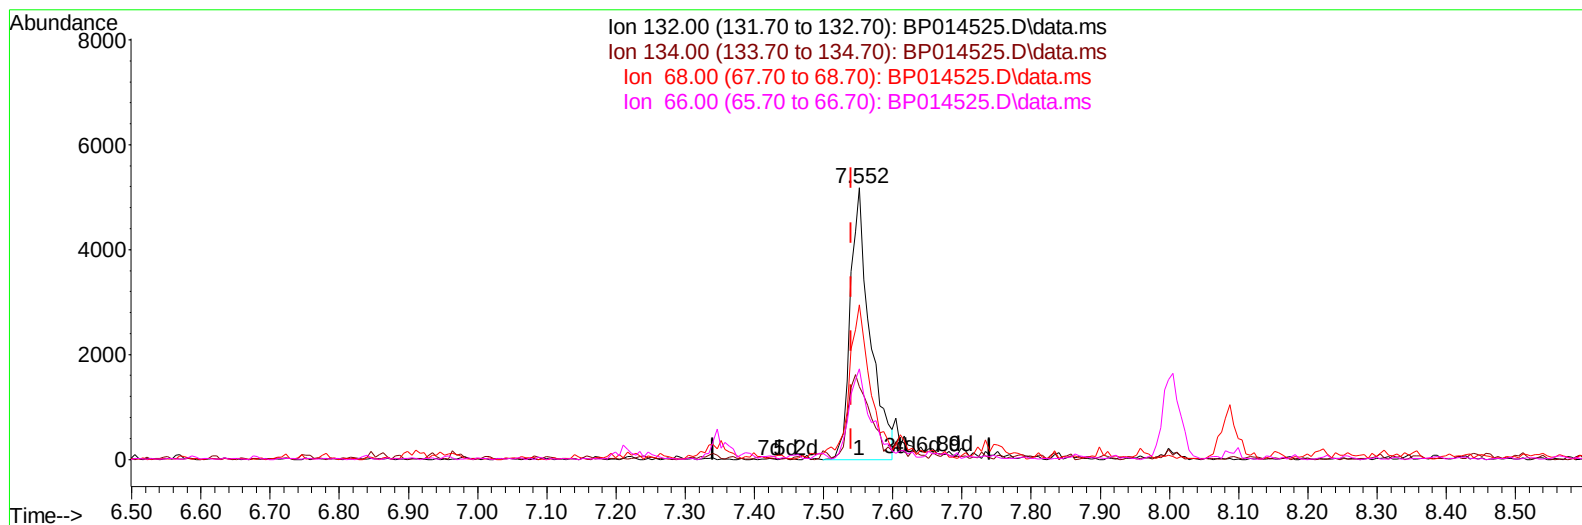

TIC: BP014525.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.552min (+ 0.012) 1.49 ng/u1

response 10126

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.10	26.73
68.00	50.20	56.94
66.00	34.70	33.32




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014525.D
 Acq On : 04 Apr 2023 13:28
 Operator : CG/JU
 Sample : 02093-15DL 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

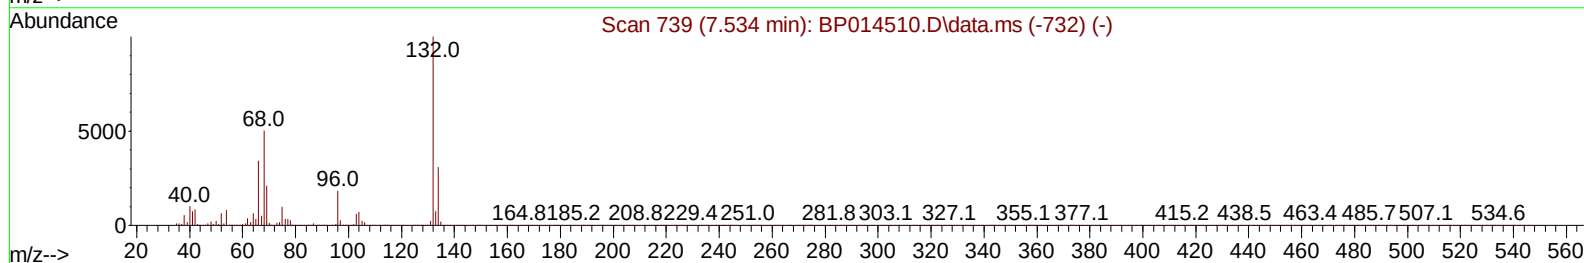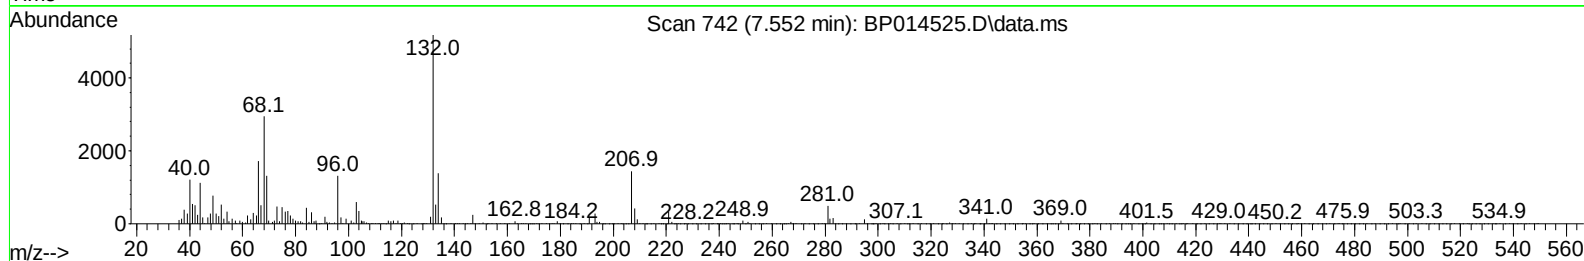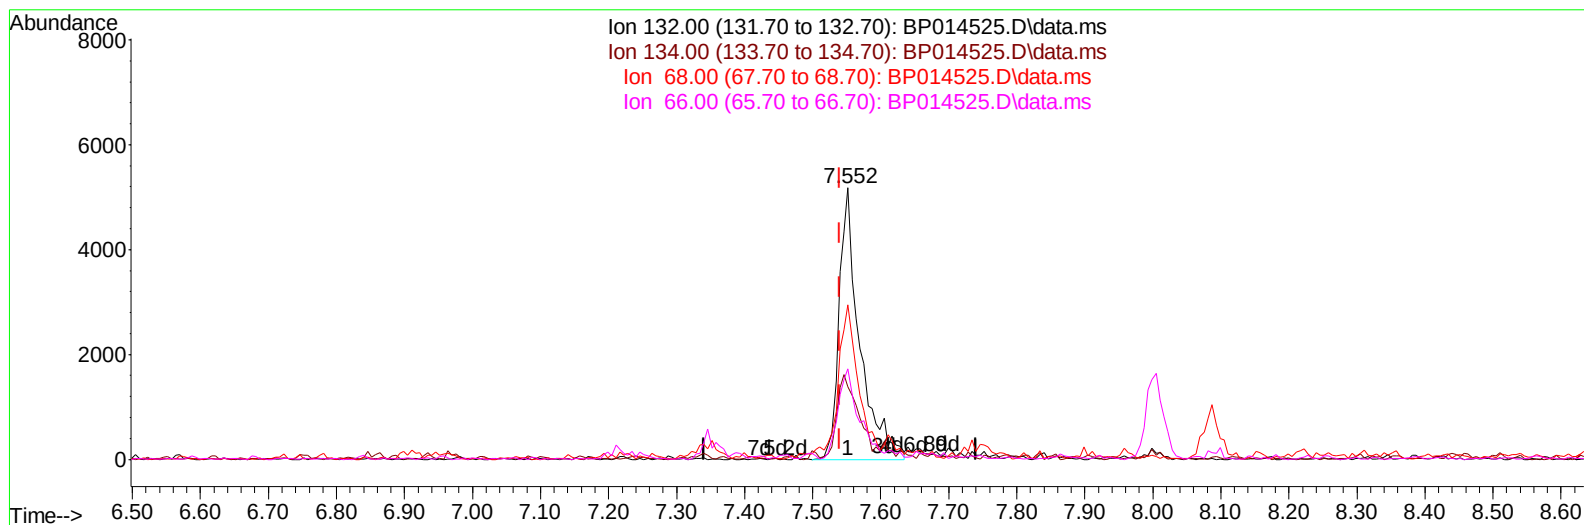

TIC: BP014525.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.552min (+ 0.012) 1.60 ng/ul m

response 10881

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.10	26.73
68.00	50.20	56.94
66.00	34.70	33.32




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014525.D
Acq On : 04 Apr 2023 13:28
Operator : CG/JU
Sample : 02093-15DL 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

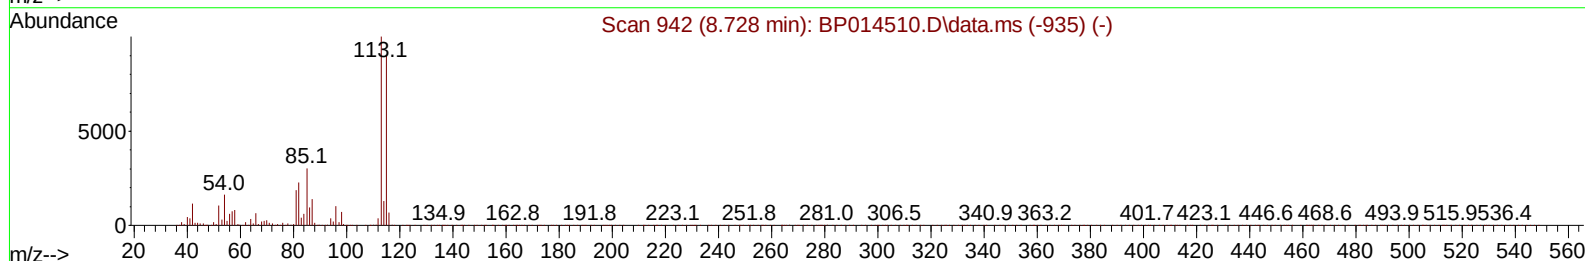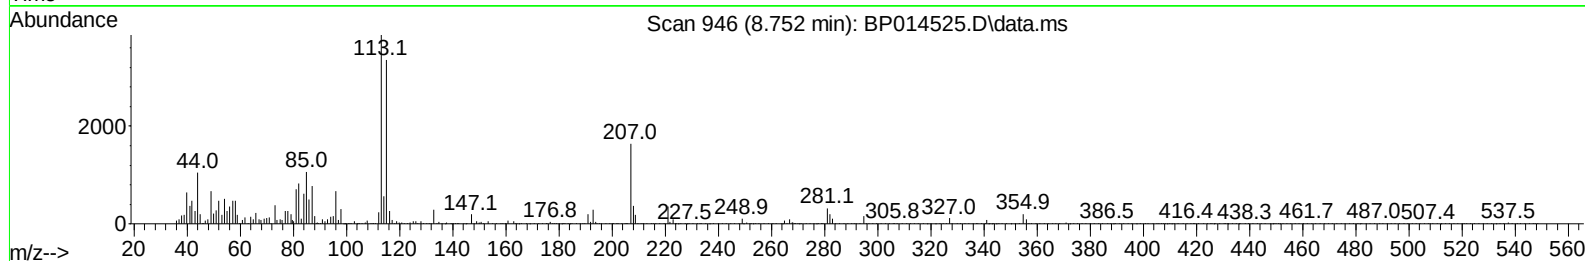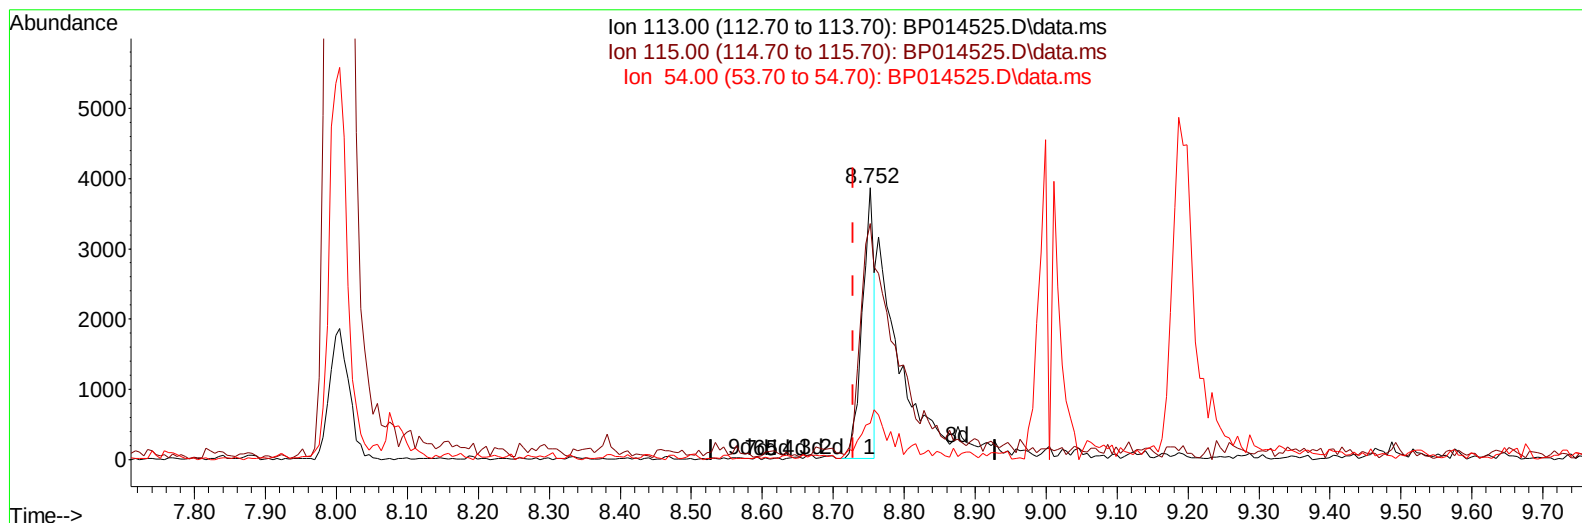

TIC: BP014525.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.752min (+ 0.024) 0.59 ng/uL

response 4474

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	86.94
54.00	15.10	13.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014525.D
 Acq On : 04 Apr 2023 13:28
 Operator : CG/JU
 Sample : 02093-15DL 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

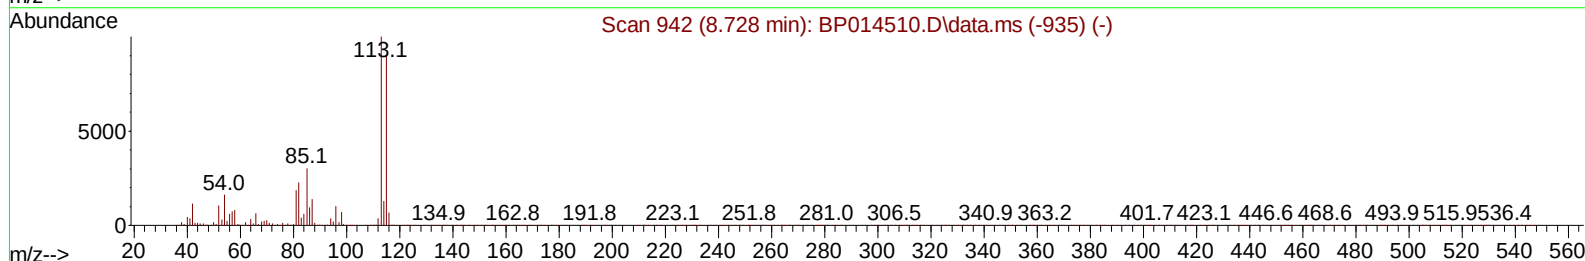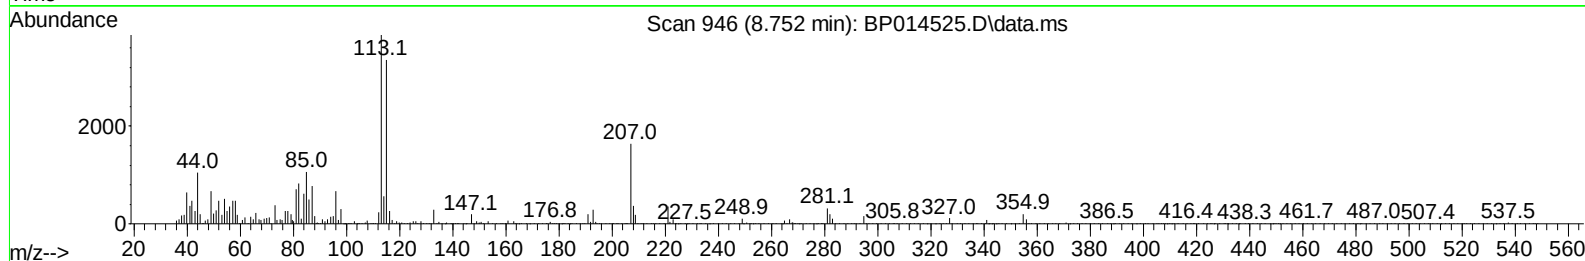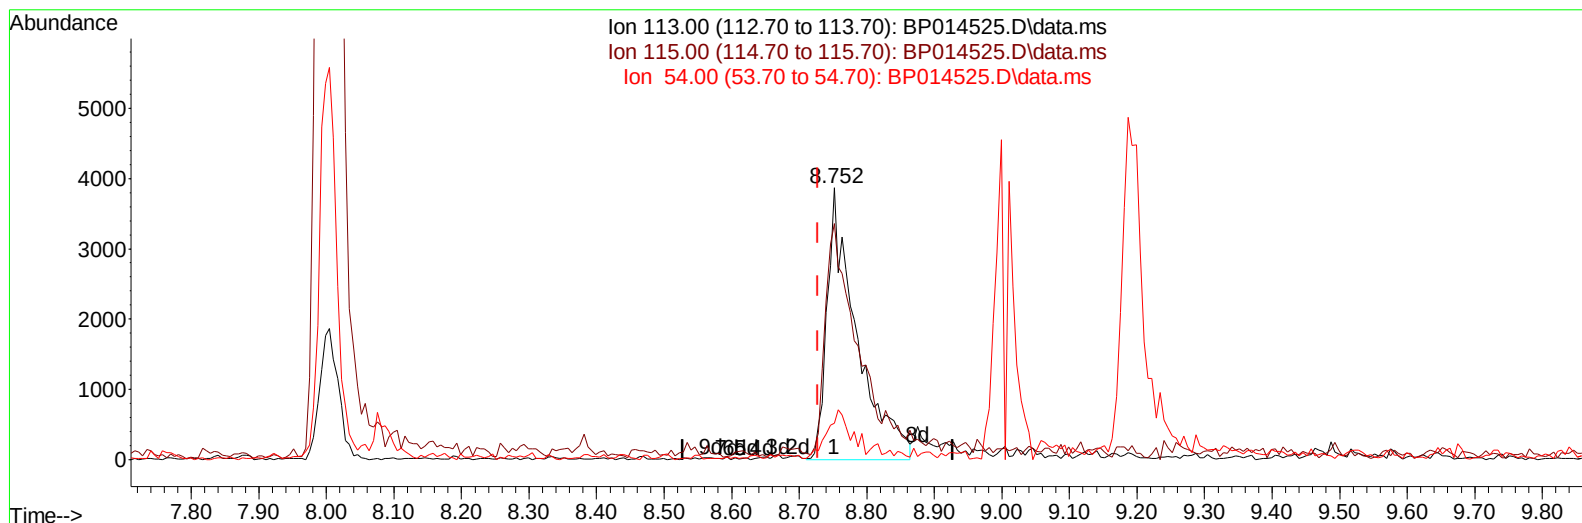

TIC: BP014525.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.752min (+ 0.024) 1.54 ng/ul m

response 11694

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	86.94
54.00	15.10	13.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014525.D
Acq On : 04 Apr 2023 13:28
Operator : CG/JU
Sample : 02093-15DL 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

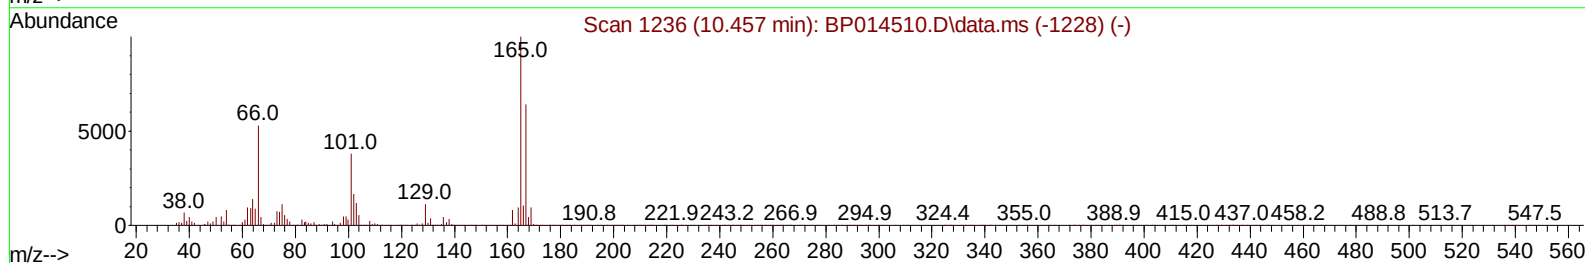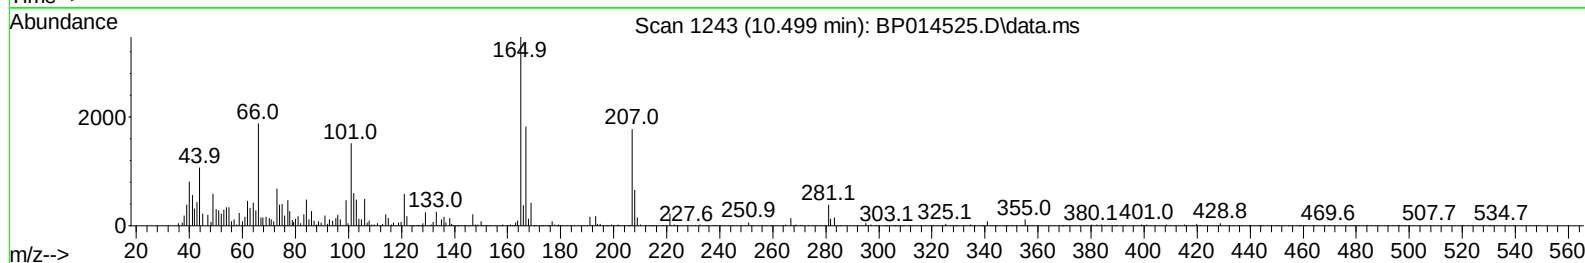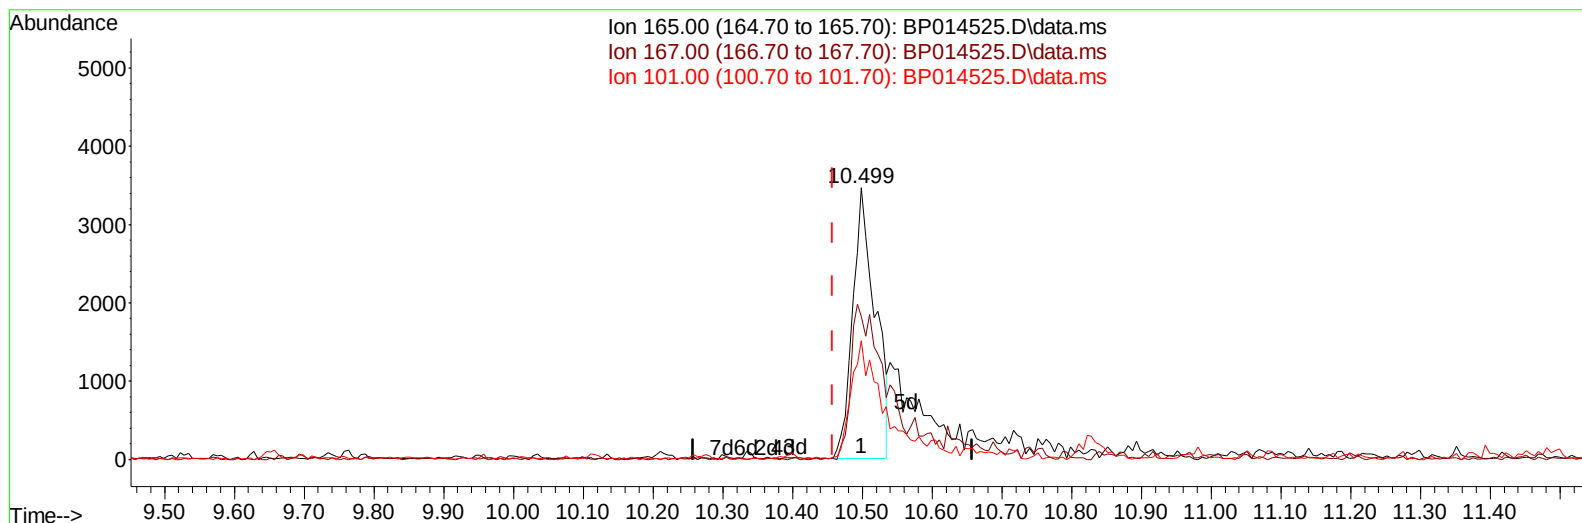

TIC: BP014525.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.499min (+ 0.041) 1.10 ng/ul

response 7725

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	52.68
101.00	39.20	43.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014525.D
 Acq On : 04 Apr 2023 13:28
 Operator : CG/JU
 Sample : 02093-15DL 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

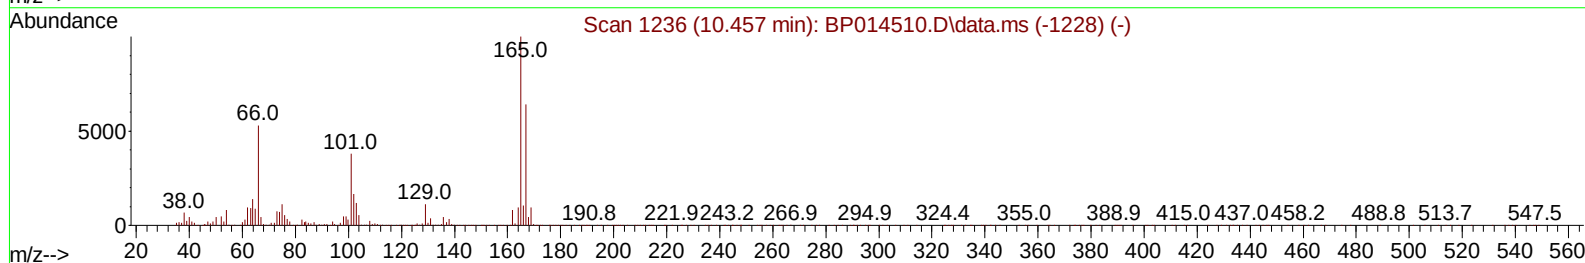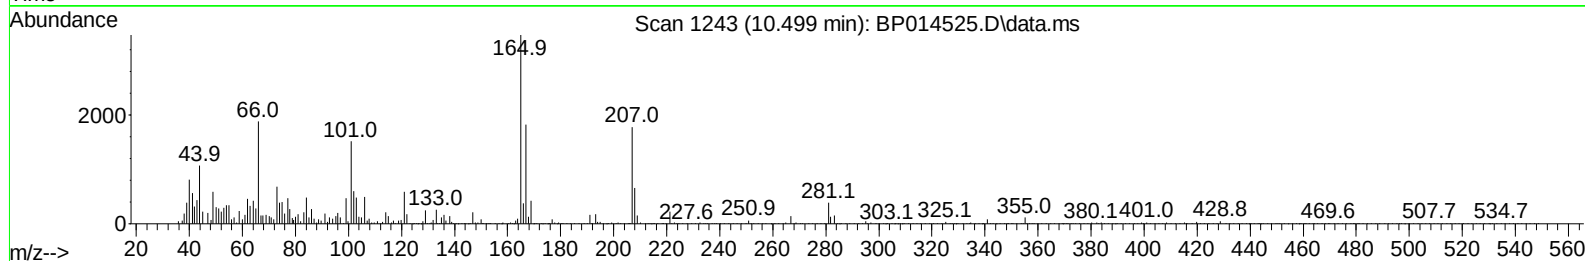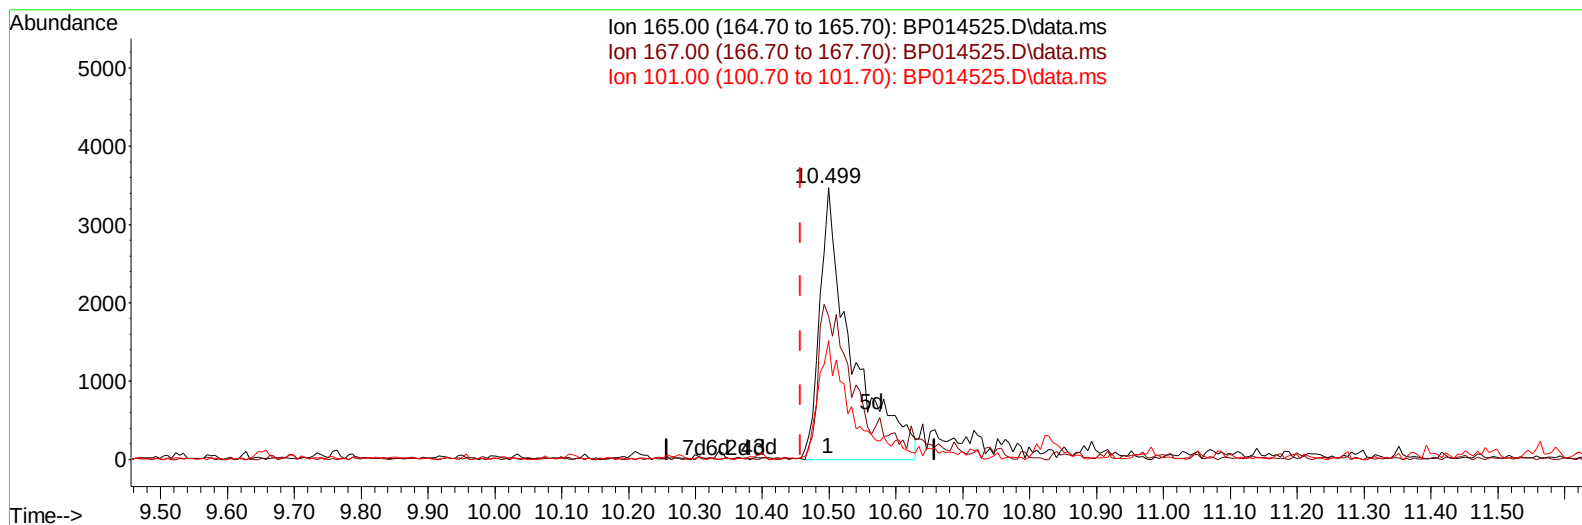

TIC: BP014525.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.499min (+ 0.041) 1.64 ng/ul m

response 11554

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	52.68
101.00	39.20	43.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014525.D
Acq On : 04 Apr 2023 13:28
Operator : CG/JU
Sample : 02093-15DL 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:09:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

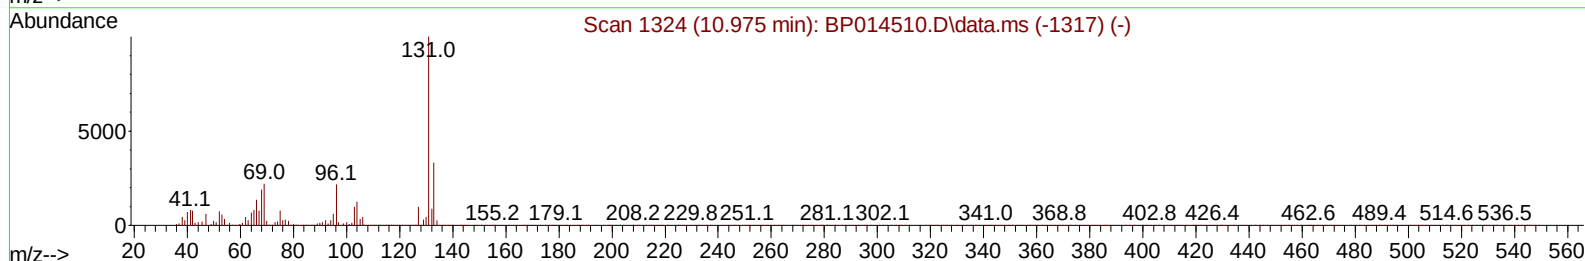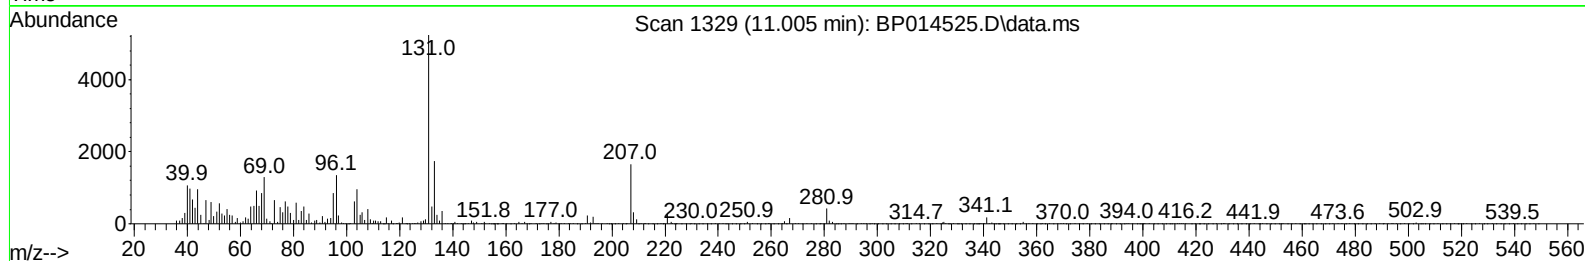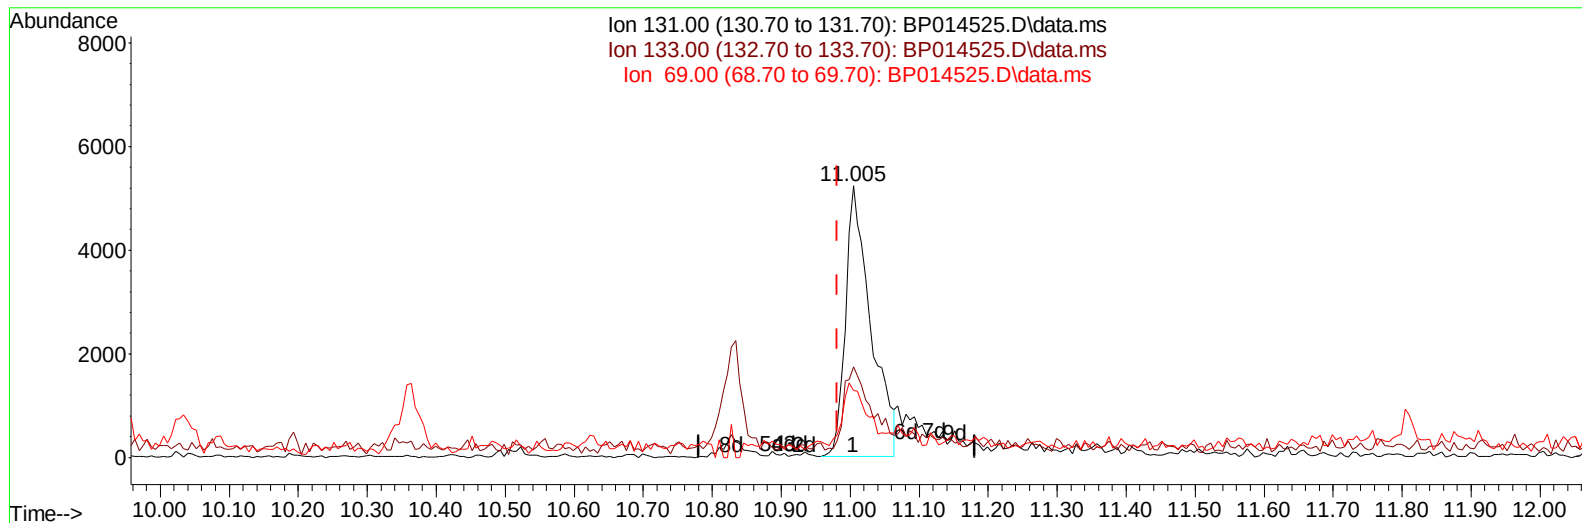

TIC: BP014525.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.005min (+ 0.024) 1.44 ng/u1

response 13313

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	33.34
69.00	21.30	24.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014525.D
Acq On : 04 Apr 2023 13:28
Operator : CG/JU
Sample : 02093-15DL 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:09:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

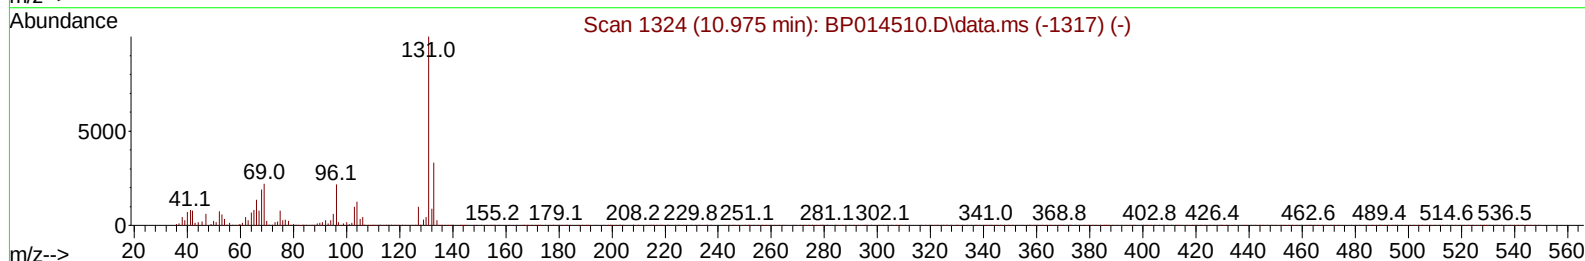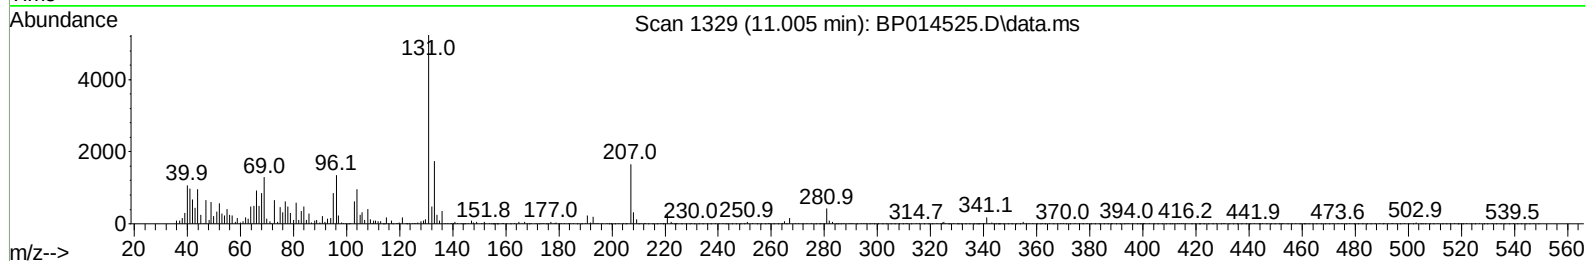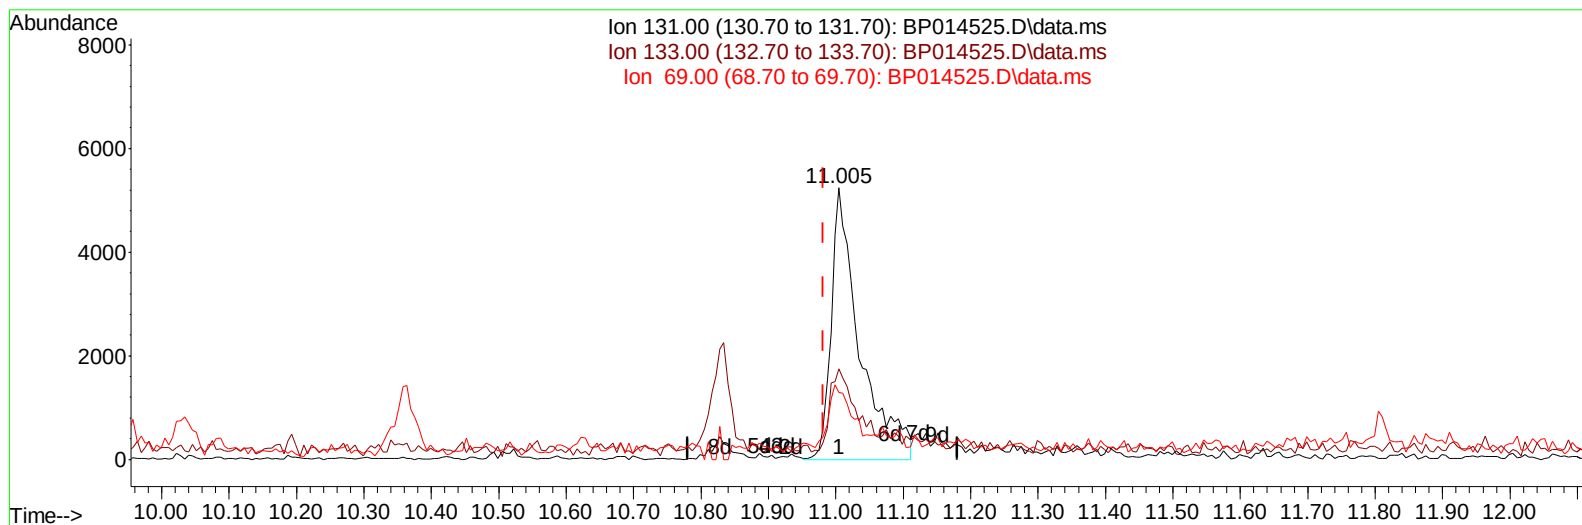

TIC: BP014525.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.005min (+ 0.024) 1.66 ng/ul m

response 15390

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	33.34
69.00	21.30	24.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014525.D
 Acq On : 04 Apr 2023 13:28
 Operator : CG/JU
 Sample : 02093-15DL 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:09:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 01:34:36 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.005	152		102123	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136		418003	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164		253252	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188		565349	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240		611994	20.000	ng/ul	-0.01
88) Perylene-d12	24.022	264		722064	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.381	96		1597	0.606	ng/uL	0.00
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.211	99		5726	0.608	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.334	67		13316	2.204	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132		10881m	1.598	ng/ul	0.01
15) 4-Methylphenol-d8	8.752	113		11694m	1.539	ng/ul	0.02
21) Nitrobenzene-d5	9.193	128		7297	2.162	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143		6379	1.651	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.499	165		11554m	1.642	ng/ul	0.04
31) 4-Chloroaniline-d4	11.005	131		15390m	1.660	ng/ul	0.02
46) Dimethylphthalate-d6	14.069	166		49435	2.407	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160		52098	2.287	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
60) Fluorene-d10	15.657	176		46306	2.704	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200		0d	0.000	ng/ul	
73) Anthracene-d10	17.522	188		70707	2.584	ng/ul	0.00
81) Pyrene-d10	19.751	212		94721	2.304	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.857	264		98257	2.561	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.417	88		58178	20.103	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014525.D
Acq On : 04 Apr 2023 13:28
Operator : CG/JU
Sample : 02093-15DL 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:09:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 01:34:36 2023
Response via : Initial Calibration

