




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:45:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

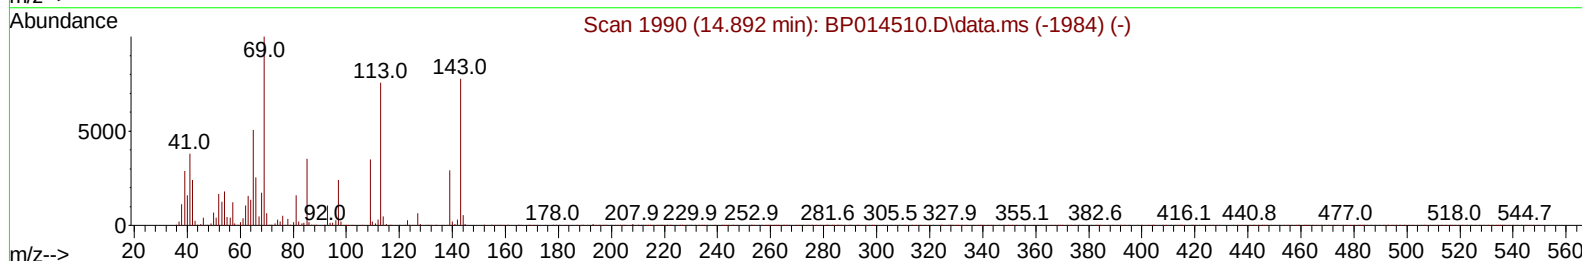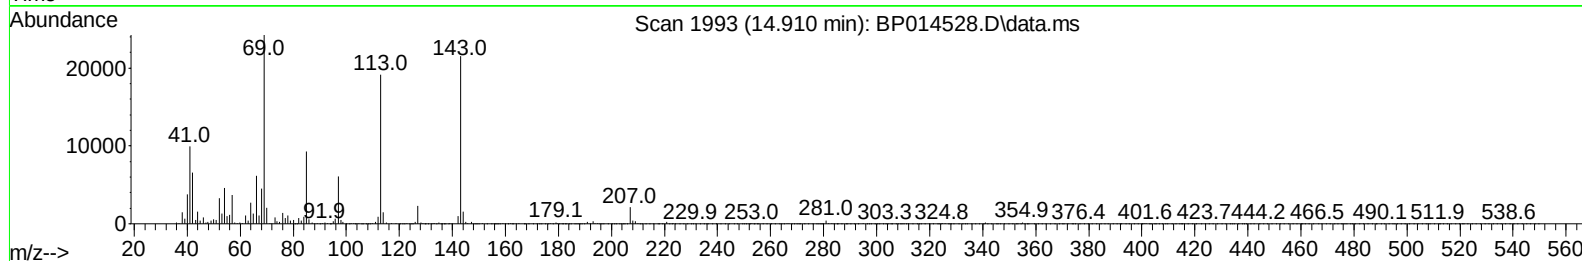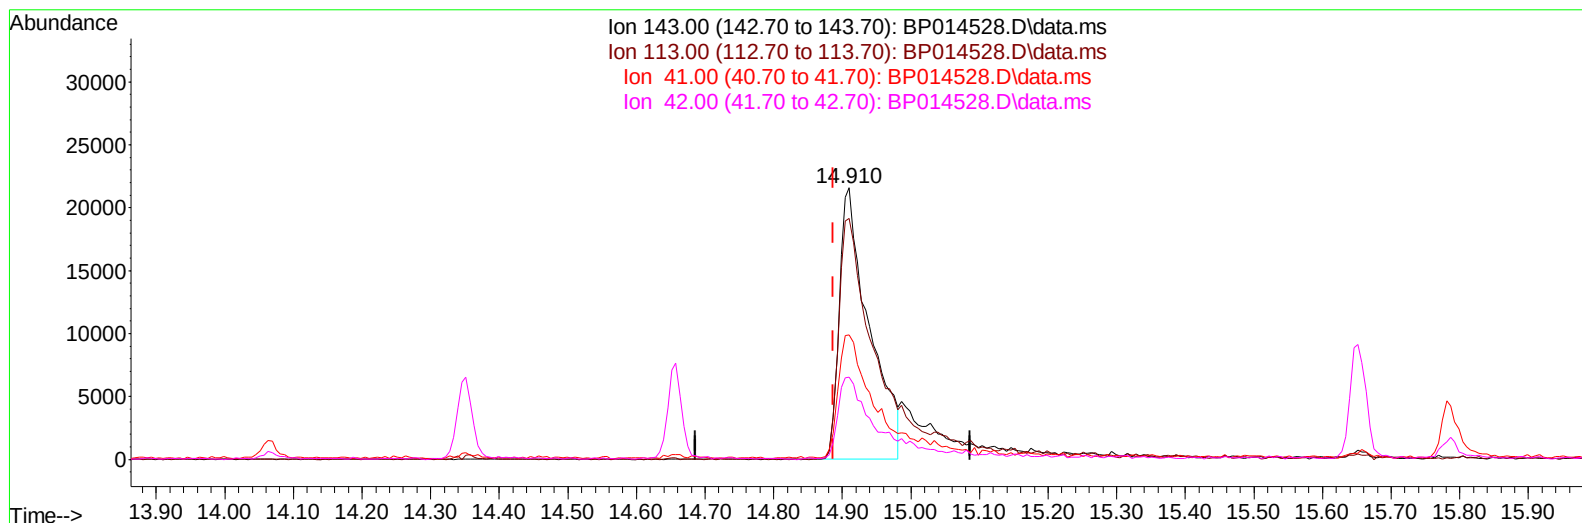

TIC: BP014528.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.024) 19.18 ng/ul

response 65119

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	88.77
41.00	44.20	45.98
42.00	31.50	30.39




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:45:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

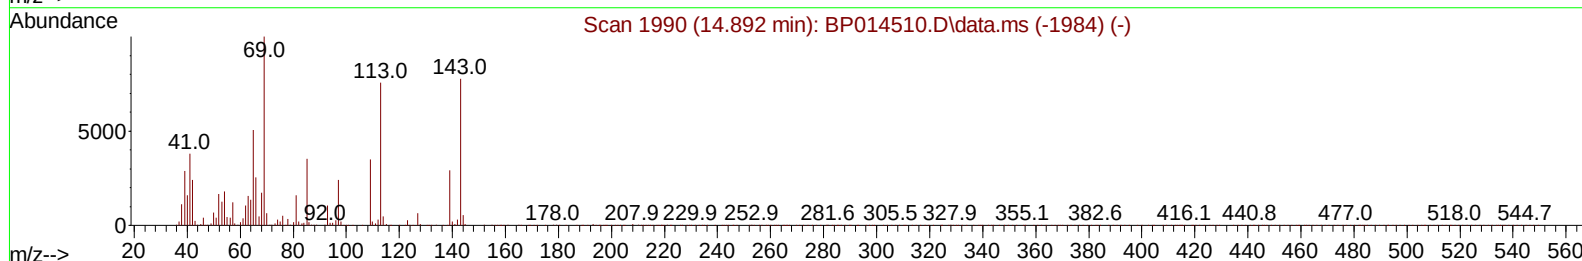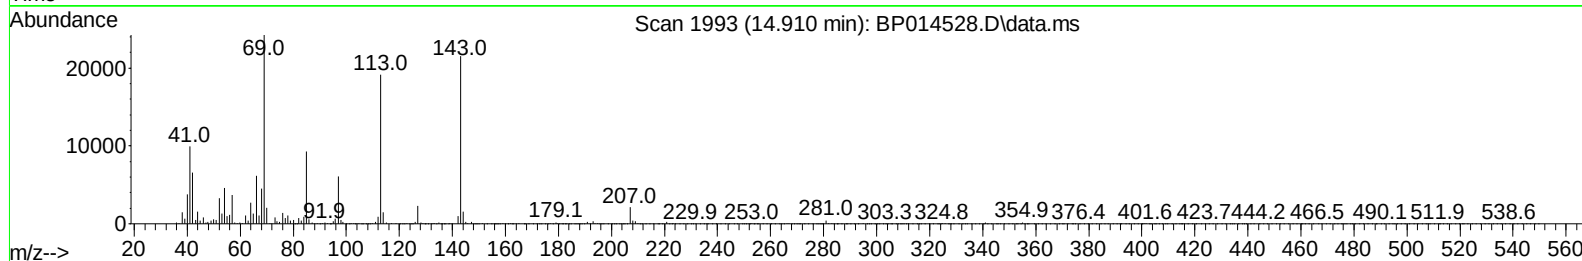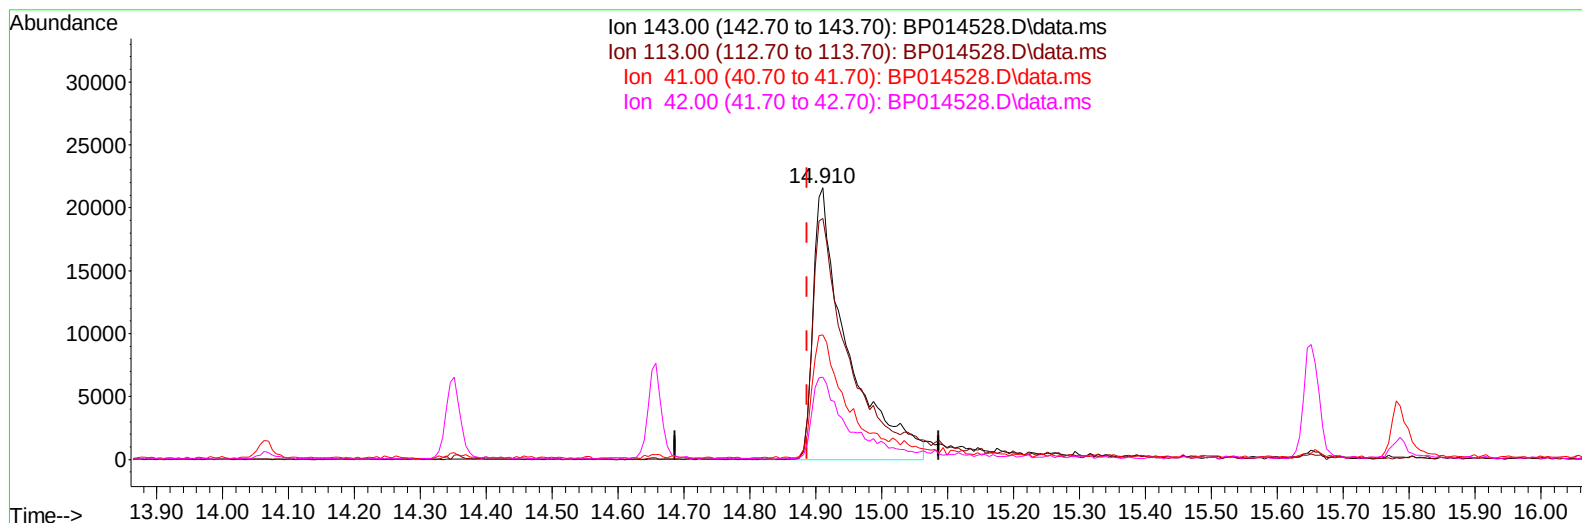

TIC: BP014528.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.024) 23.11 ng/ul m

response 78467

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	88.77
41.00	44.20	45.98
42.00	31.50	30.39

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014528.D
 Acq On : 04 Apr 2023 15:10
 Operator : CG/JU
 Sample : PB151803BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK803

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:45:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	101349	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	428180	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164	277225	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.416	188	650925	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	675912	20.000	ng/ul	0.00
88) Perylene-d12	24.016	264	764656	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	15230	5.827	ng/uL	0.00
4) Pyridine-d5	3.817	84	184470	27.543	ng/ul	0.00
7) Phenol-d5	7.175	99	239543	25.628	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	161696	26.963	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	181969	26.936	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	182930	24.263	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	87062	25.187	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	100015	25.269	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.458	165	161951	22.467	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	178324	18.781	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	590384	26.265	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	638733	25.609	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	78467m	23.107	ng/ul	0.02
60) Fluorene-d10	15.651	176	506362	27.013	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	81034	16.919	ng/ul	0.00
73) Anthracene-d10	17.516	188	849266	26.959	ng/ul	0.00
81) Pyrene-d10	19.745	212	1057884	23.301	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.851	264	1108599	27.288	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:45:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

