




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014531.D
Acq On : 04 Apr 2023 16:53
Operator : CG/JU
Sample : 02123-02
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A2

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:46:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

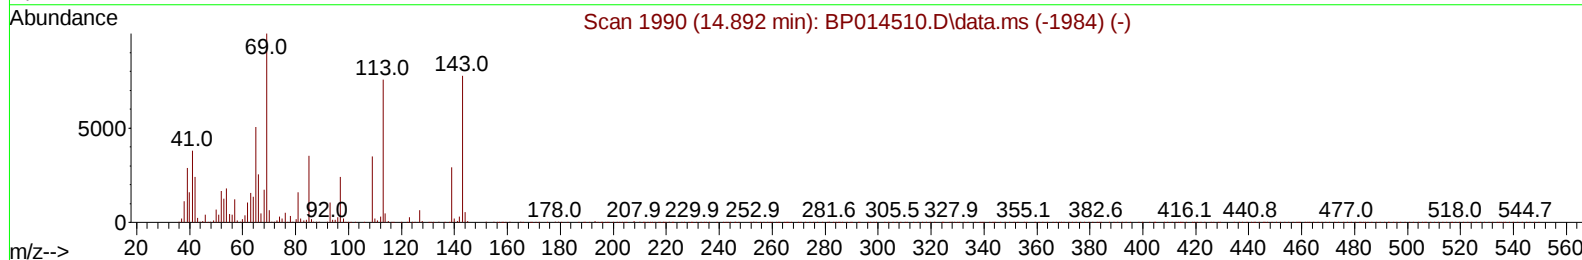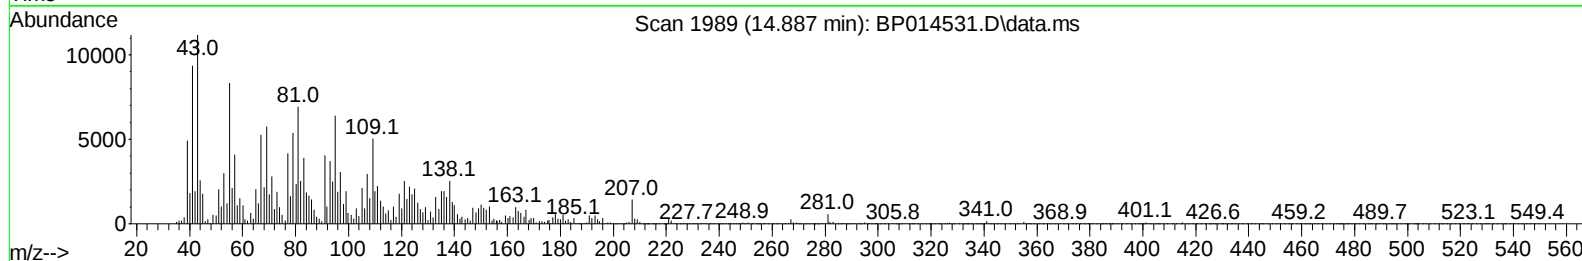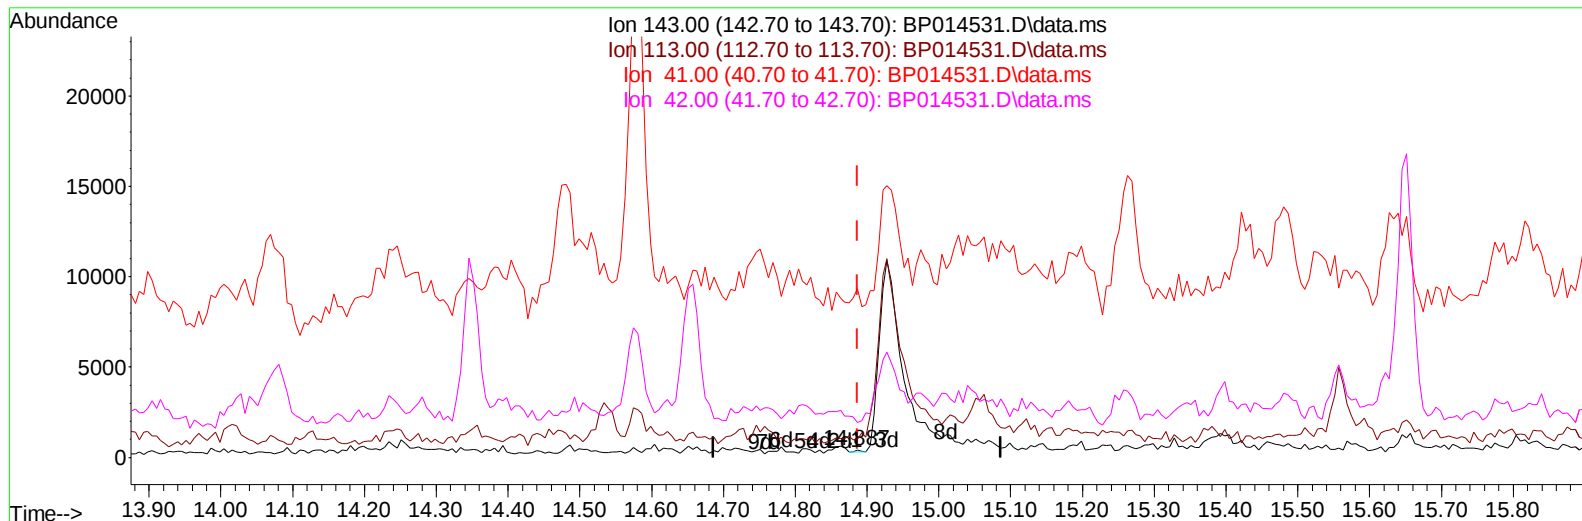

TIC: BP014531.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.887min (-0.000) 0.02 ng/u1

response 76

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	243.84#
41.00	44.20	2215.17#
42.00	31.50	454.27#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014531.D
Acq On : 04 Apr 2023 16:53
Operator : CG/JU
Sample : 02123-02
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A2

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:46:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

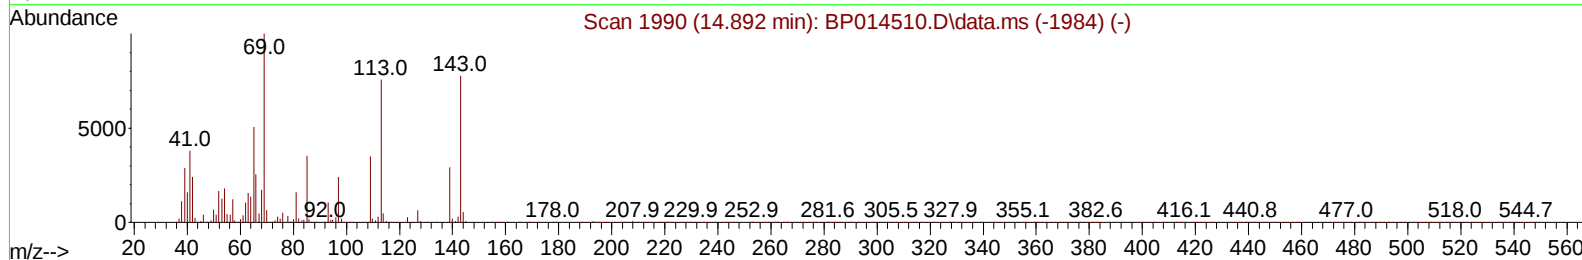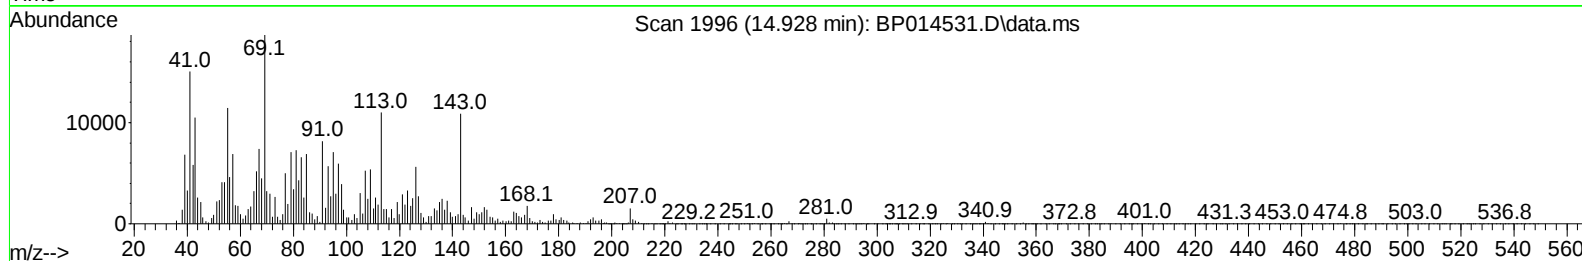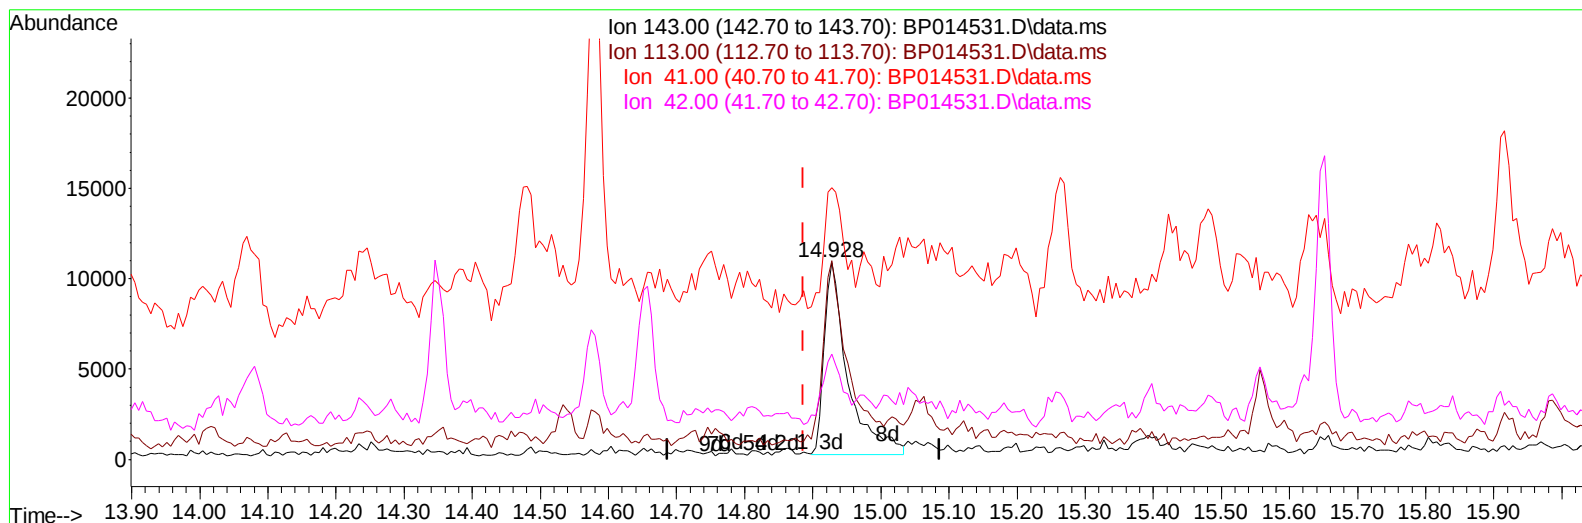

TIC: BP014531.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.928min (+ 0.041) 6.56 ng/ul m

response 25653

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	100.90
41.00	44.20	137.83#
42.00	31.50	53.43#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014531.D
 Acq On : 04 Apr 2023 16:53
 Operator : CG/JU
 Sample : 02123-02
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:46:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	116472	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	484526	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164	319192	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	742904	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	759110	20.000	ng/ul	0.00
88) Perylene-d12	24.021	264	871551	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	14407	4.797	ng/uL	0.00
4) Pyridine-d5	3.822	84	129761	16.859	ng/ul	0.01
7) Phenol-d5	7.181	99	126651	11.791	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.328	67	166846	24.209	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	172766	22.253	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	211747	24.438	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	98530	25.190	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	103917	23.201	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	219725	26.937	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	278180	25.891	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	808843	31.253	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	851643	29.656	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	25653m	6.561	ng/ul	0.04
60) Fluorene-d10	15.651	176	675087	31.279	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	54877	10.039	ng/ul	0.00
73) Anthracene-d10	17.516	188	1116541	31.055	ng/ul	0.00
81) Pyrene-d10	19.745	212	1390701	27.274	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.857	264	1428779	30.856	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.417	88	738743	223.820	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014531.D
Acq On : 04 Apr 2023 16:53
Operator : CG/JU
Sample : 02123-02
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A2

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:46:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

