




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014532.D
Acq On : 04 Apr 2023 17:27
Operator : CG/JU
Sample : 02123-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A4

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:46:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

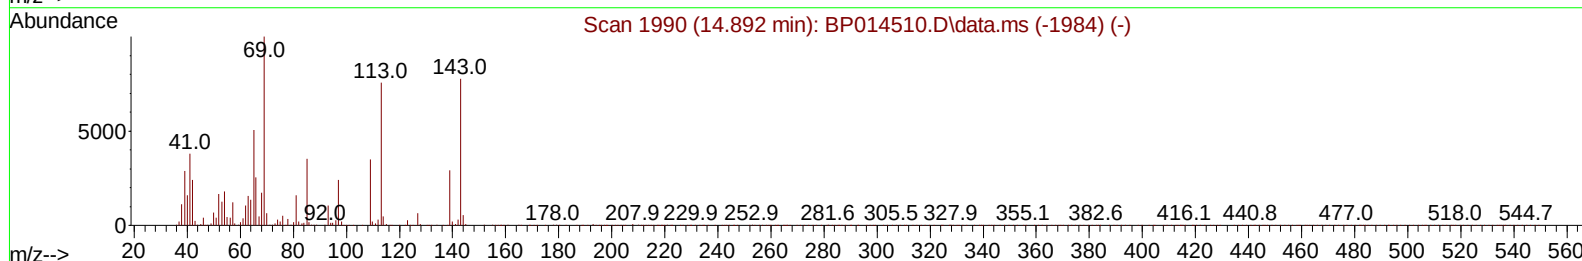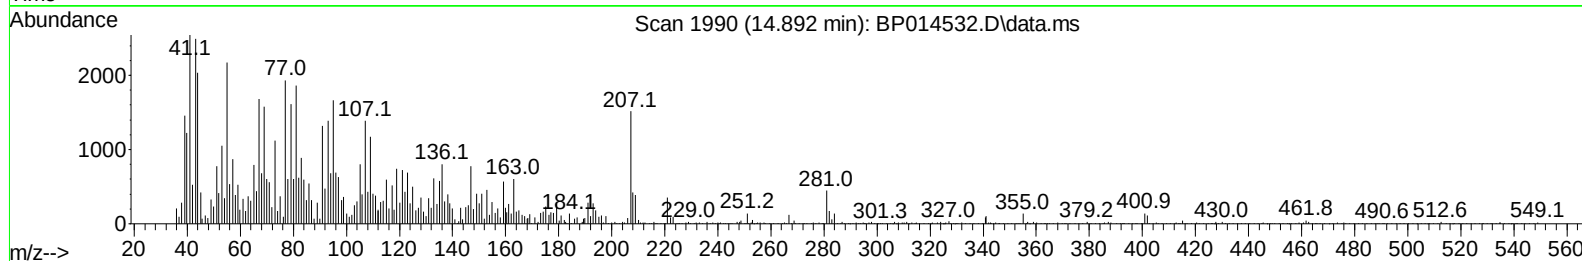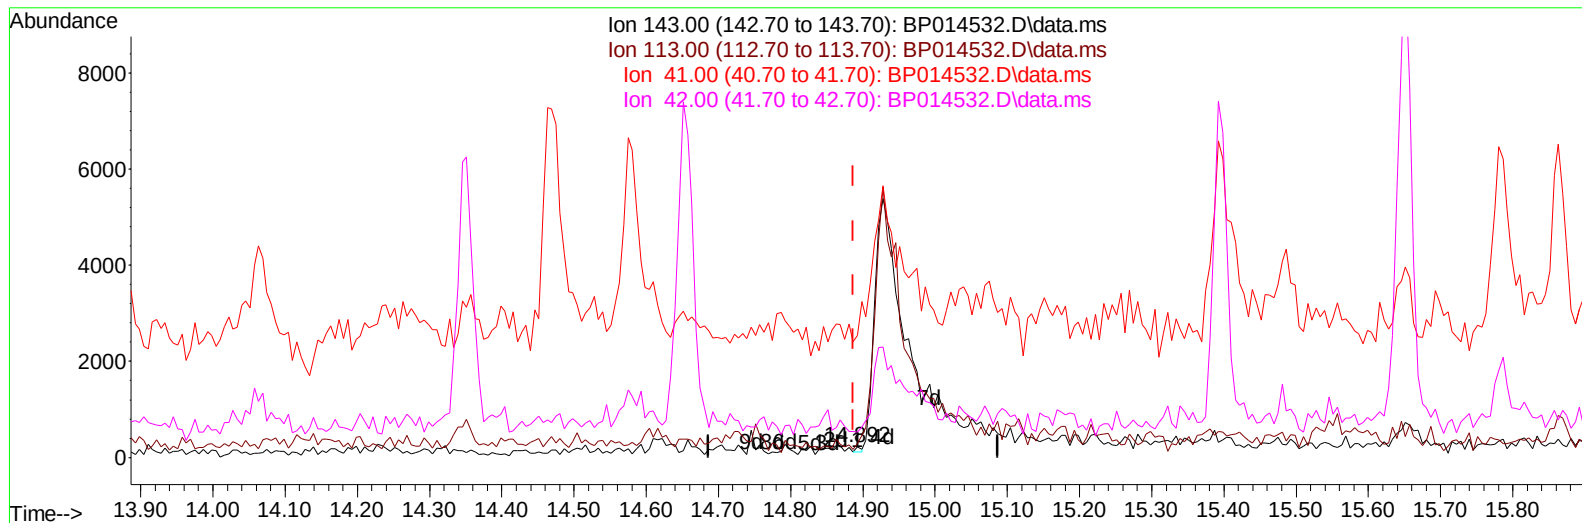

TIC: BP014532.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.892min (+ 0.006) 0.02 ng/ul

response 57

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	135.19#
41.00	44.20	1177.31#
42.00	31.50	241.67#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014532.D
Acq On : 04 Apr 2023 17:27
Operator : CG/JU
Sample : 02123-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A4

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:46:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

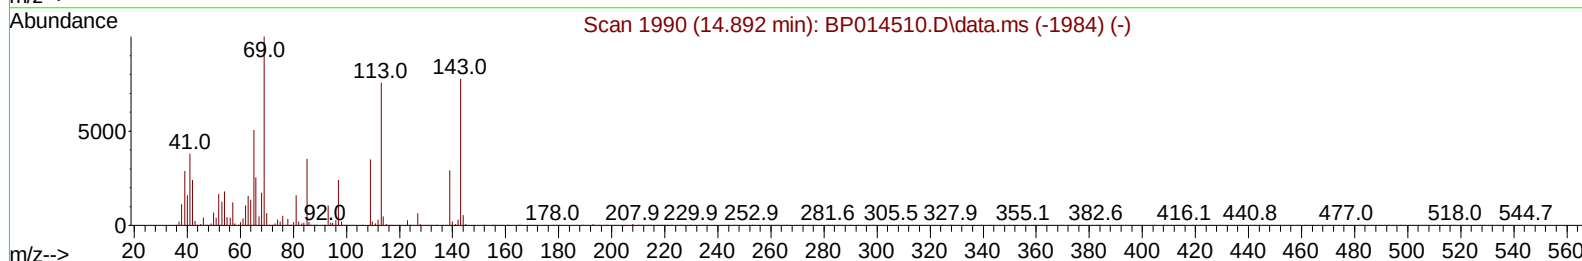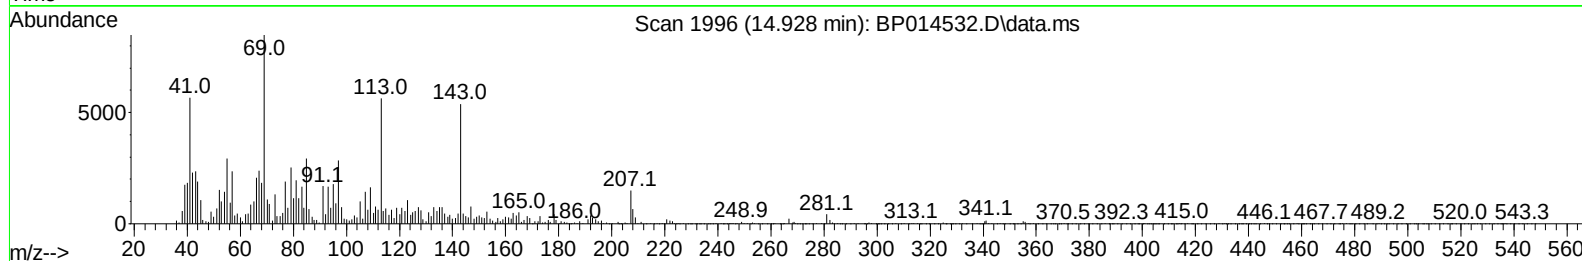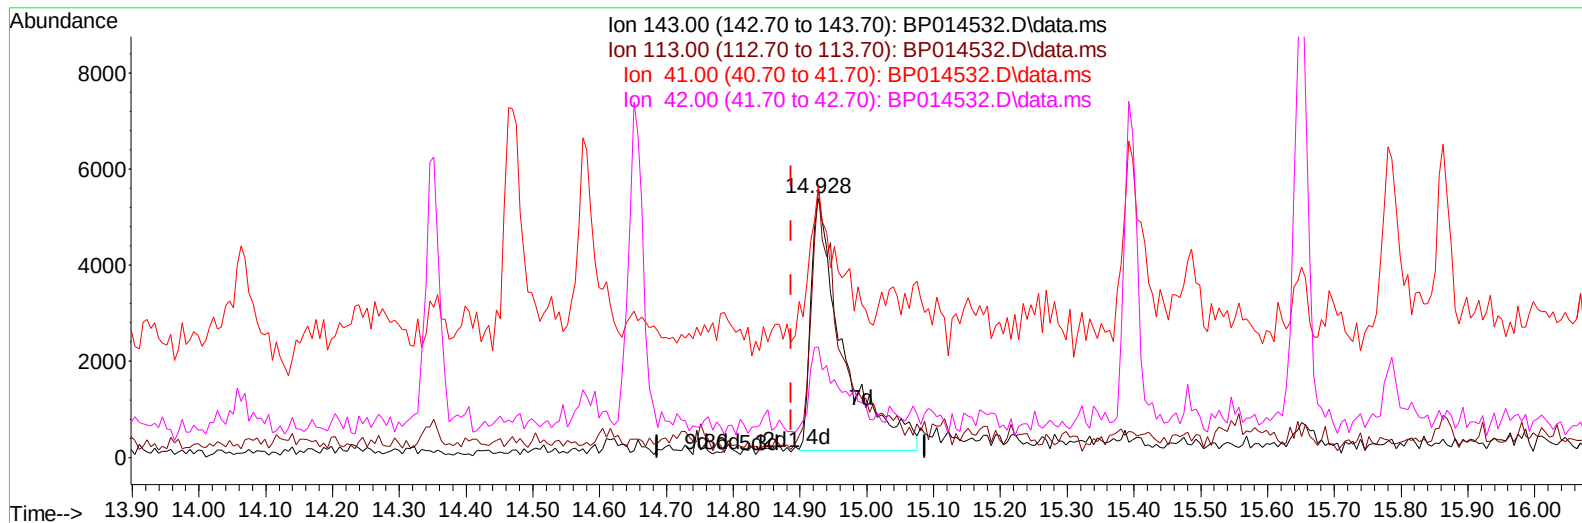

TIC: BP014532.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.928min (+ 0.041) 5.31 ng/ul m

response 17785

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	104.53
41.00	44.20	104.84#
42.00	31.50	42.61#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014532.D
 Acq On : 04 Apr 2023 17:27
 Operator : CG/JU
 Sample : 02123-03
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:46:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	110538	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	448442	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.657	164	273596	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.416	188	623500	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	677842	20.000	ng/ul	0.00
88) Perylene-d12	24.015	264	781919	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	11426	4.009	ng/uL	0.00
4) Pyridine-d5	3.822	84	94702	12.965	ng/ul	0.01
7) Phenol-d5	7.181	99	50747	4.978	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.328	67	151521	23.166	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	126846	17.215	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	93035	11.314	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	82977	22.921	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	82495	19.900	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	146448	19.398	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	183508	18.454	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	578205	26.064	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	587193	23.855	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	17785m	5.307	ng/ul	0.04
60) Fluorene-d10	15.651	176	458919	24.807	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	66906	14.583	ng/ul	0.00
73) Anthracene-d10	17.516	188	778686	25.806	ng/ul	0.00
81) Pyrene-d10	19.745	212	998289	21.926	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.851	264	1089483	26.225	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.417	88	36191	11.554	ng/uL	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014532.D
Acq On : 04 Apr 2023 17:27
Operator : CG/JU
Sample : 02123-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:46:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

