




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014537.D
Acq On : 04 Apr 2023 20:18
Operator : CG/JU
Sample : 02122-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A0

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:47:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

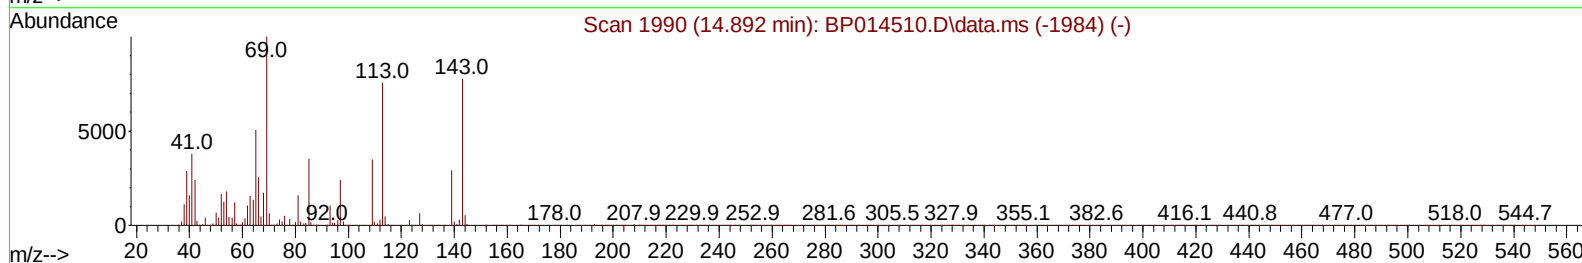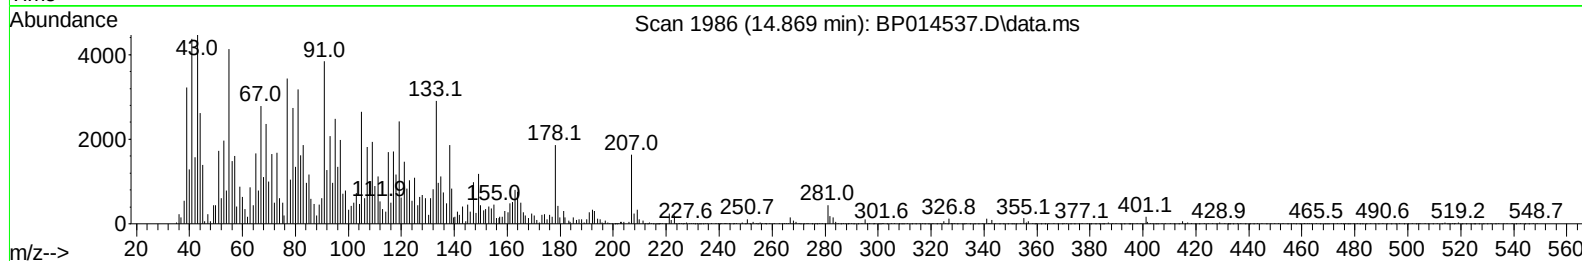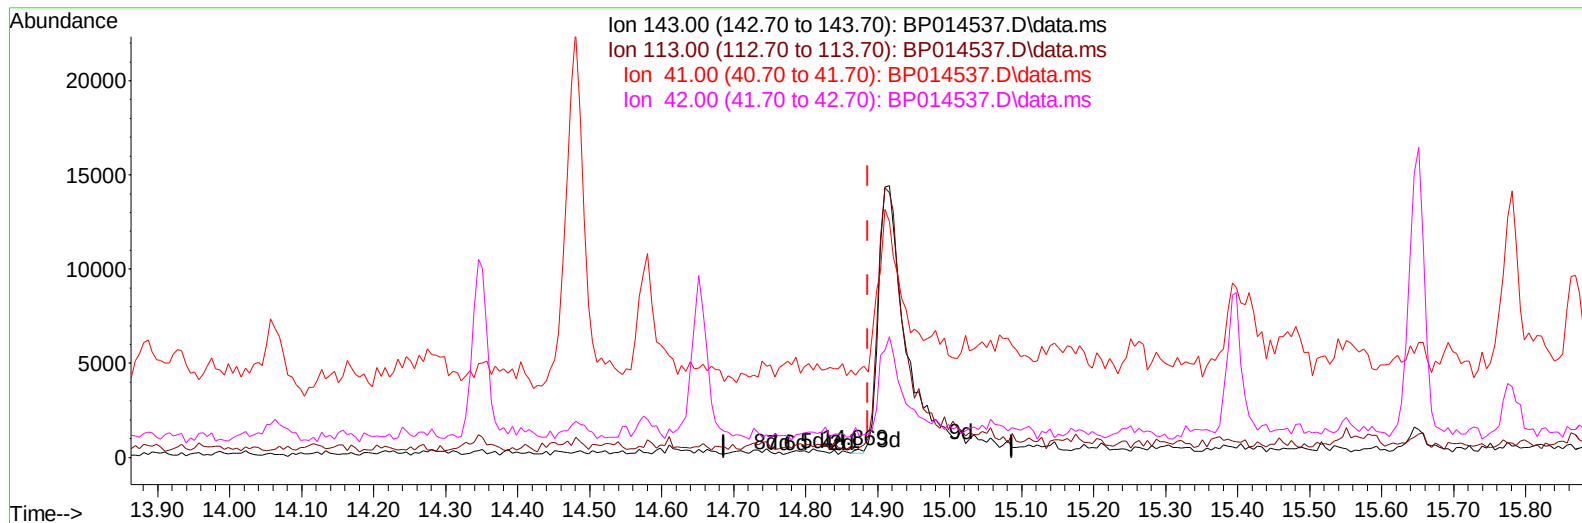

TIC: BP014537.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (-0.018) 0.04 ng/u1

response 154

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	83.54
41.00	44.20	1059.56#
42.00	31.50	380.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014537.D
Acq On : 04 Apr 2023 20:18
Operator : CG/JU
Sample : 02122-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A0

Manual IntegrationsAPPROVED

Quant Time: Apr 04 23:47:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

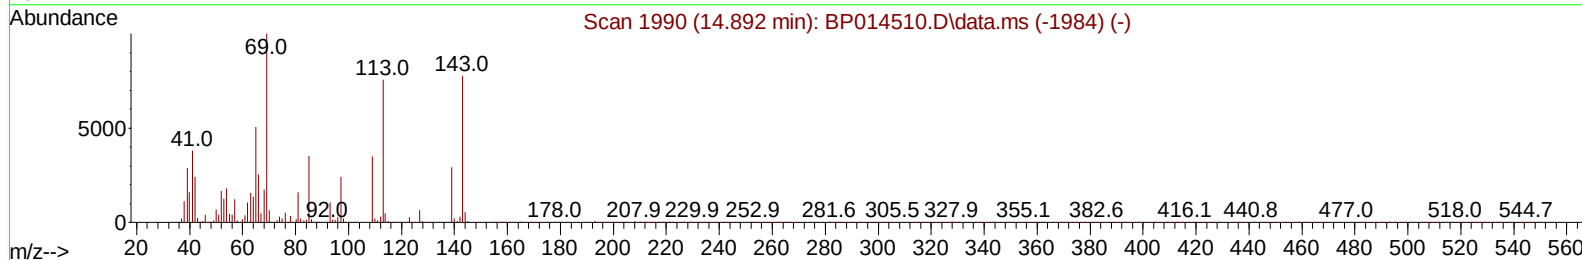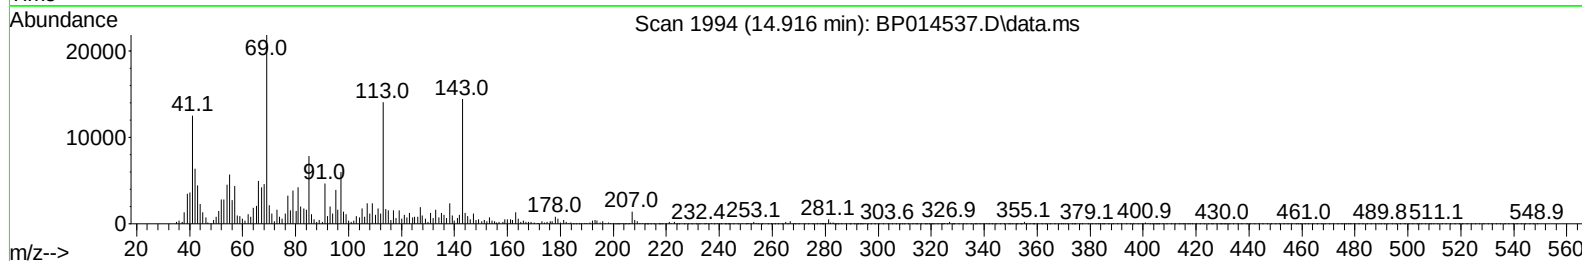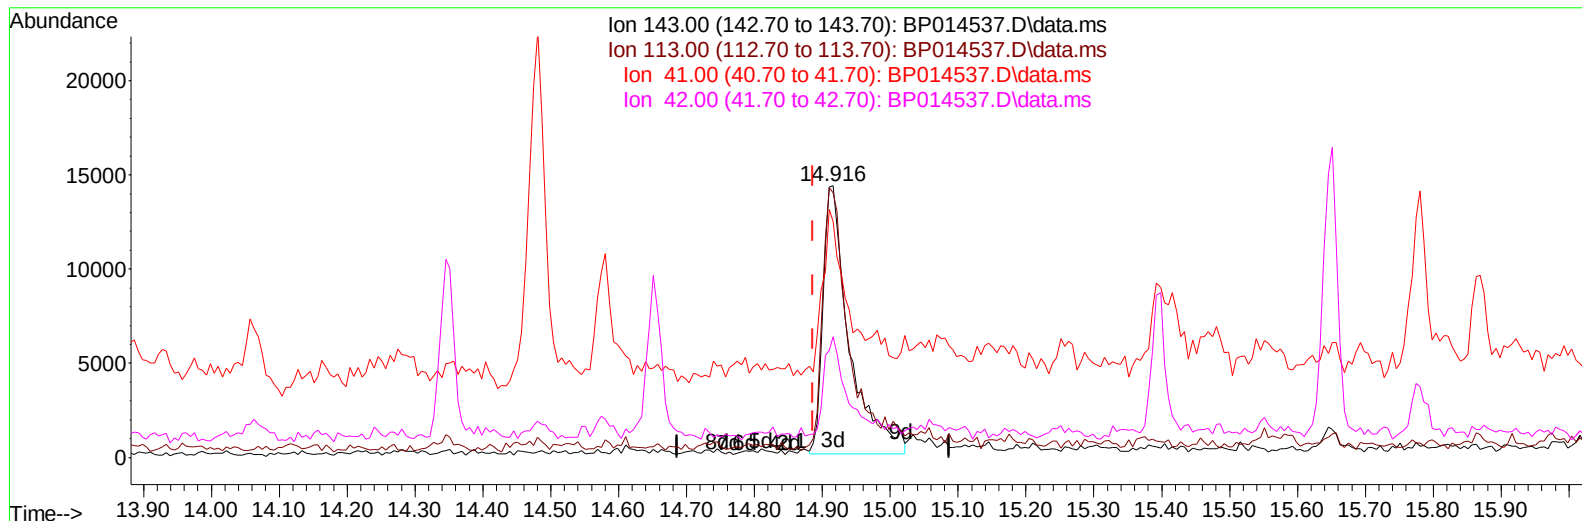

TIC: BP014537.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.029) 10.05 ng/ul m

response 38413

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	97.51
41.00	44.20	86.85#
42.00	31.50	44.35#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014537.D
 Acq On : 04 Apr 2023 20:18
 Operator : CG/JU
 Sample : 02122-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:47:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	113721	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	472891	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	312181	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.416	188	722902	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	736065	20.000	ng/ul	0.00
88) Perylene-d12	24.015	264	842107	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	14449	4.927	ng/uL	0.00
4) Pyridine-d5	3.822	84	104861	13.954	ng/ul	0.01
7) Phenol-d5	7.175	99	104399	9.954	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	201689	29.973	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	201631	26.599	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	181018	21.397	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	116920	30.627	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	130299	29.807	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	243971	30.645	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	203841	19.439	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	887356	35.056	ng/ul	0.00
49) Acenaphthylene-d8	14.351	160	977497	34.803	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	38413m	10.045	ng/ul	0.03
60) Fluorene-d10	15.651	176	748623	35.465	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.781	200	135159	25.410	ng/ul	0.00
73) Anthracene-d10	17.516	188	1248930	35.699	ng/ul	0.00
81) Pyrene-d10	19.745	212	1554162	31.434	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.857	264	1600972	35.783	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.417	88	52759	16.371	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014537.D
Acq On : 04 Apr 2023 20:18
Operator : CG/JU
Sample : 02122-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 04 23:47:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

