




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014543.D
 Acq On : 04 Apr 2023 23:42
 Operator : CG/JU
 Sample : 02158-18RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

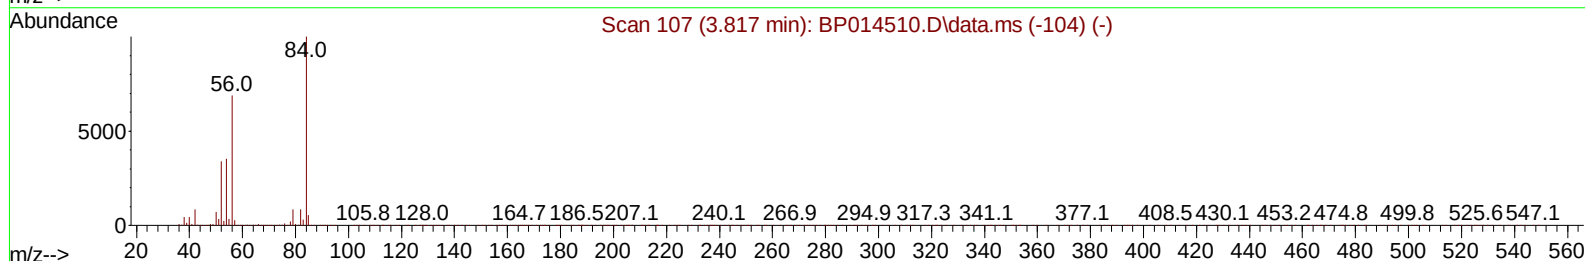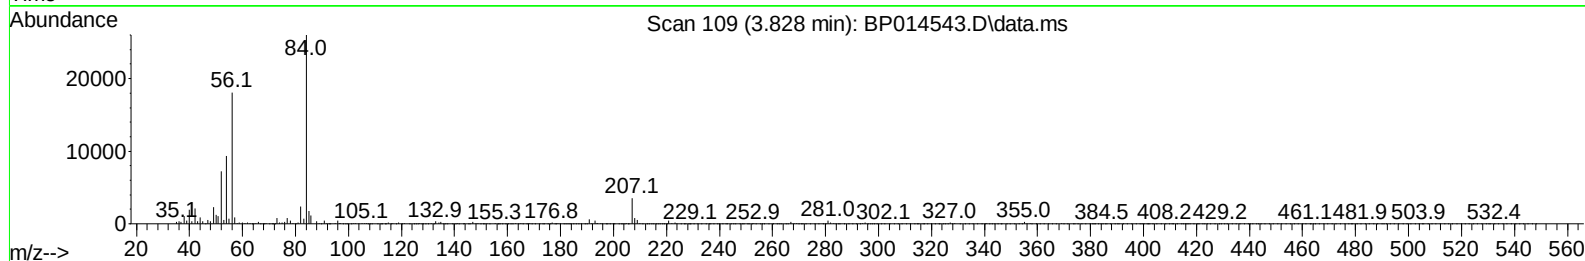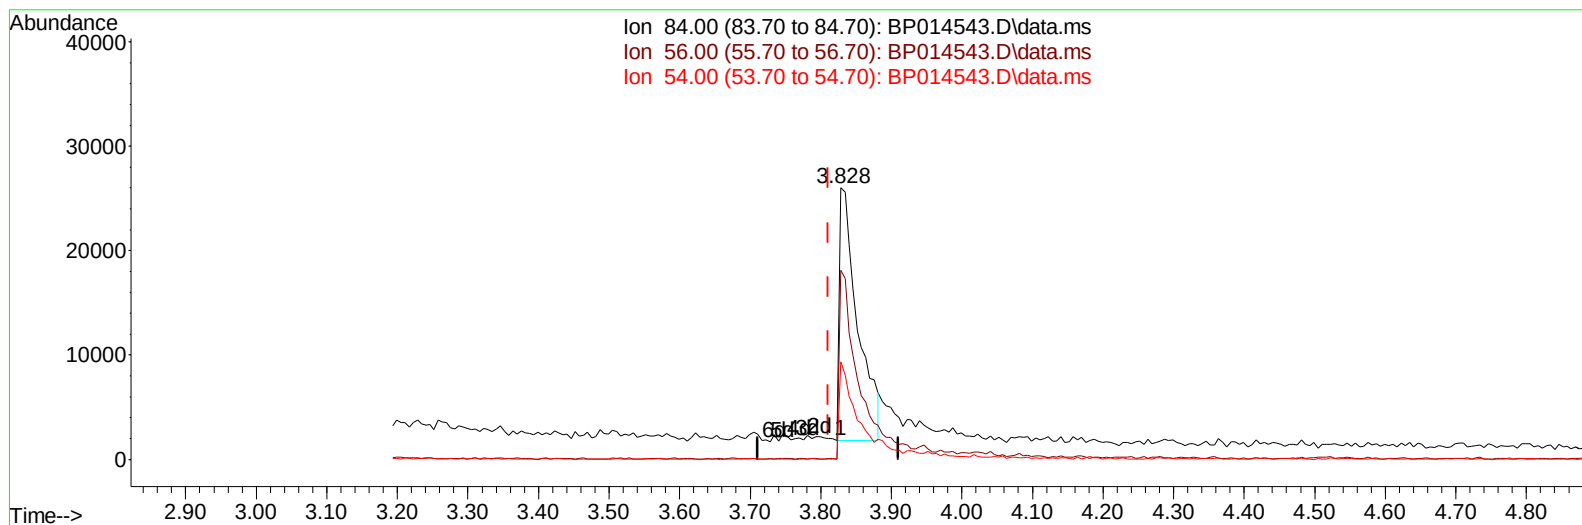

TIC: BP014543.D\data.ms

(4) Pyridine-d5 (S)

3.828min (+ 0.018) 5.78 ng/u1

response 44024

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	69.61
54.00	32.60	36.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014543.D
 Acq On : 04 Apr 2023 23:42
 Operator : CG/JU
 Sample : 02158-18RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

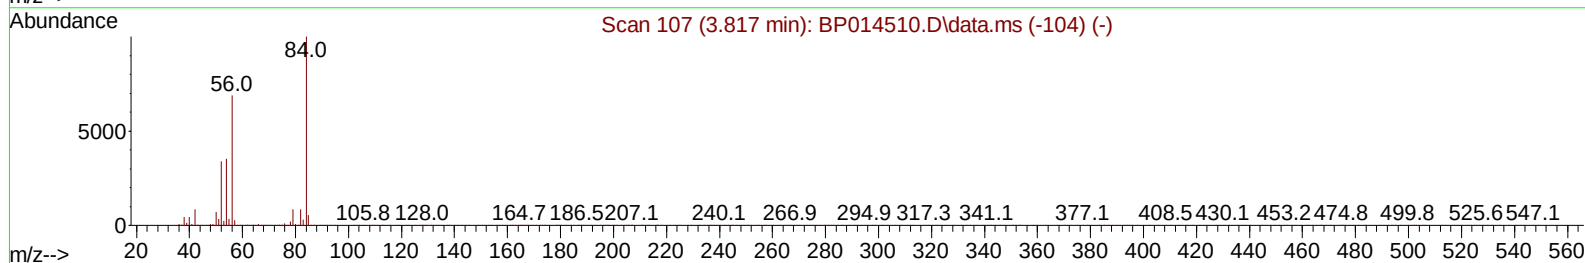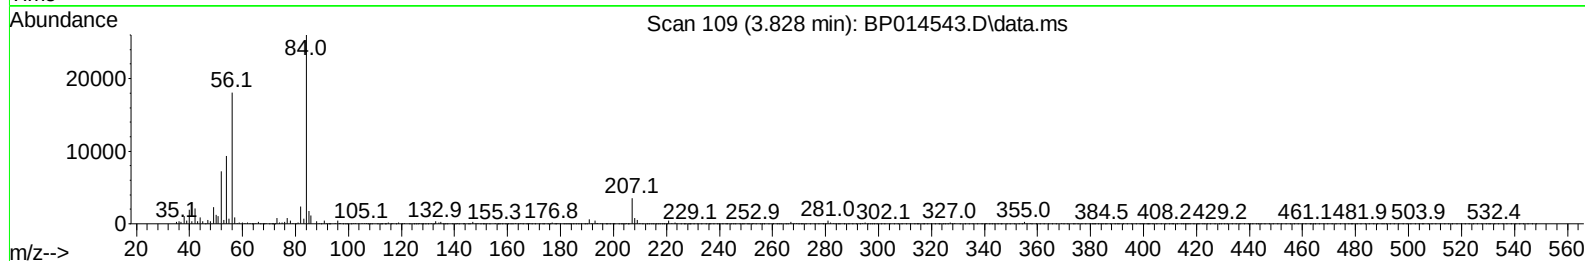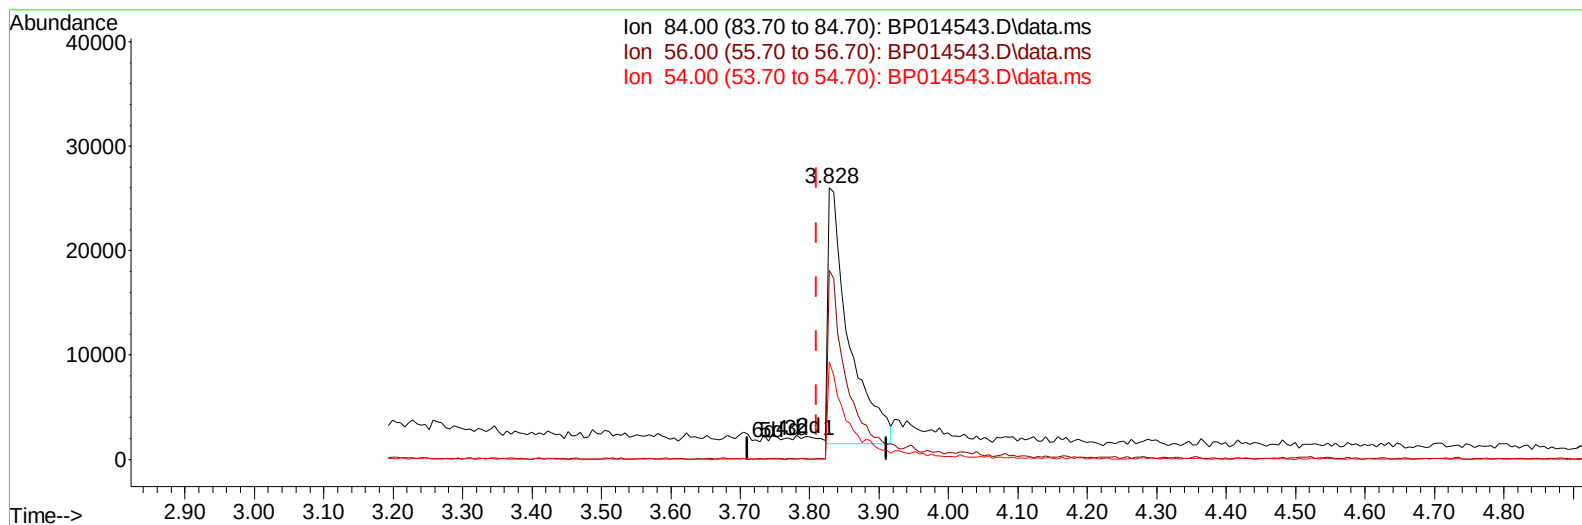

TIC: BP014543.D\data.ms

(4) Pyridine-d5 (S)

3.828min (+ 0.018) 6.78 ng/ul m

response 51617

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	69.61
54.00	32.60	36.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014543.D
Acq On : 04 Apr 2023 23:42
Operator : CG/JU
Sample : 02158-18RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

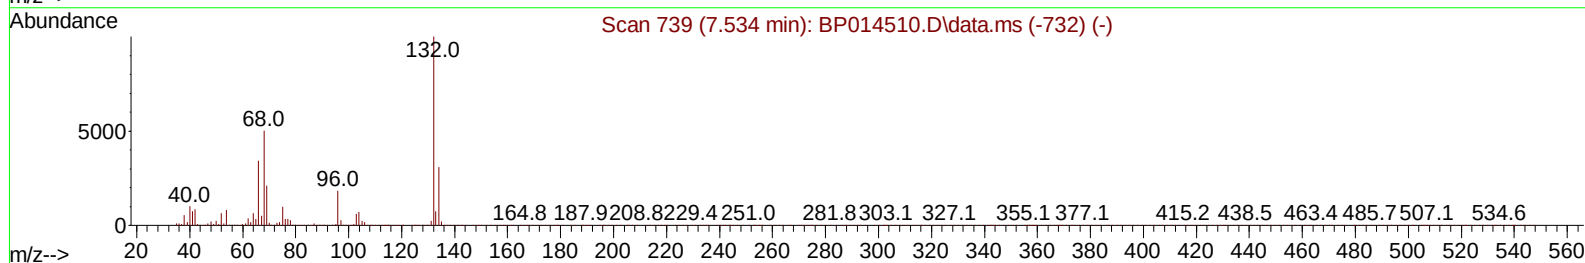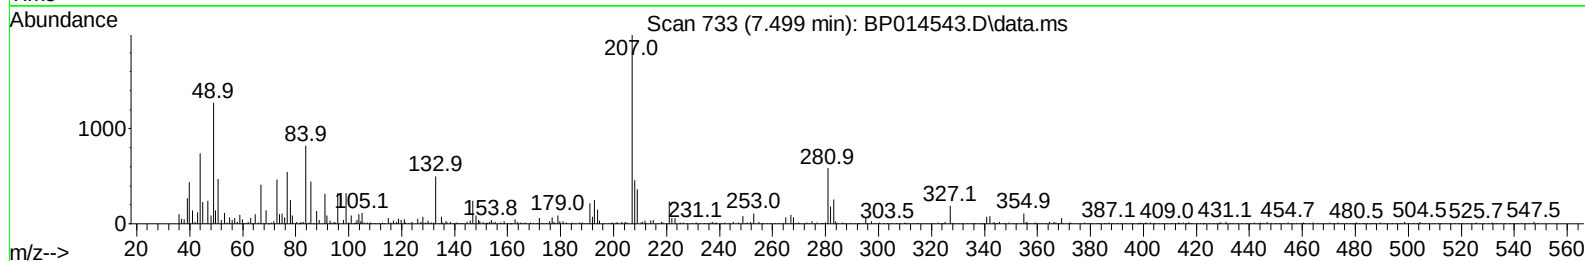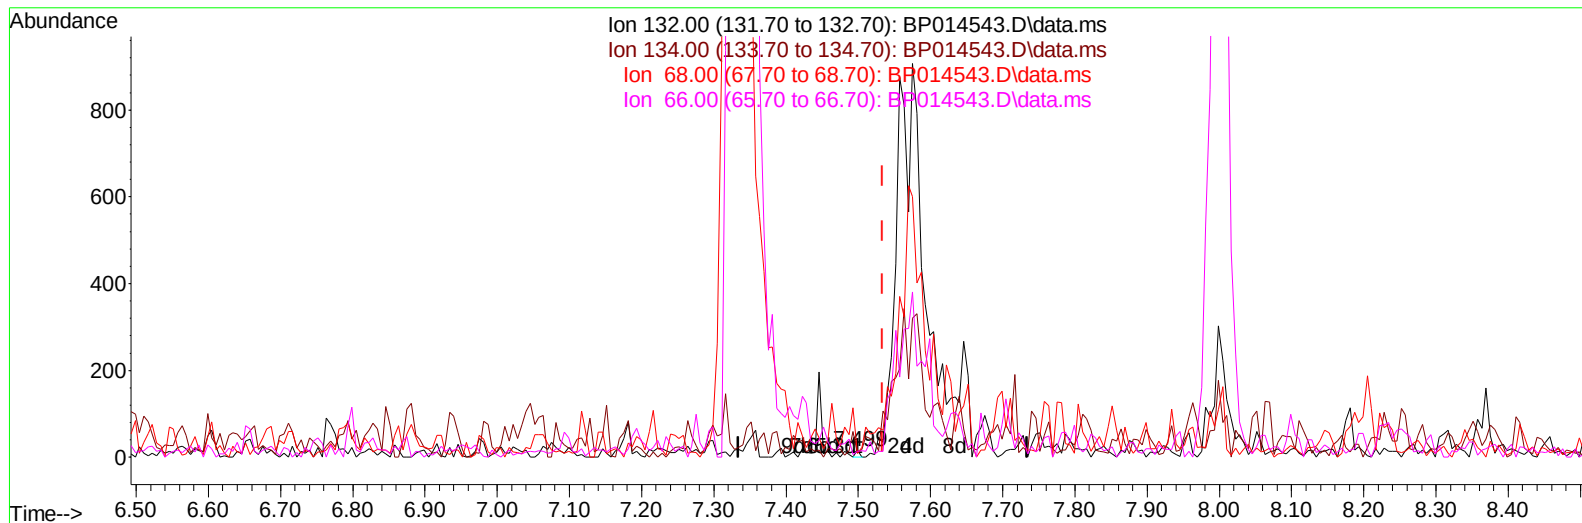

TIC: BP014543.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.499min (-0.035) 0.00 ng/u1

response 6

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.10	62.50#
68.00	50.20	62.50#
66.00	34.70	81.25#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014543.D
Acq On : 04 Apr 2023 23:42
Operator : CG/JU
Sample : 02158-18RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230328)RE

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 05 01:22:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

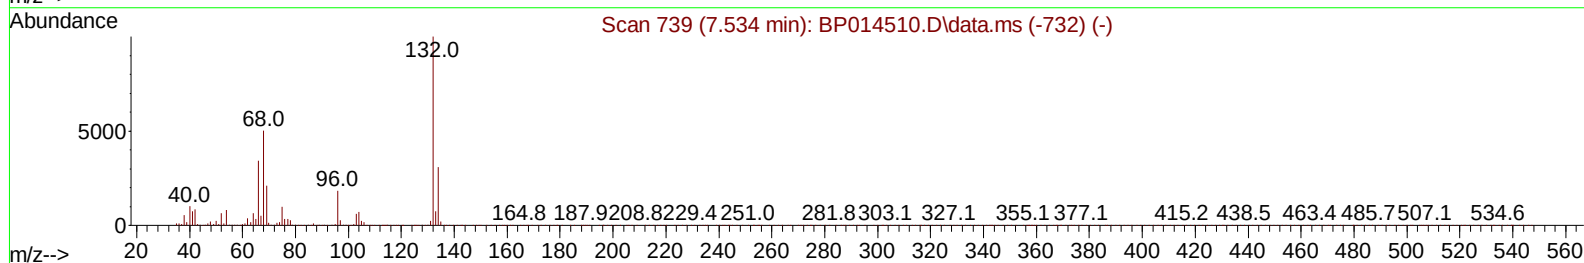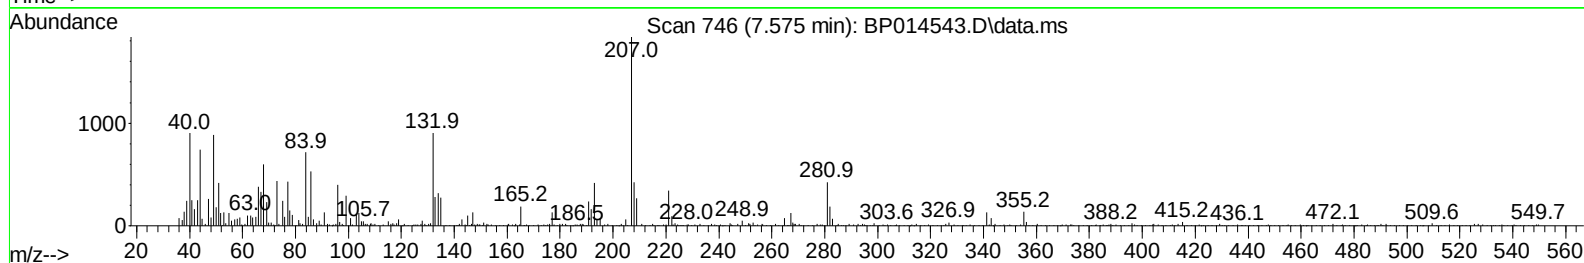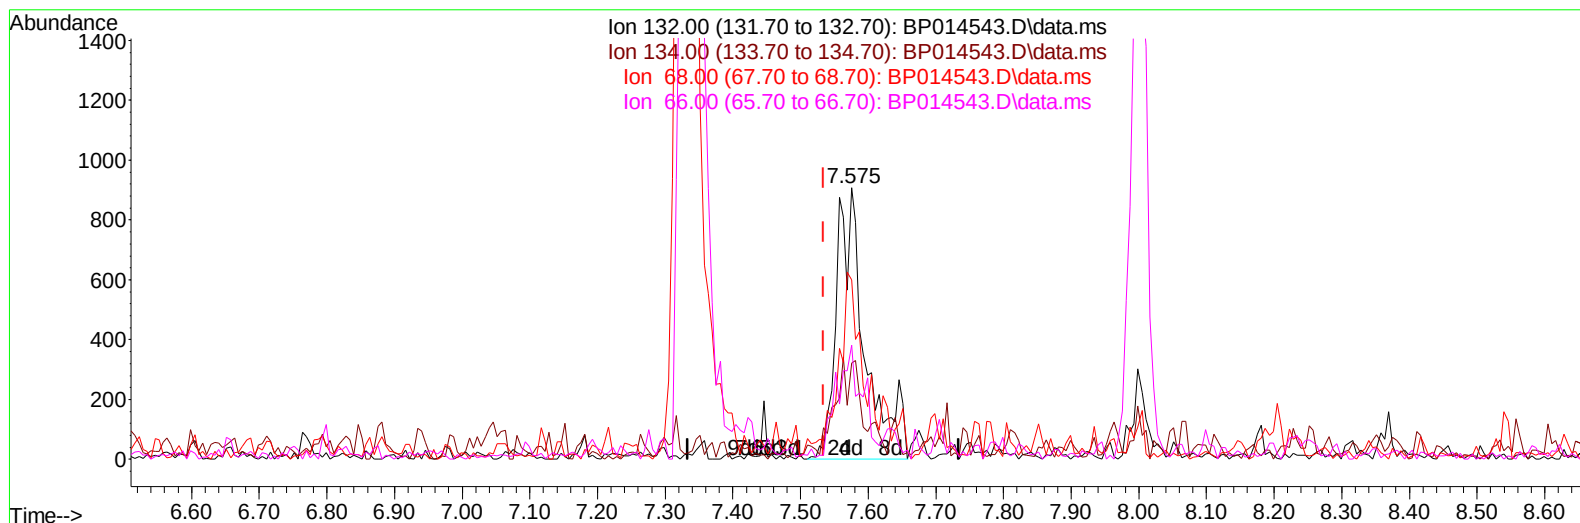

TIC: BP014543.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.575min (+ 0.041) 0.35 ng/ul m

response 2677

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.10	35.39
68.00	50.20	66.15#
66.00	34.70	42.01#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014543.D
 Acq On : 04 Apr 2023 23:42
 Operator : CG/JU
 Sample : 02158-18RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

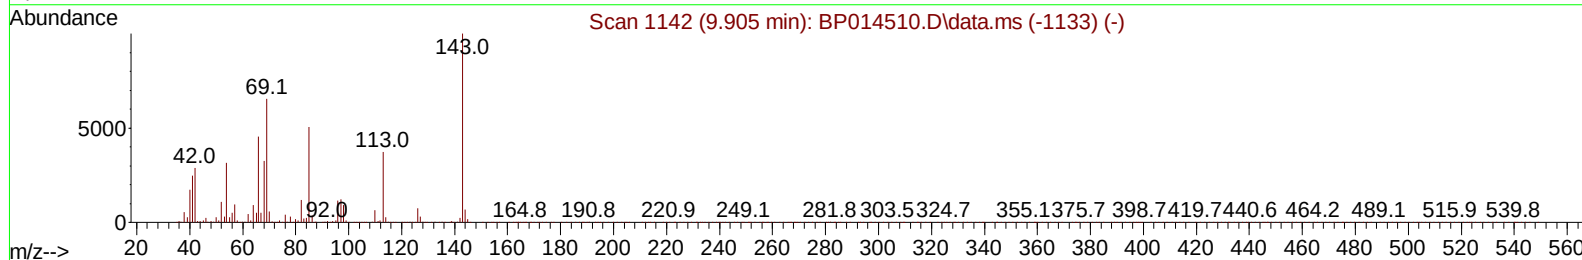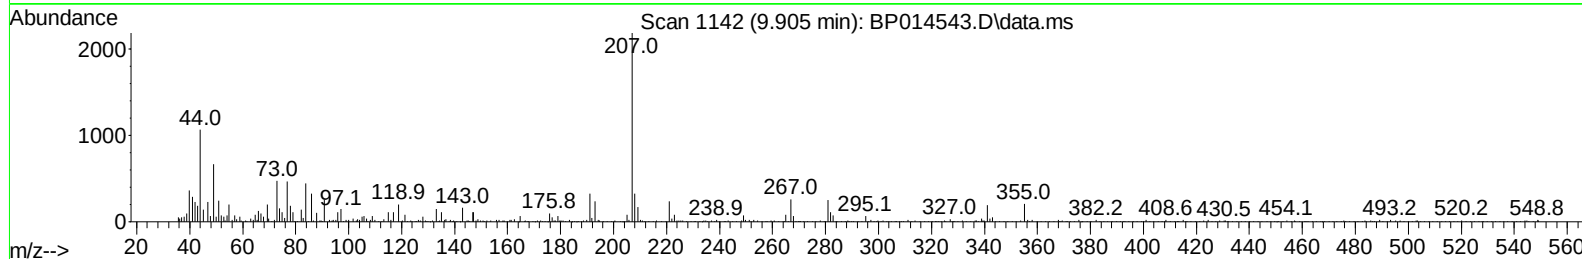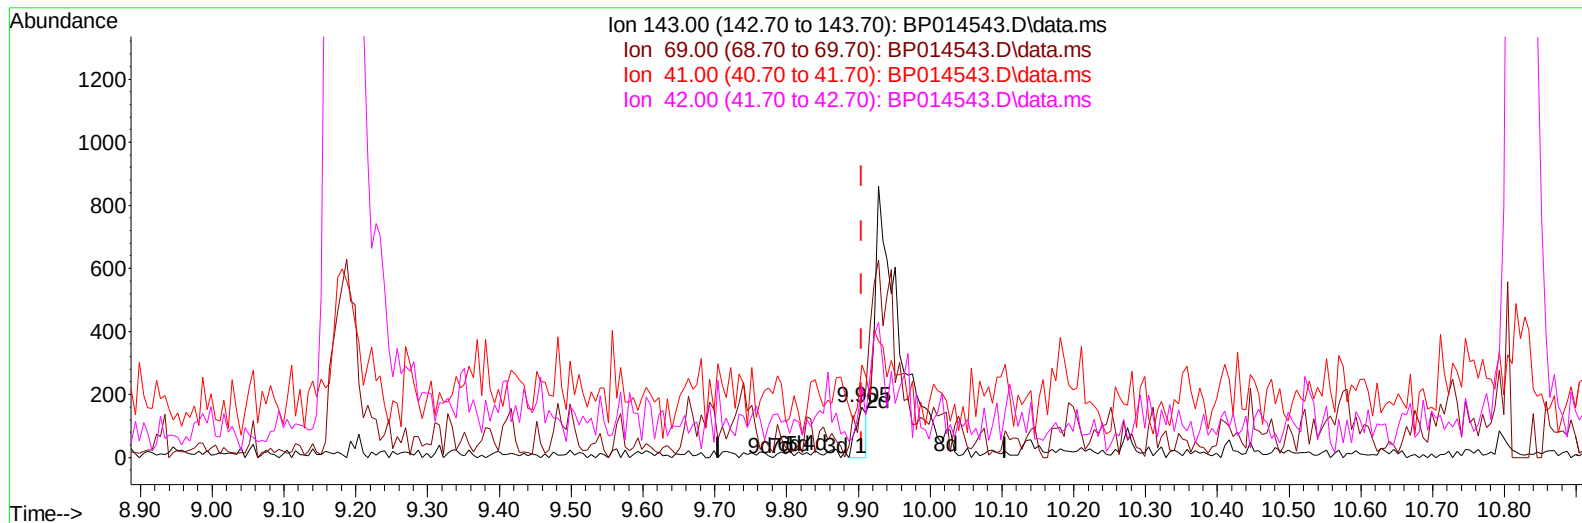

TIC: BP014543.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.905min (+ 0.000) 0.04 ng/ul

response 167

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.40	125.00#
41.00	24.10	183.12#
42.00	25.90	141.88#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014543.D
Acq On : 04 Apr 2023 23:42
Operator : CG/JU
Sample : 02158-18RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

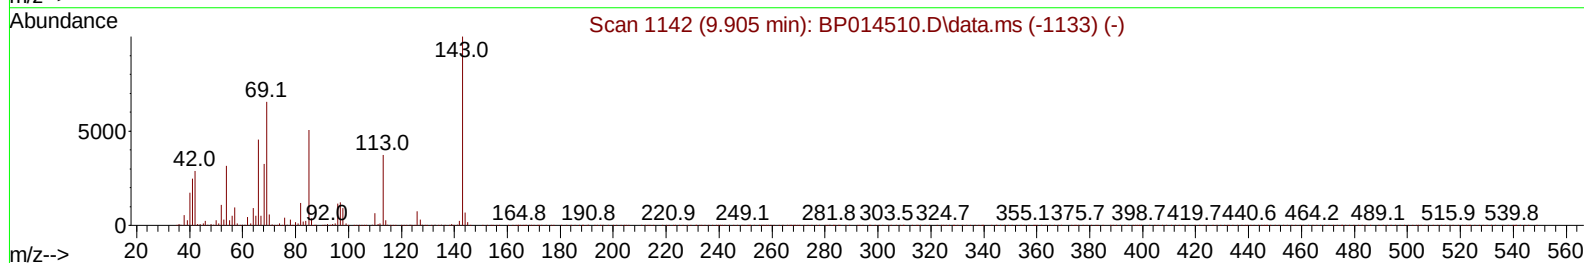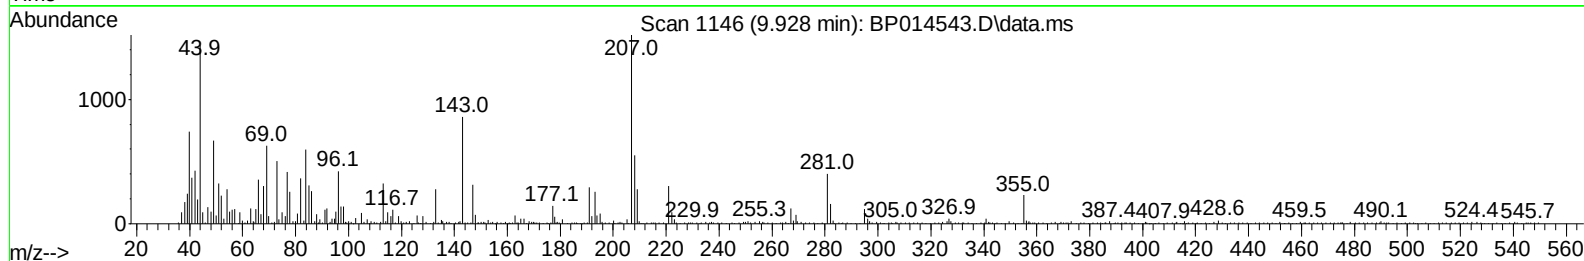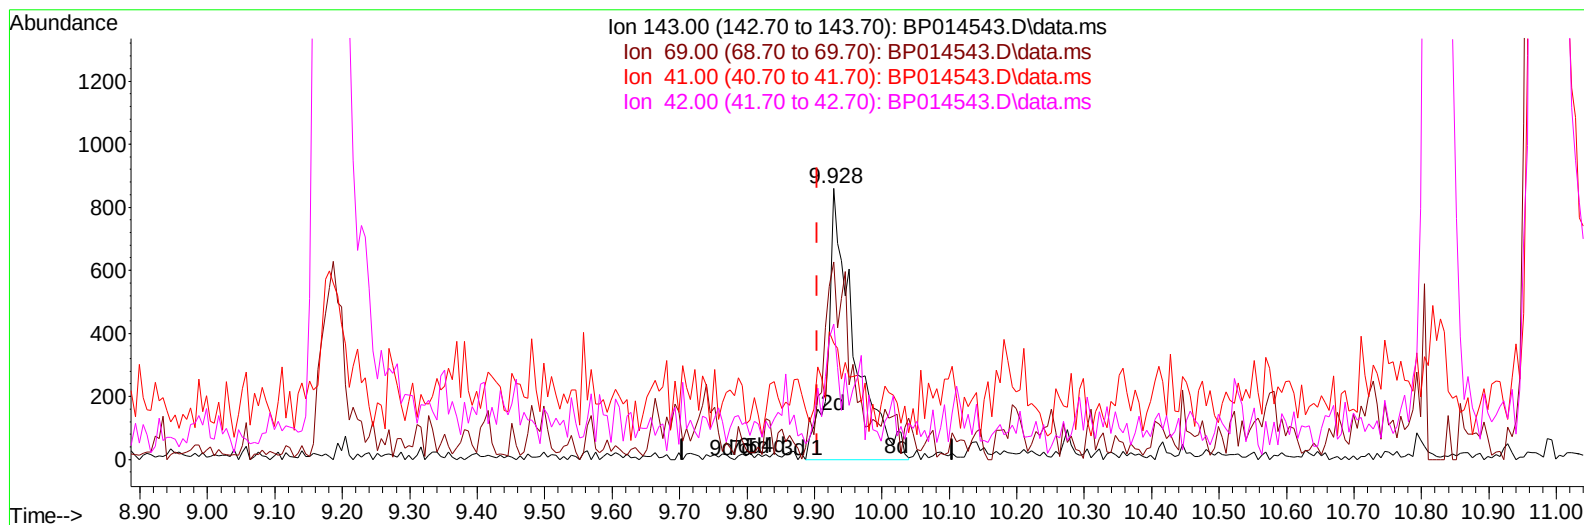

TIC: BP014543.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.928min (+ 0.024) 0.52 ng/ul m

response 2315

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.40	72.71
41.00	24.10	42.86#
42.00	25.90	49.83#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014543.D
Acq On : 04 Apr 2023 23:42
Operator : CG/JU
Sample : 02158-18RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

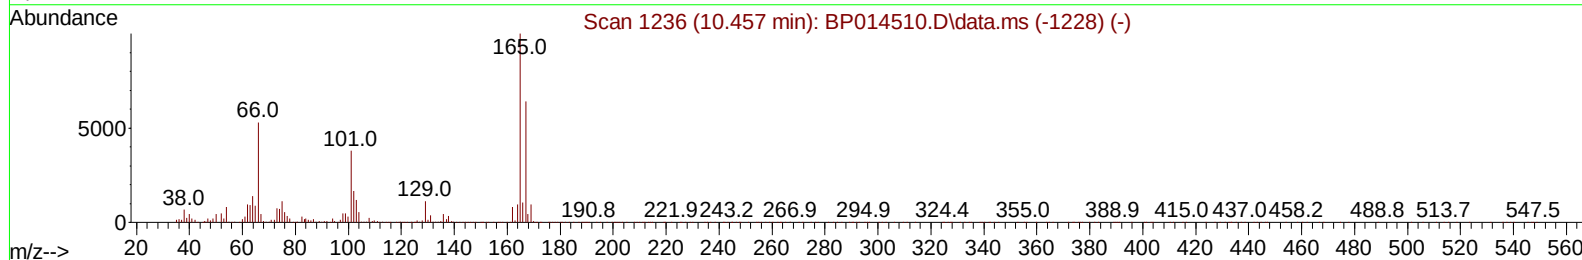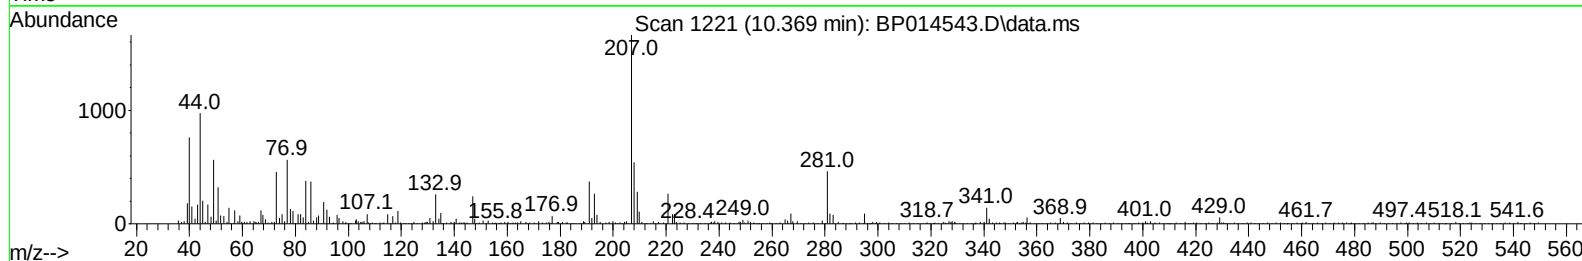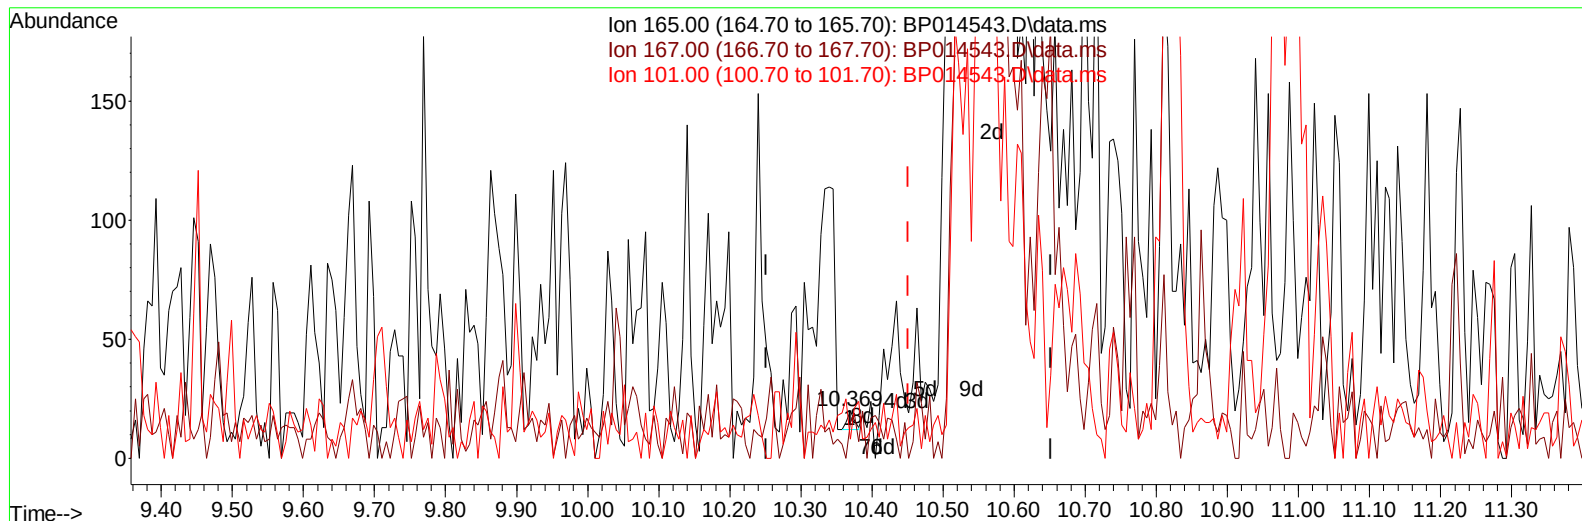

TIC: BP014543.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.369min (-0.082) 0.00 ng/ul

response 6

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	75.00
101.00	39.20	40.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014543.D
Acq On : 04 Apr 2023 23:42
Operator : CG/JU
Sample : 02158-18RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230328)RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:22:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

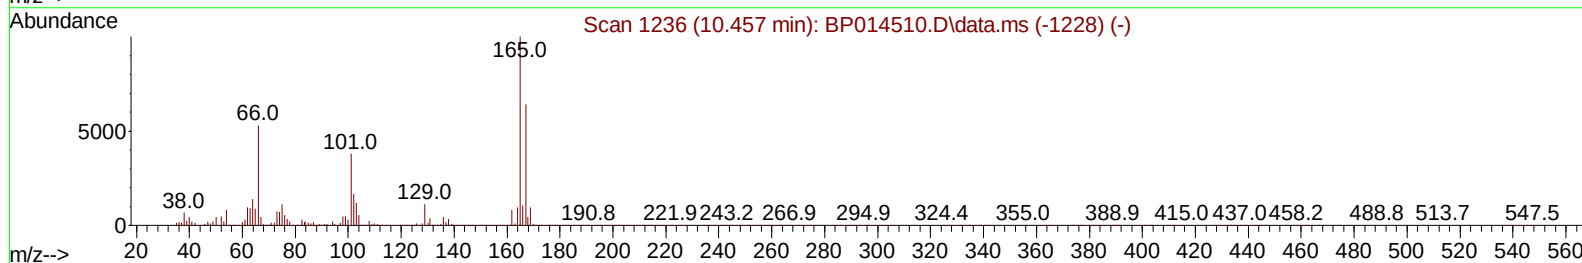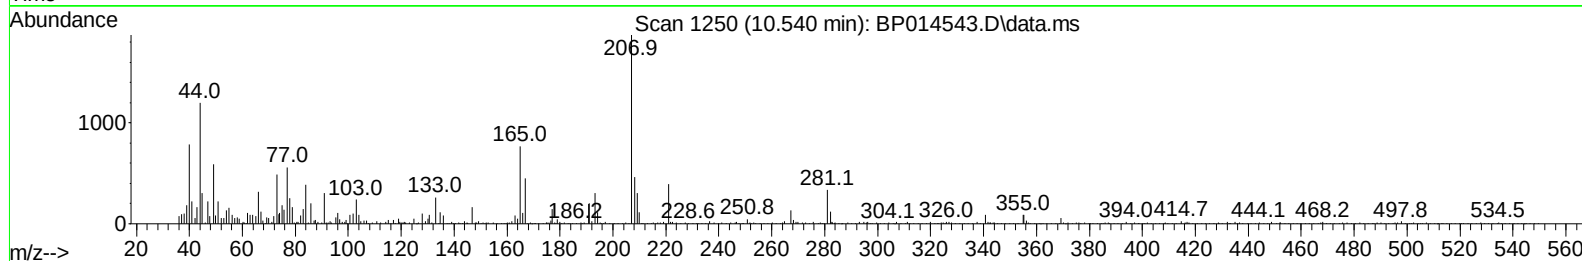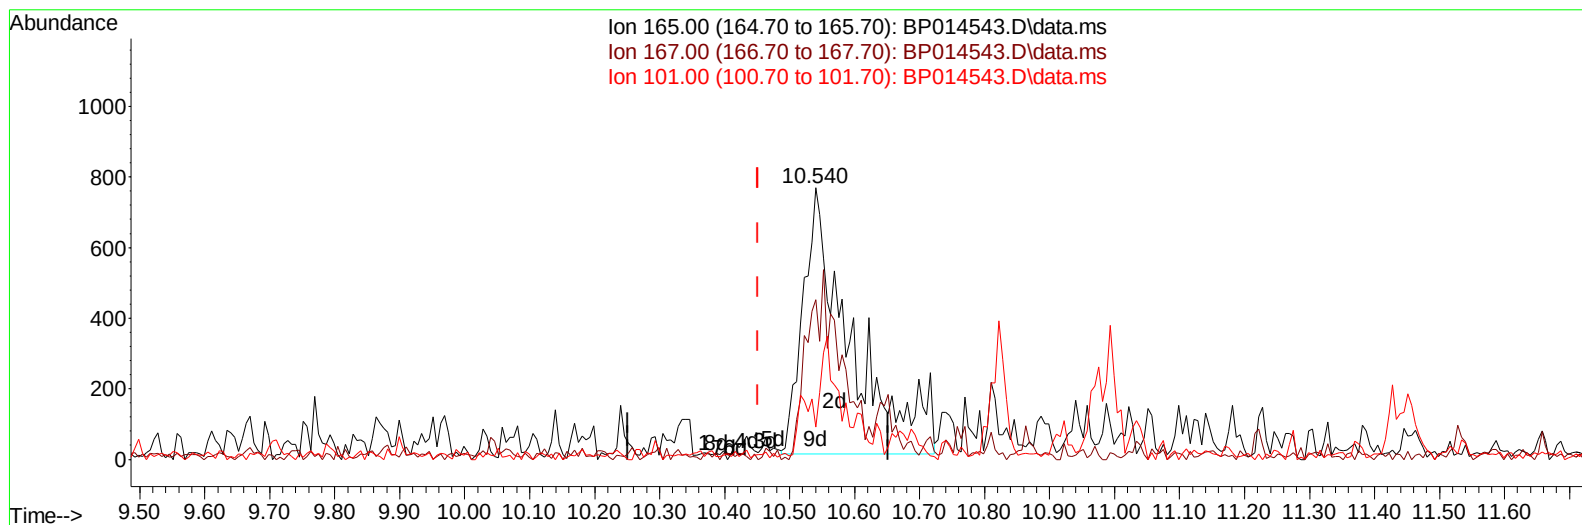

TIC: BP014543.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.540min (+ 0.088) 0.47 ng/ul m

response 3801

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	58.78
101.00	39.20	11.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014543.D
 Acq On : 04 Apr 2023 23:42
 Operator : CG/JU
 Sample : 02158-18RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230328)RE

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 05 01:22:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	115199	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	480755	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	304556	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.416	188	692378	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	749672	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	869046	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	15082	5.077	ng/uL	0.00
4) Pyridine-d5	3.828	84	51617m	6.780	ng/ul	0.02
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	7.328	67	231374	33.943	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	2677m	0.349	ng/ul	0.04
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	9.181	128	126416	32.573	ng/ul	0.00
24) 2-Nitrophenol-d4	9.928	143	2315m	0.521	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.540	165	3801m	0.470	ng/ul	0.09
31) 4-Chloroaniline-d4	10.981	131	203221	19.062	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	826322	33.463	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	911161	33.253	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.651	176	717284	34.832	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.516	188	1257596	37.531	ng/ul	0.00
81) Pyrene-d10	19.745	212	1590963	31.595	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.851	264	1746361	37.823	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014543.D
Acq On : 04 Apr 2023 23:42
Operator : CG/JU
Sample : 02158-18RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230328)RE

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 05 01:22:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

