




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014547.D
Acq On : 05 Apr 2023 02:32
Operator : CG/JU
Sample : PB151869BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 05 03:50:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 05 02:40:56 2023
Response via : Initial Calibration

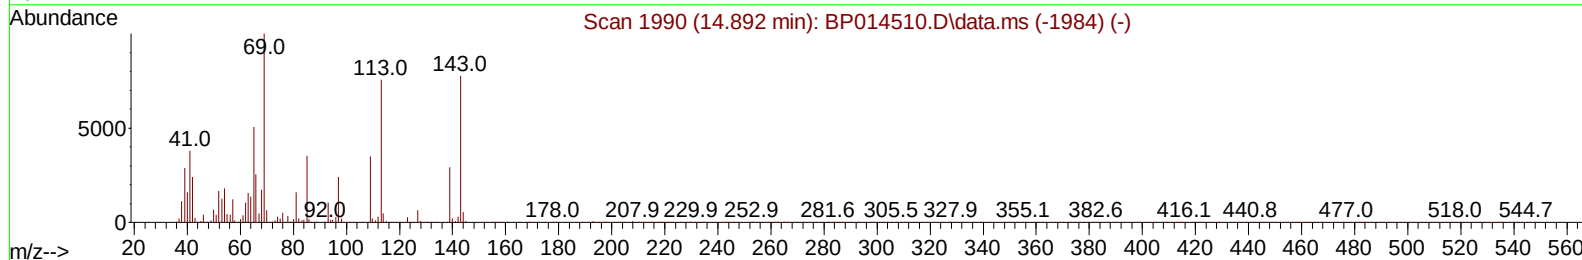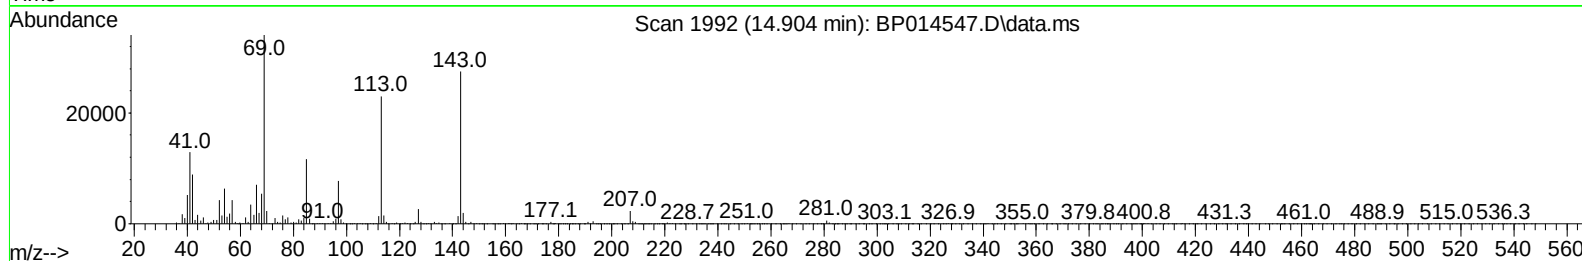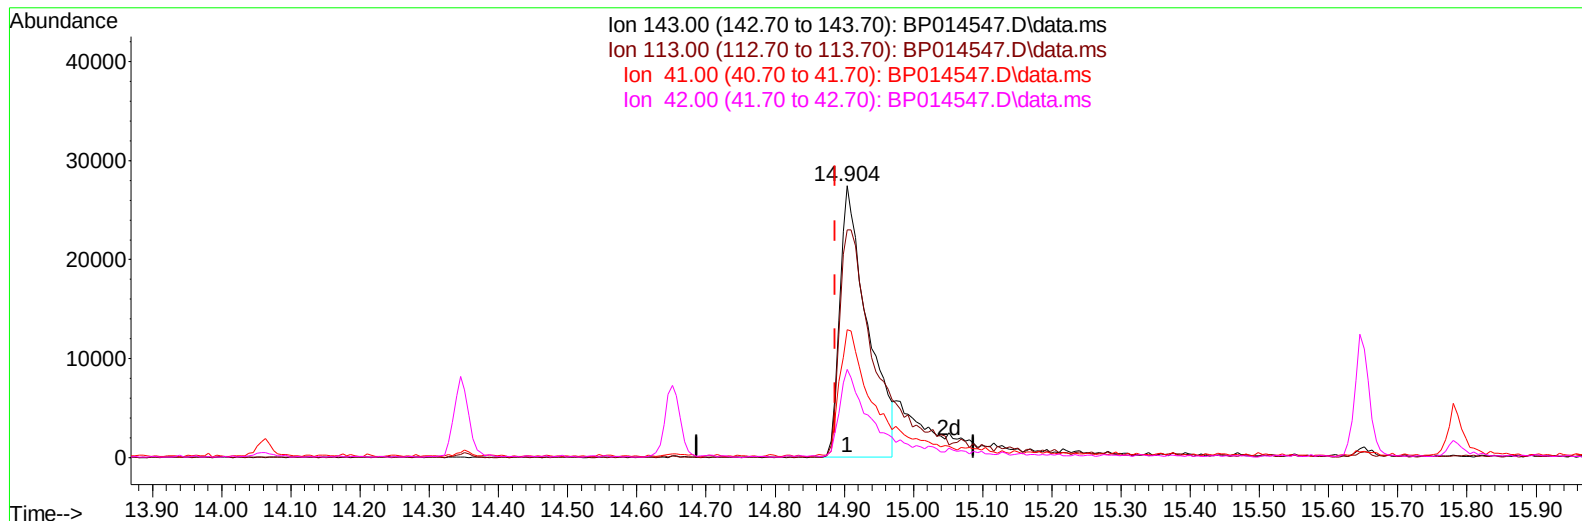

TIC: BP014547.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.904min (+ 0.017) 21.05 ng/ul

response 75604

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	83.79
41.00	44.20	47.07
42.00	31.50	32.54




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014547.D
 Acq On : 05 Apr 2023 02:32
 Operator : CG/JU
 Sample : PB151869BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK869

Manual IntegrationsAPPROVED

Quant Time: Apr 05 03:50:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 05 02:40:56 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

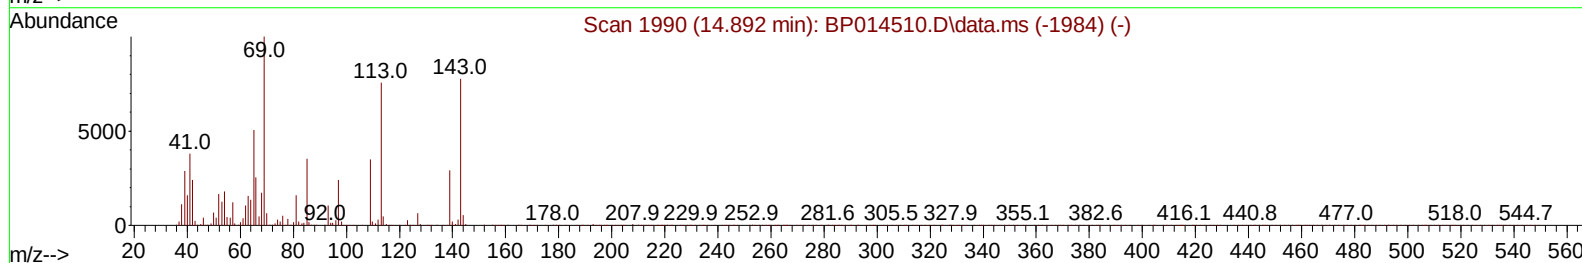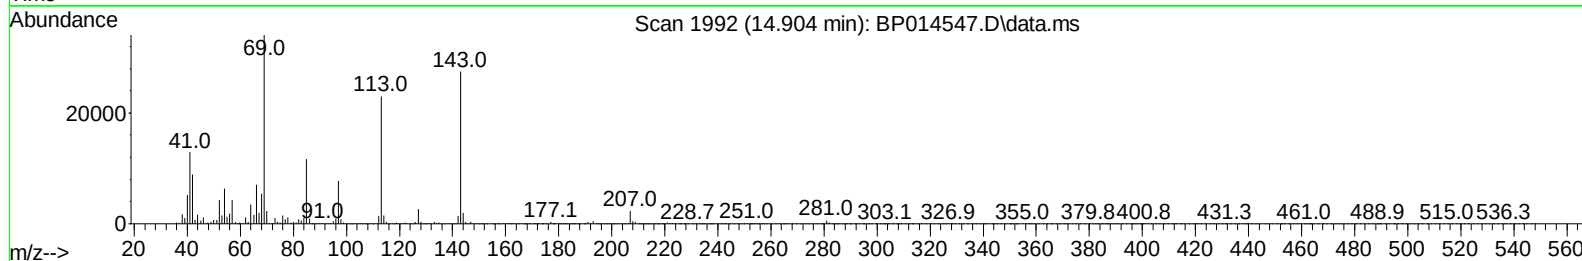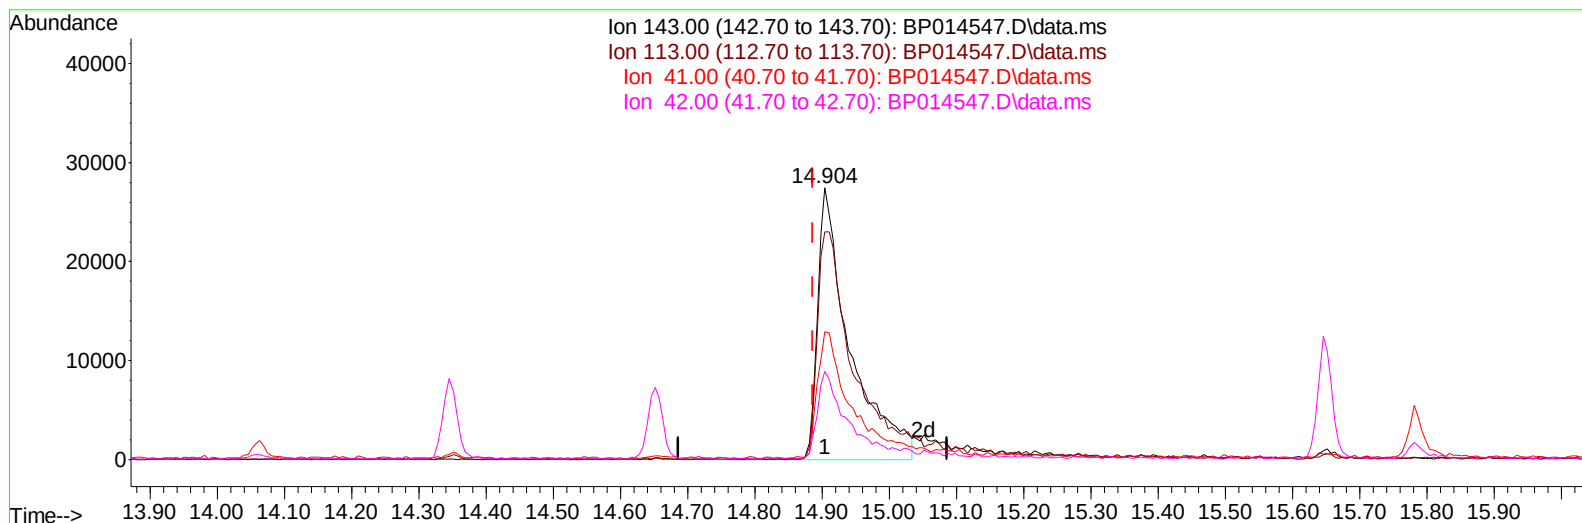

TIC: BP014547.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.904min (+ 0.017) 25.29 ng/ul m

response 90811

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	83.79
41.00	44.20	47.07
42.00	31.50	32.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014547.D
 Acq On : 05 Apr 2023 02:32
 Operator : CG/JU
 Sample : PB151869BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK869

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
 Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 05 03:50:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 05 02:40:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	115977	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	470477	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	293175	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.416	188	657460	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	706518	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	816689	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	18313	6.123	ng/uL	0.00
4) Pyridine-d5	3.811	84	230187	30.034	ng/ul	0.00
7) Phenol-d5	7.169	99	310912	29.068	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	203935	29.717	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	236843	30.637	ng/ul	0.00
15) 4-Methylphenol-d8	8.722	113	243324	28.203	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	111224	29.284	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	125654	28.892	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	210225	26.542	ng/ul	0.00
31) 4-Chloroaniline-d4	10.975	131	278158	26.662	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	678840	28.557	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	766664	29.066	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	90811m	25.287	ng/ul	0.02
60) Fluorene-d10	15.651	176	583854	29.453	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	82806	17.117	ng/ul	0.01
73) Anthracene-d10	17.516	188	975604	30.662	ng/ul	0.00
81) Pyrene-d10	19.745	212	1222243	25.755	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	1375472	31.700	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014547.D
Acq On : 05 Apr 2023 02:32
Operator : CG/JU
Sample : PB151869BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/05/2023
Supervised By :Jagrut Upadhyay 04/05/2023

Quant Time: Apr 05 03:50:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 05 02:40:56 2023
Response via : Initial Calibration

