

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014484.D
 Acq On : 03 Apr 2023 13:33
 Operator : CG/JU
 Sample : 02093-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB978DL

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/04/2023
 Supervised By : Jagrut Upadhyay 04/04/2023

Quant Time: Apr 04 00:52:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	143542	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	664345	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.663	164	457527	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.427	188	1049143	20.000	ng/u1	0.00
79) Chrysene-d12	21.515	240	899218	20.000	ng/u1	0.00
88) Perylene-d12	24.033	264	855150	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	1735	0.469	ng/uL	0.00
4) Pyridine-d5	3.869	84	14318m	1.509	ng/u1	0.05
7) Phenol-d5	7.204	99	14971	1.131	ng/u1	0.03
9) Bis-(2-Chloroethyl)eth...	7.334	67	32422	3.817	ng/u1	0.00
11) 2-Chlorophenol-d4	7.551	132	27946m	2.921	ng/u1	0.01
15) 4-Methylphenol-d8	8.745	113	22151	2.074	ng/u1	0.02
21) Nitrobenzene-d5	9.192	128	17960	3.349	ng/u1	0.00
24) 2-Nitrophenol-d4	9.922	143	17719	2.885	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	30466m	2.724	ng/u1	0.03
31) 4-Chloroaniline-d4	11.004	131	12930	0.878	ng/u1	0.02
46) Dimethylphthalate-d6	14.069	166	150996	4.070	ng/u1	0.00
49) Acenaphthylene-d8	14.357	160	157202	3.819	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	0.00
60) Fluorene-d10	15.657	176	129765	4.195	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	11696	1.515	ng/u1	0.00
73) Anthracene-d10	17.527	188	210128	4.139	ng/u1	0.00
81) Pyrene-d10	19.751	212	254485	4.213	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.868	264	189234	4.165	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.422	88	73171	17.988	ng/uL	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014484.D
Acq On : 03 Apr 2023 13:33
Operator : CG/JU
Sample : 02093-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
CB978DL

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 04/04/2023
Supervised By : Jagrut Upadhyay 04/04/2023


Quant Time: Apr 04 00:52:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

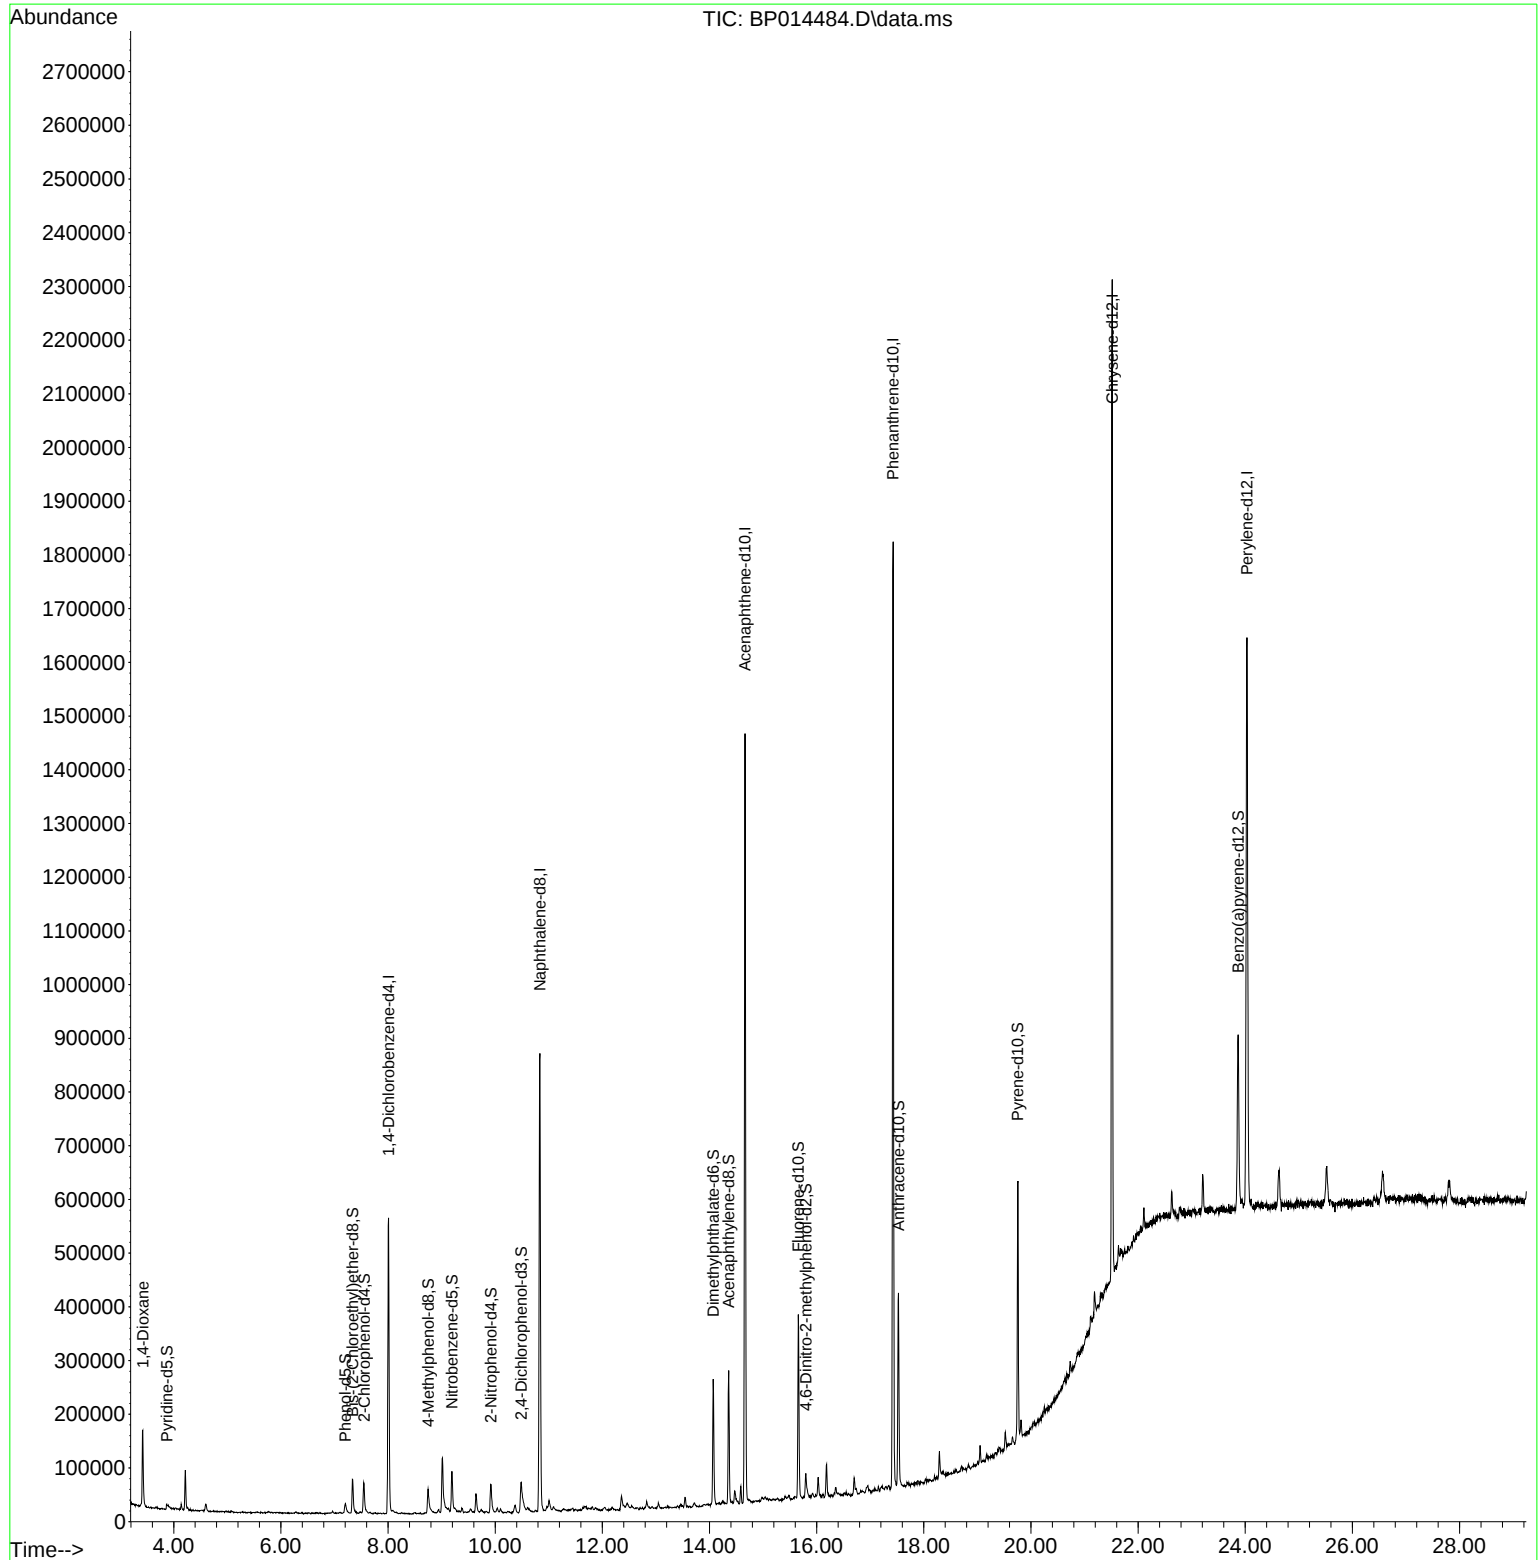

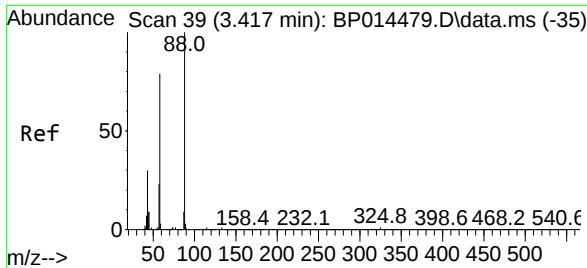

#2
 1,4-Dioxane
 Concen: 17.988 ng/uL
 RT: 3.422 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: BP014484.D
 Acq: 03 Apr 2023 13:33

Instrument :
 BNA_P
 ClientSampleId :
 CB978DL

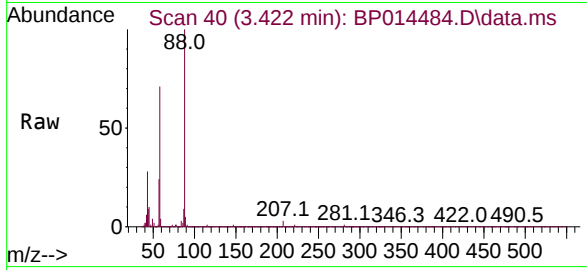

Tgt Ion:	88	Resp:	7317
Ion	Ratio	Lower	Upper
88	100		
43	28.4	24.4	36.6
58	71.4	57.4	86.0

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 04/04/2023
 Supervised By :Jagrut Upadhyay 04/04/2023

